

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070721\
 Data File : FF008744.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jul 2021 14:59
 Operator : DD\AJ
 Sample : M2935-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 08 01:48:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	1418101	12.443 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.943	89484	0.679 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070721\
Data File : FF008744.D
Signal(s) : FID2B.ch
Acq On : 07 Jul 2021 14:59
Operator : DD\AJ
Sample : M2935-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 08 01:48:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

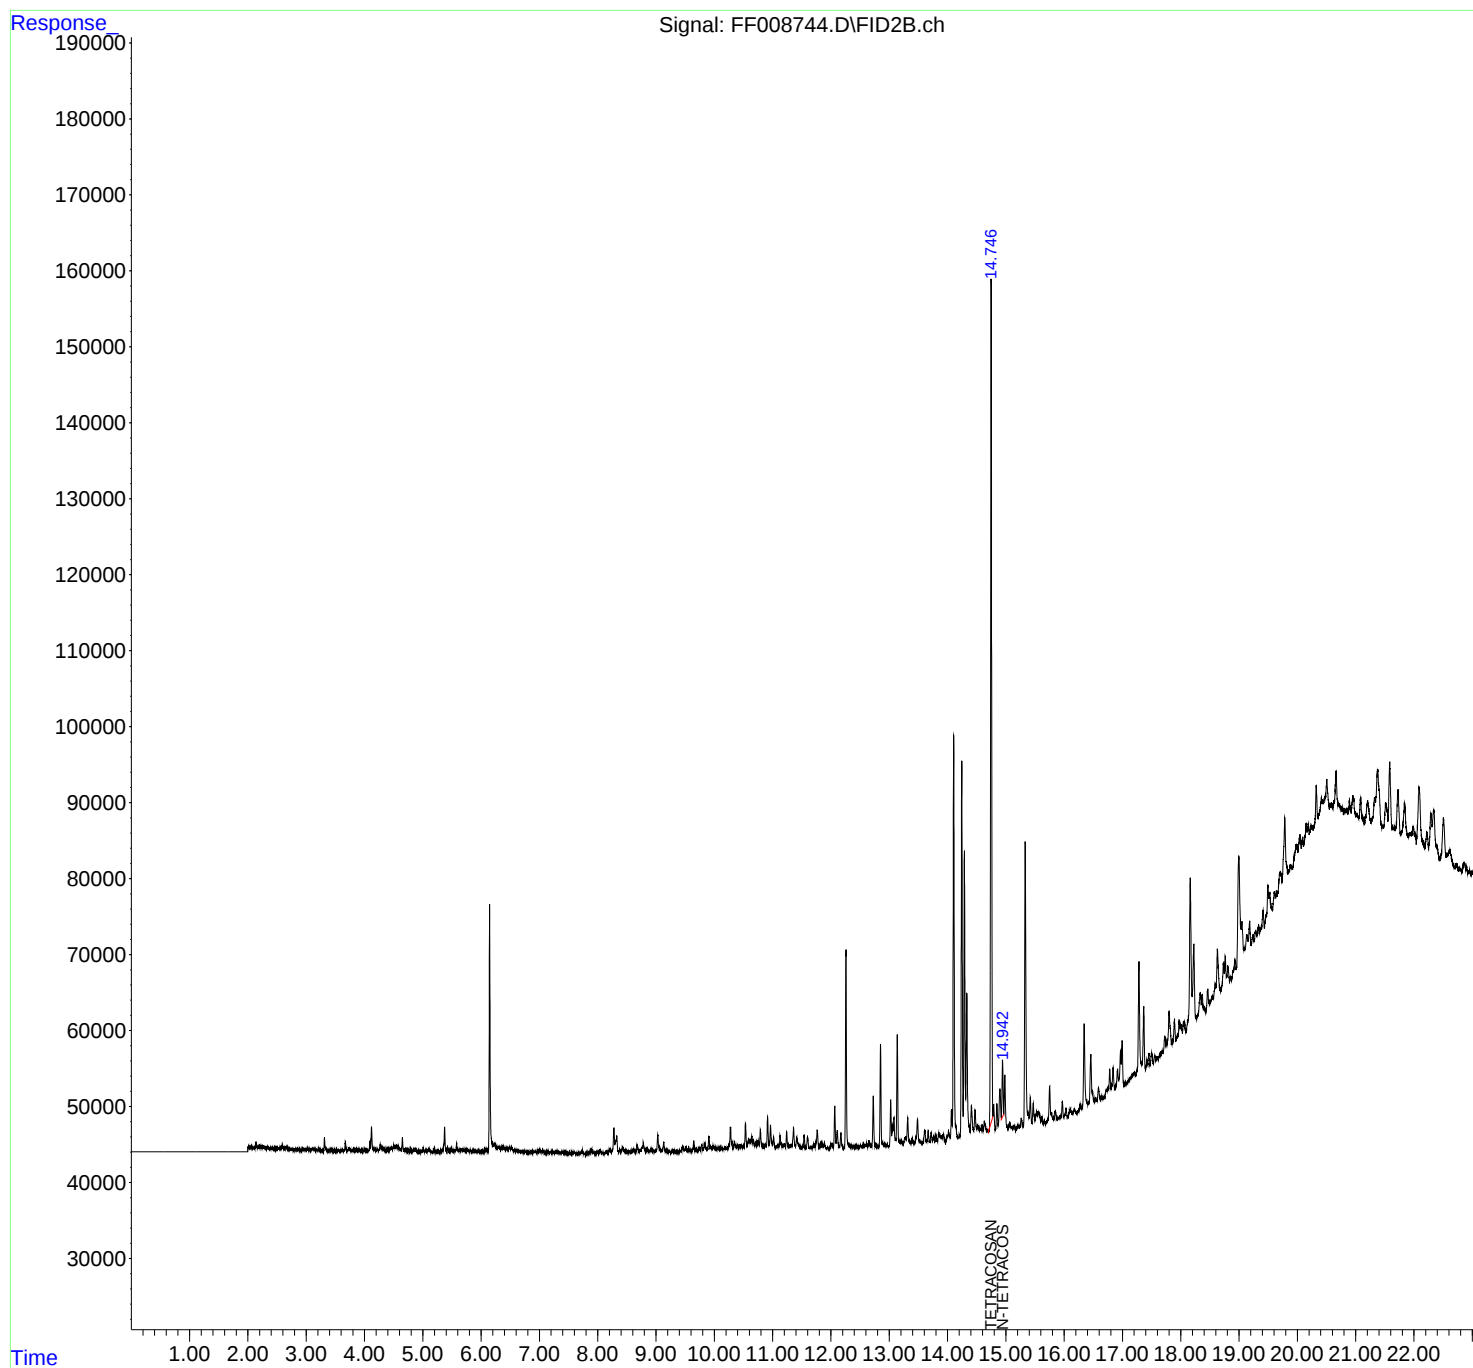


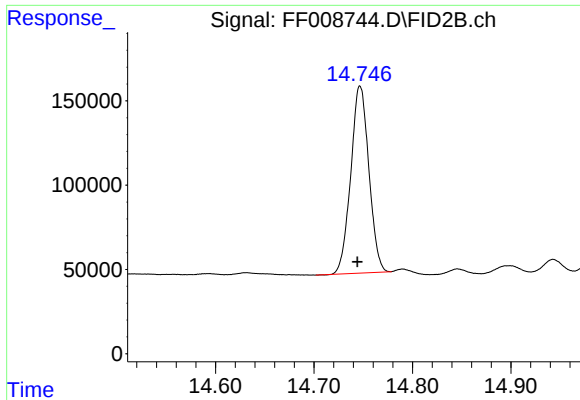

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.747 min
Delta R.T.: 0.003 min
Response: 1418101
Conc: 12.44 ug/ml

Instrument :
FID_F
ClientSampleId :

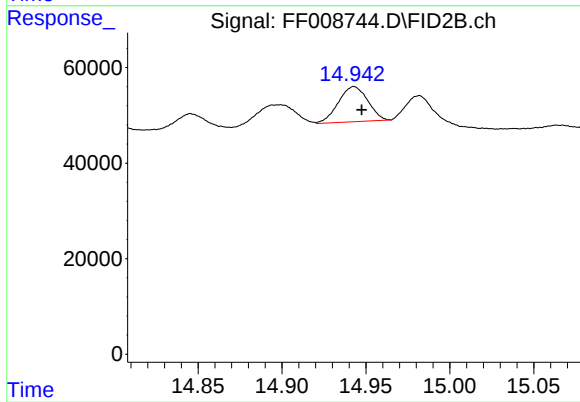

#10 N-TETRACOSANE

R.T.: 14.943 min
Delta R.T.: -0.005 min
Response: 89484
Conc: 0.68 ug/ml