

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070722\
Data File : FF011022.D
Signal(s) : FID2B.ch
Acq On : 07 Jul 2022 12:30
Operator : AJ\MA
Sample : PB145928BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 08 03:14:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.809	1920726	20.475 ug/ml

Target Compounds


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070722\
Data File : FF011022.D
Signal(s) : FID2B.ch
Acq On : 07 Jul 2022 12:30
Operator : AJ\MA
Sample : PB145928BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 08 03:14:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

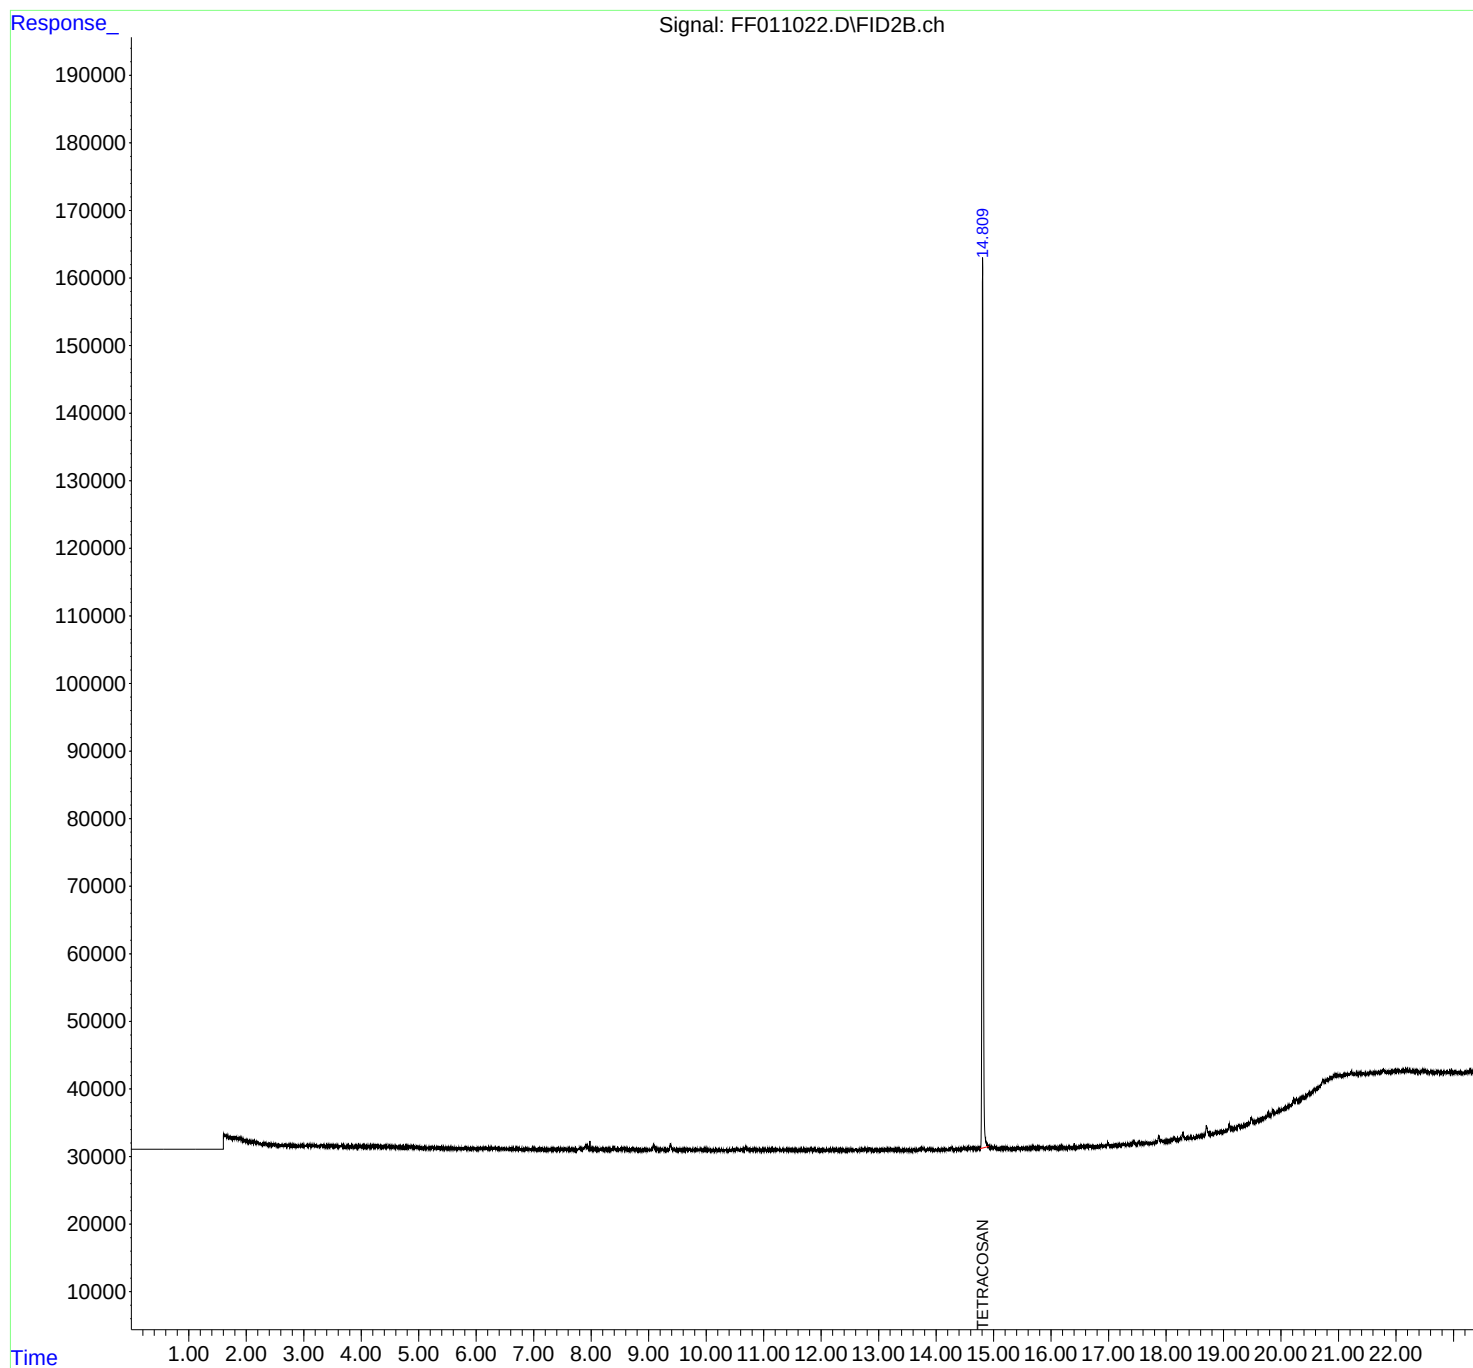

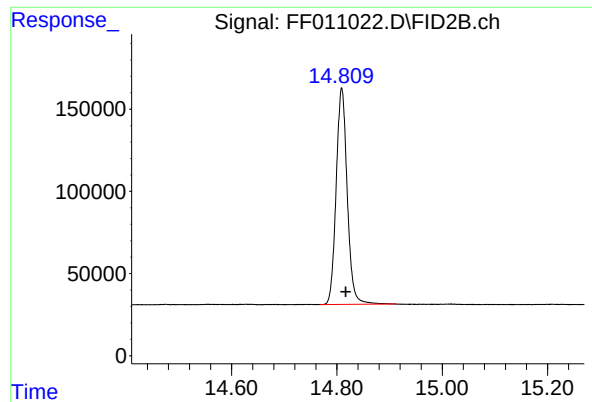

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.809 min
Delta R.T.: -0.008 min
Response: 1920726
Conc: 20.47 ug/ml