

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070819\
 Data File : FF004994.D
 Signal(s) : FID2B.ch
 Acq On : 08 Jul 2019 15:43
 Operator : DD\AJ
 Sample : K3624-03 2X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 09 00:49:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.688	772862	7.946 ug/ml
Target Compounds			
4) N-TETRADECANE	8.275f	213253	1.704 ug/ml
7) N-EICOSANE	12.640f	813686	7.013 ug/ml
8) N-DOCOSANE	13.809	150168	1.335 ug/ml
10) N-TETRACOSANE	14.870	631408	5.672 ug/ml
11) N-HEXACOSANE	15.920	117567	1.063 ug/ml
12) N-OCTACOSANE	16.879	361161	3.238 ug/ml
13) N-TRIACONTANE	17.768	509089	4.532 ug/ml
14) N-DOTRIACONTANE	18.607	211798	1.860 ug/ml
15) N-TETRATRIACONTANE	19.429	34632	0.319 ug/ml
16) N-HEXATRIACONTANE	20.117	59590	0.575 ug/ml
17) N-OCTATRIACONTANE	20.862	39888	0.418 ug/ml
18) N-TETRACONTANE	21.835	169265	1.456 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070819\
Data File : FF004994.D
Signal(s) : FID2B.ch
Acq On : 08 Jul 2019 15:43
Operator : DD\AJ
Sample : K3624-03 2X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 09 00:49:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

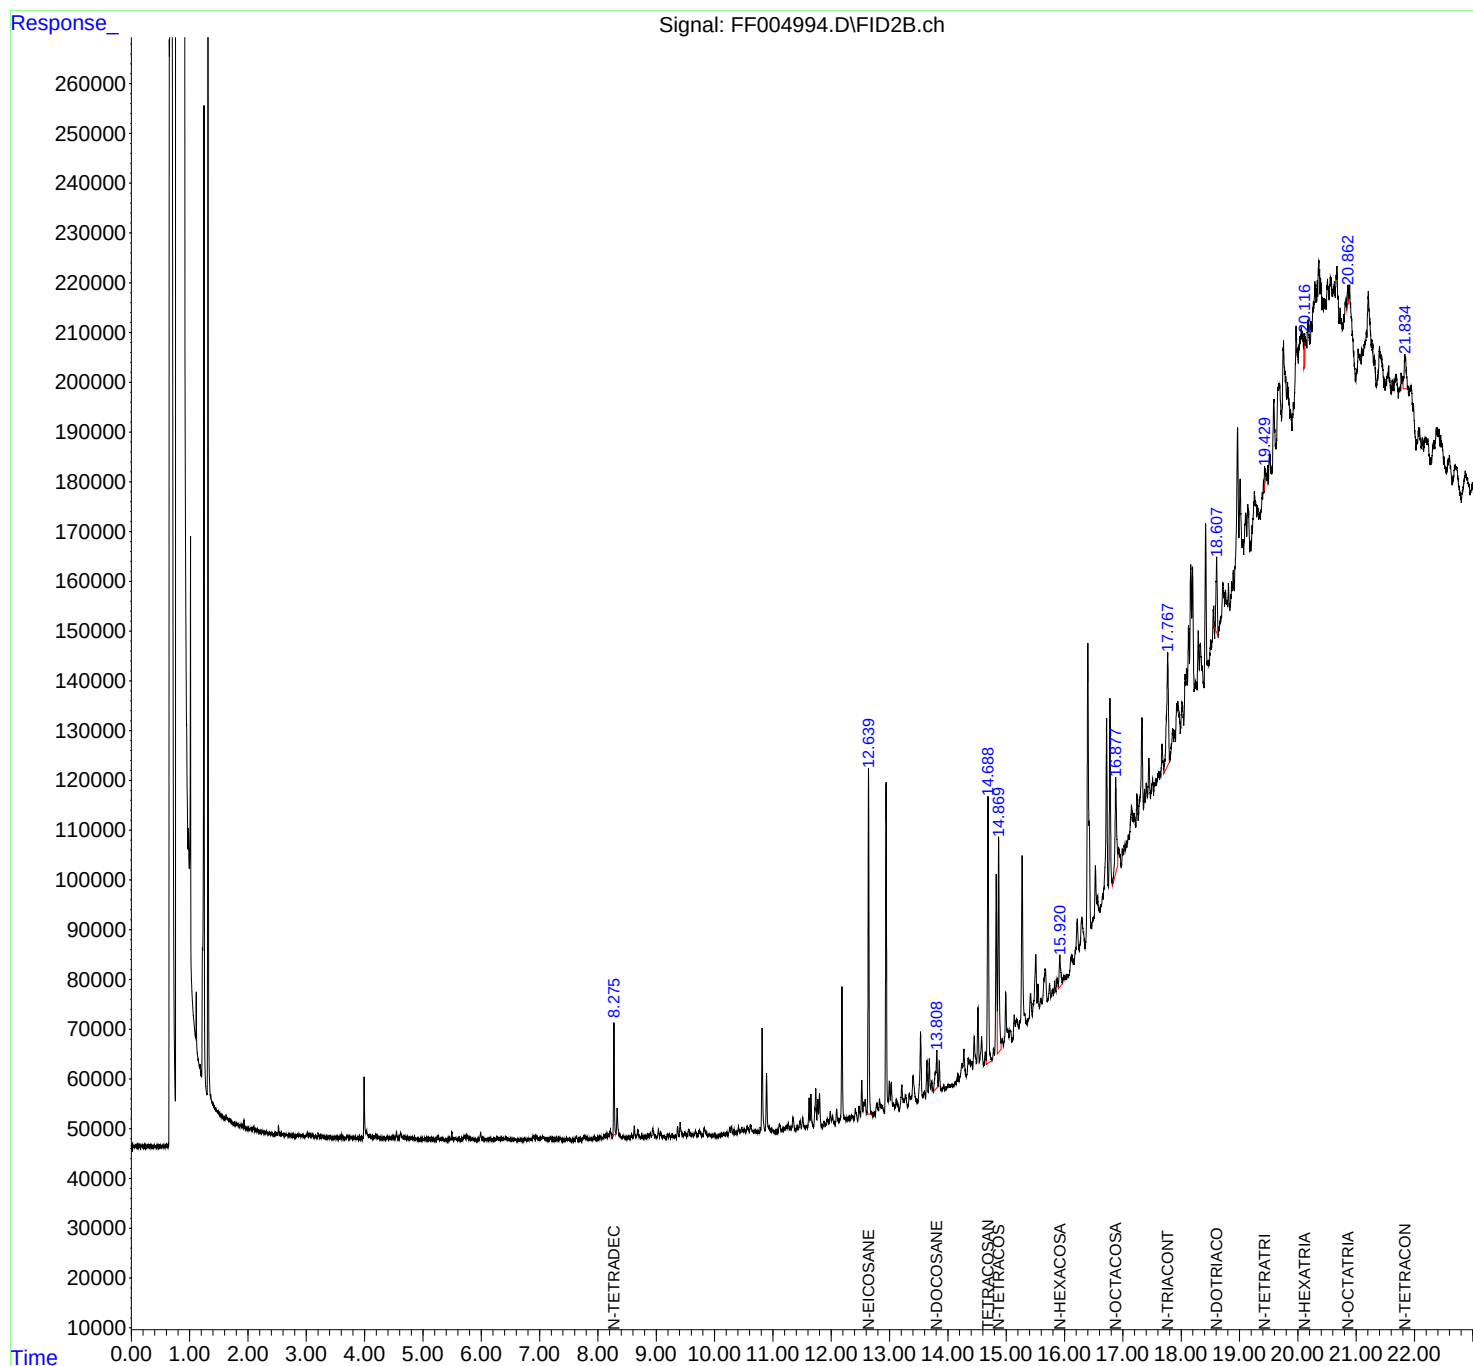

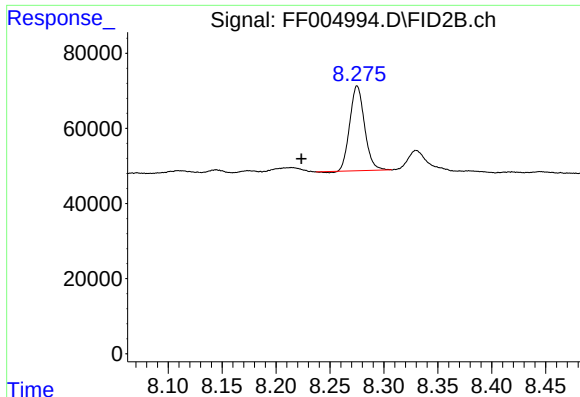


#4 N-TETRADECANE

R.T.: 8.275 min
Delta R.T.: 0.052 min
Response: 213253
Conc: 1.70 ug/ml

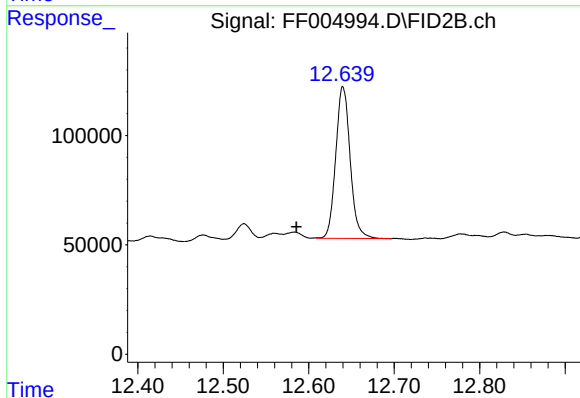


#7 N-EICOSANE

R.T.: 12.640 min
Delta R.T.: 0.055 min
Response: 813686
Conc: 7.01 ug/ml

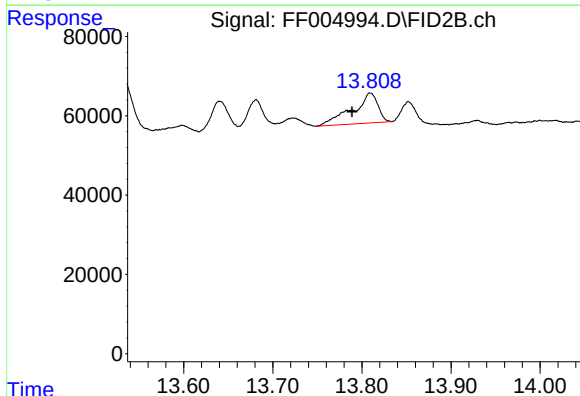


#8 N-DOCOSANE

R.T.: 13.809 min
Delta R.T.: 0.021 min
Response: 150168
Conc: 1.33 ug/ml

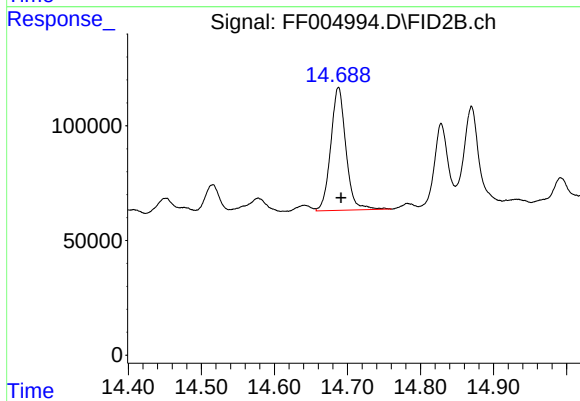


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.688 min
Delta R.T.: -0.004 min
Response: 772862
Conc: 7.95 ug/ml

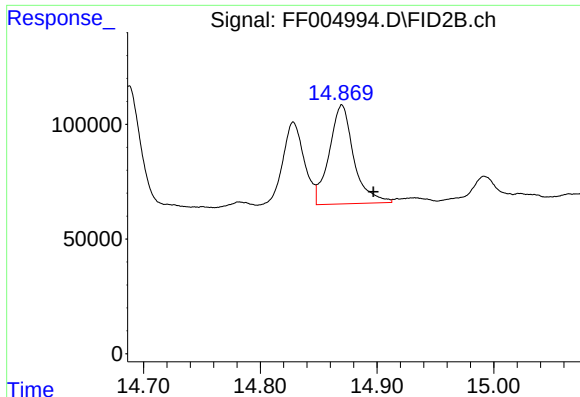


#10 N-TETRACOSANE

R.T.: 14.870 min
Delta R.T.: -0.027 min
Response: 631408
Conc: 5.67 ug/ml

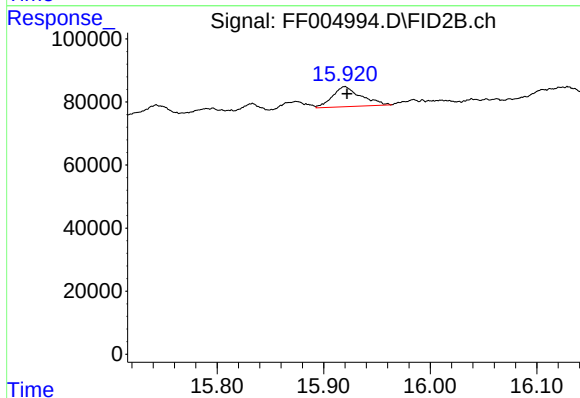


#11 N-HEXACOSANE

R.T.: 15.920 min
Delta R.T.: -0.002 min
Response: 117567
Conc: 1.06 ug/ml

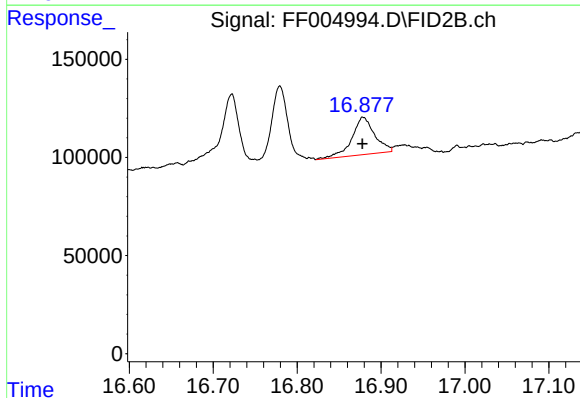


#12 N-OCTACOSANE

R.T.: 16.879 min
Delta R.T.: 0.000 min
Response: 361161
Conc: 3.24 ug/ml

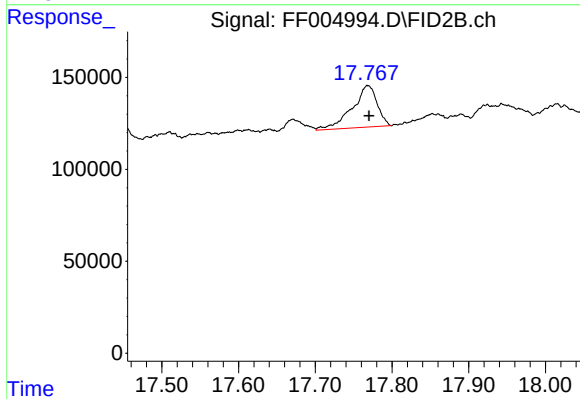


#13 N-TRIACONTANE

R.T.: 17.768 min
Delta R.T.: -0.001 min
Response: 509089
Conc: 4.53 ug/ml

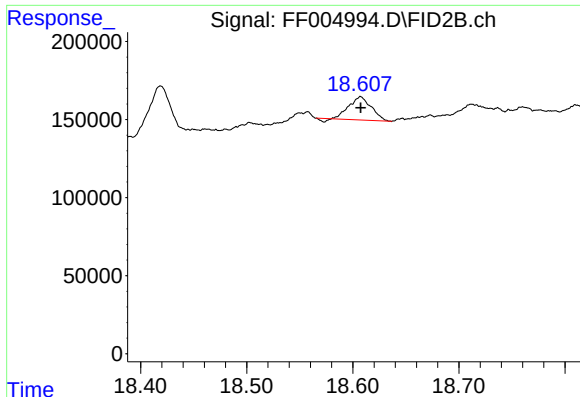


#14 N-DOTRIACONTANE

R.T.: 18.607 min
Delta R.T.: 0.000 min
Response: 211798
Conc: 1.86 ug/ml

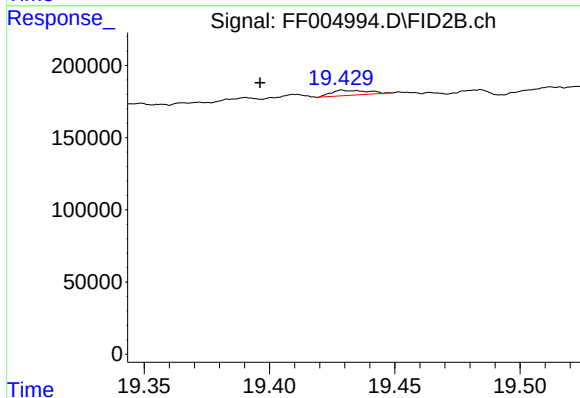


#15 N-TETRATRIACONTANE

R.T.: 19.429 min
Delta R.T.: 0.033 min
Response: 34632
Conc: 0.32 ug/ml

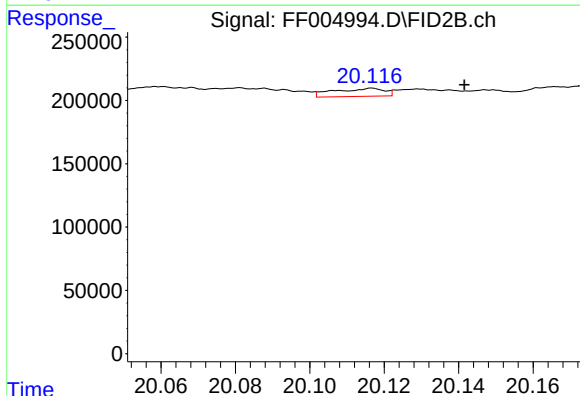


#16 N-HEXATRIACONTANE

R.T.: 20.117 min
Delta R.T.: -0.025 min
Response: 59590
Conc: 0.58 ug/ml

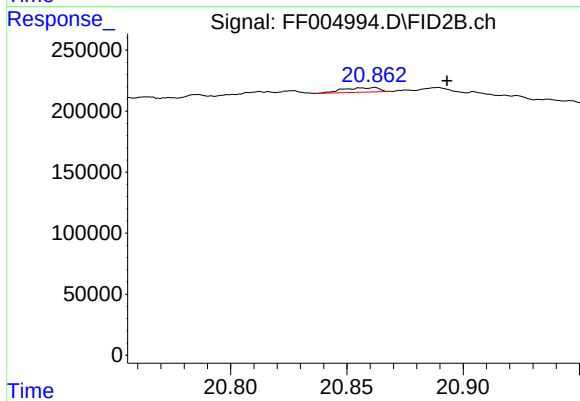

#17 N-OCTATRIACONTANE

R.T.: 20.862 min
Delta R.T.: -0.031 min
Response: 39888
Conc: 0.42 ug/ml

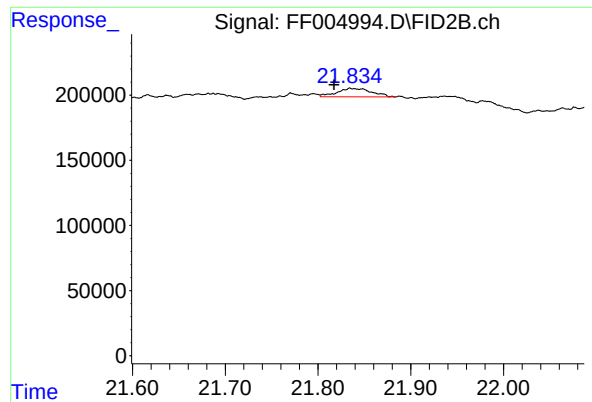

#18 N-TETRACONTANE

R.T.: 21.835 min
Delta R.T.: 0.017 min
Response: 169265
Conc: 1.46 ug/ml