

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070819\
 Data File : FF004990.D
 Signal(s) : FID2B.ch
 Acq On : 08 Jul 2019 13:46
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 09 00:47:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.688	5249141	53.971 ug/ml
Target Compounds			
2) N-DECANE	4.389	6278475	49.718 ug/ml
3) N-DODECANE	6.415	6359261	50.119 ug/ml
4) N-TETRADECANE	8.213	6319452	50.504 ug/ml
5) N-HEXADECANE	9.818	6328999	51.256 ug/ml
6) N-OCTADECANE	11.265	6171922	52.097 ug/ml
7) N-EICOSANE	12.581	6123054	52.774 ug/ml
8) N-DOCOSANE	13.785	6017577	53.482 ug/ml
10) N-TETRACOSANE	14.895	6050532	54.355 ug/ml
11) N-HEXACOSANE	15.921	6014374	54.377 ug/ml
12) N-OCTACOSANE	16.878	6017704	53.951 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070819\
Data File : FF004990.D
Signal(s) : FID2B.ch
Acq On : 08 Jul 2019 13:46
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 09 00:47:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

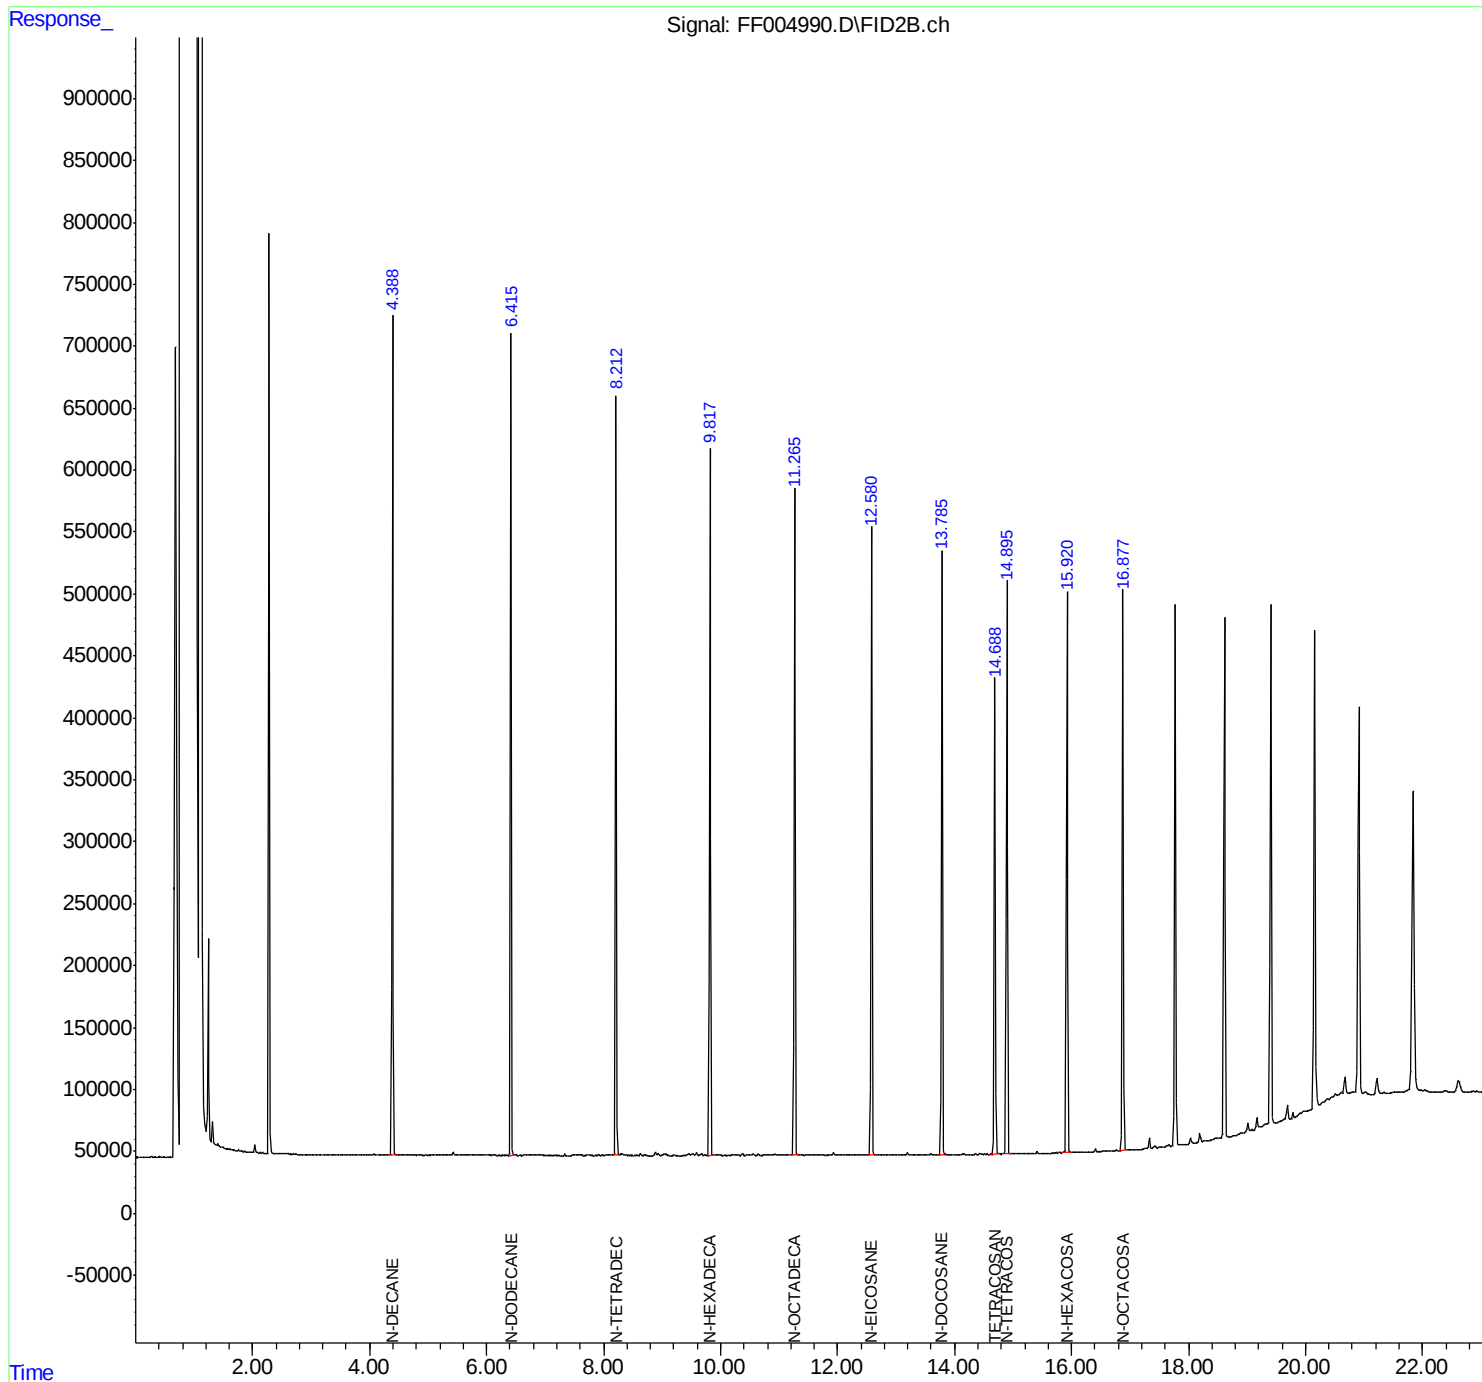

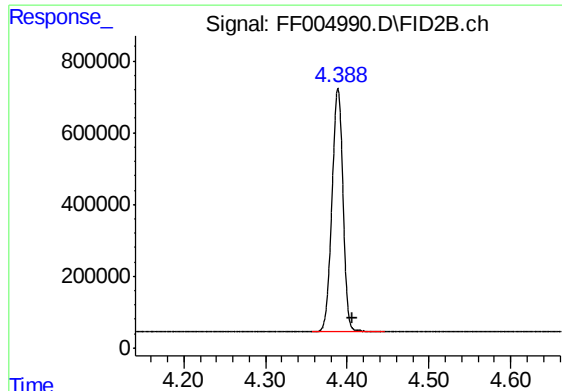


#2 N-DECANE

R.T.: 4.389 min
Delta R.T.: -0.017 min
Response: 6278475
Conc: 49.72 ug/ml

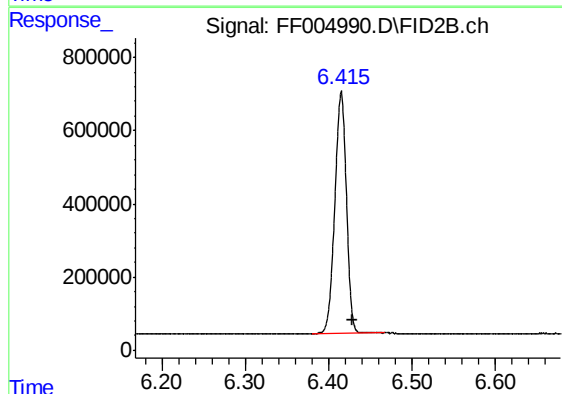


#3 N-DODECANE

R.T.: 6.415 min
Delta R.T.: -0.013 min
Response: 6359261
Conc: 50.12 ug/ml

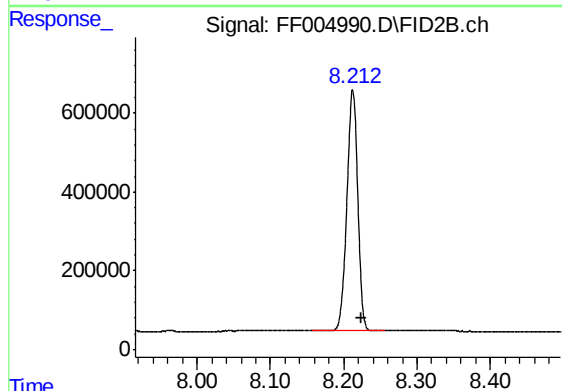


#4 N-TETRADECANE

R.T.: 8.213 min
Delta R.T.: -0.011 min
Response: 6319452
Conc: 50.50 ug/ml

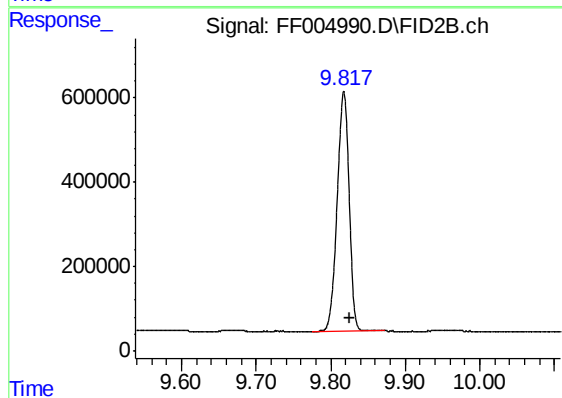


#5 N-HEXADECANE

R.T.: 9.818 min
Delta R.T.: -0.008 min
Response: 6328999
Conc: 51.26 ug/ml

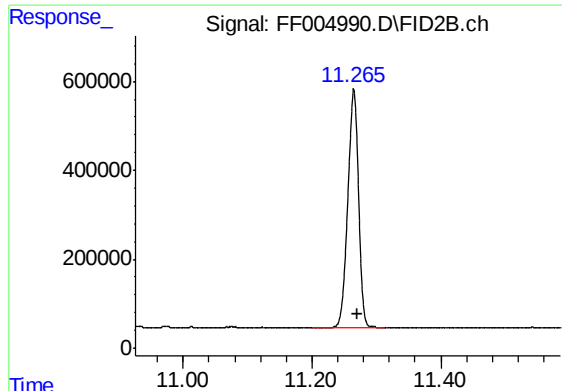


#6 N-OCTADECANE

R.T.: 11.265 min
Delta R.T.: -0.006 min
Response: 6171922
Conc: 52.10 ug/ml

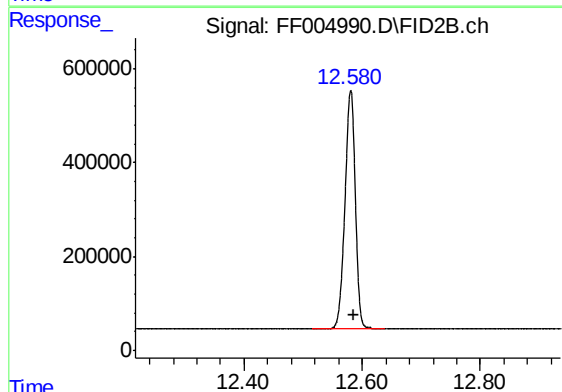


#7 N-EICOSANE

R.T.: 12.581 min
Delta R.T.: -0.005 min
Response: 6123054
Conc: 52.77 ug/ml

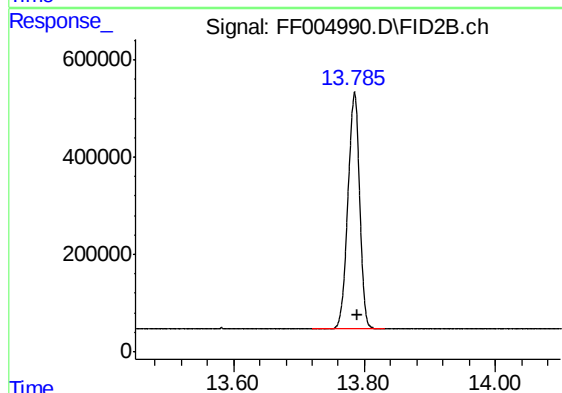


#8 N-DOCOSANE

R.T.: 13.785 min
Delta R.T.: -0.004 min
Response: 6017577
Conc: 53.48 ug/ml

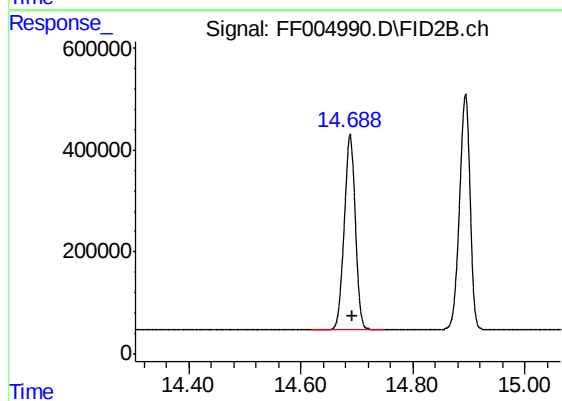


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.688 min
Delta R.T.: -0.004 min
Response: 5249141
Conc: 53.97 ug/ml

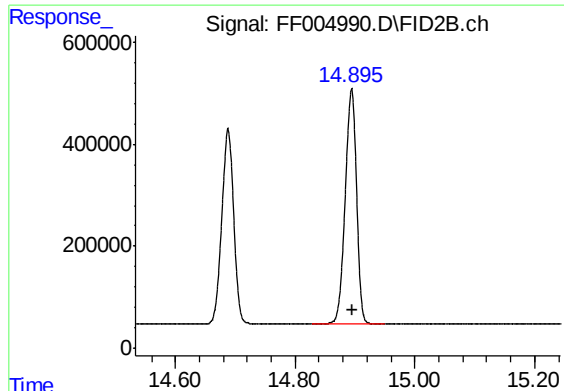


#10 N-TETRACOSANE

R.T.: 14.895 min
Delta R.T.: -0.002 min
Response: 6050532
Conc: 54.35 ug/ml

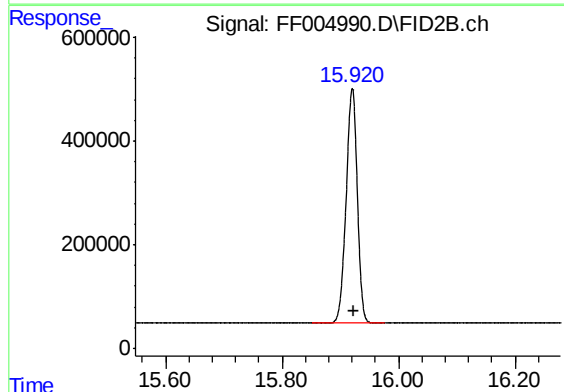

#11 N-HEXACOSANE

R.T.: 15.921 min
Delta R.T.: -0.001 min
Response: 6014374
Conc: 54.38 ug/ml

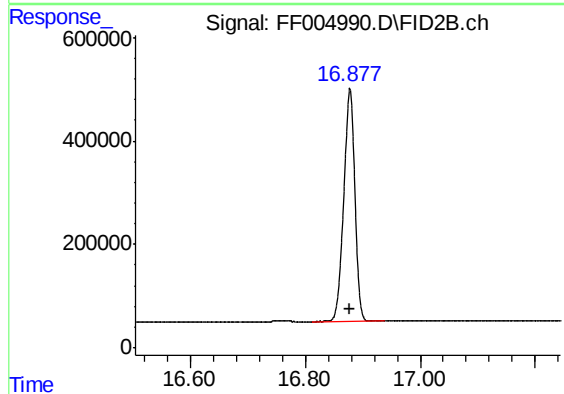

#12 N-OCTACOSANE

R.T.: 16.878 min
Delta R.T.: 0.000 min
Response: 6017704
Conc: 53.95 ug/ml