

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070921\
Data File : FF008751.D
Signal(s) : FID2B.ch
Acq On : 09 Jul 2021 09:36
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 09 22:46:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8)	N-DOCOSANE	13.802	58362	0.436 ug/ml
14)	N-DOTRIACONTANE	18.636	217003	1.852 ug/ml
16)	N-HEXATRIACONTANE	20.185	126695	1.349 ug/ml
18)	N-TETRACONTANE	21.857	122907	1.328 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070921\
Data File : FF008751.D
Signal(s) : FID2B.ch
Acq On : 09 Jul 2021 09:36
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 09 22:46:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

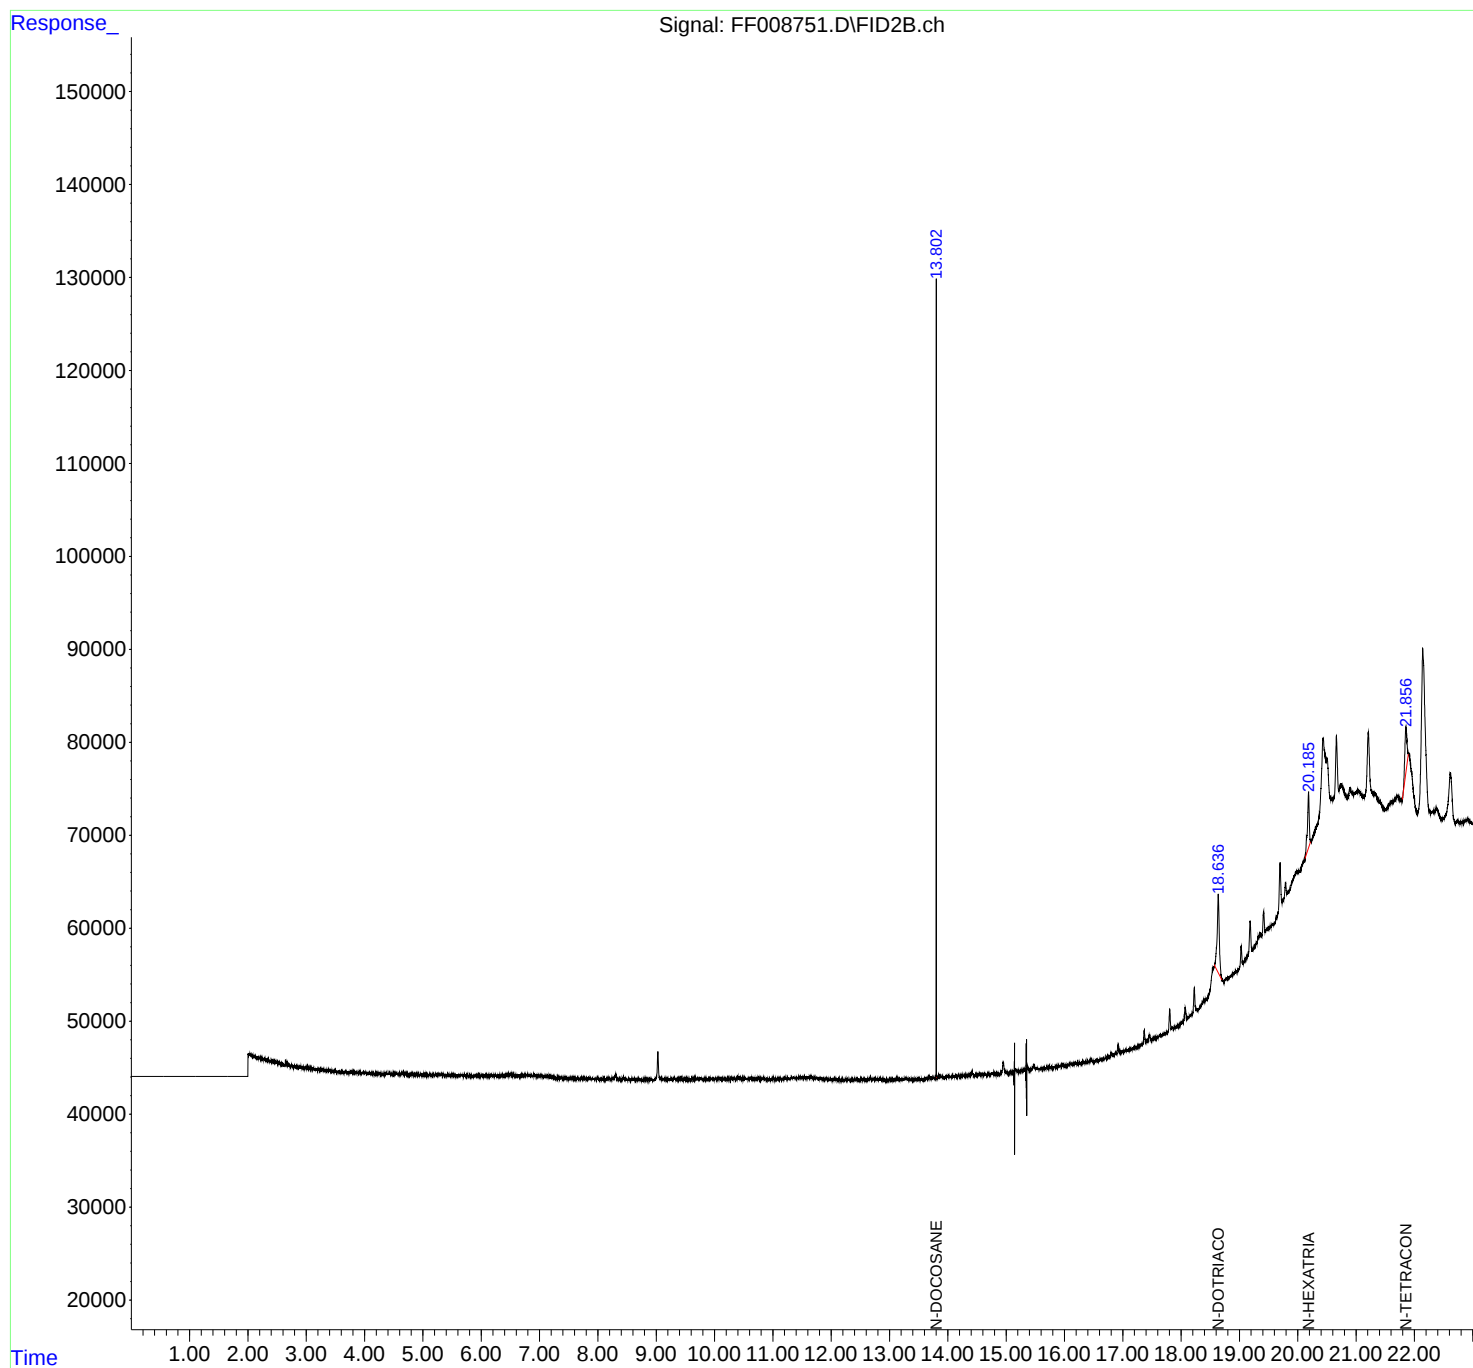


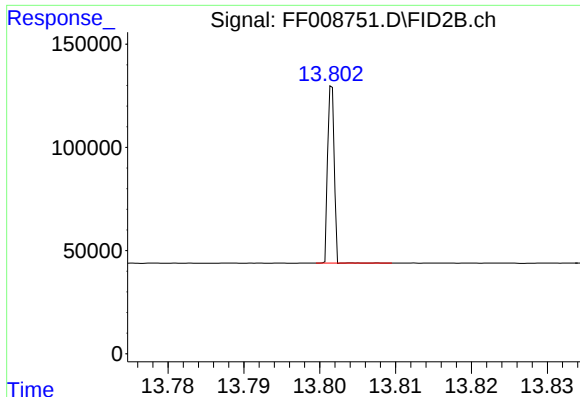

#8 N-DOCOSANE


R.T.: 13.802 min
Delta R.T.: -0.045 min
Response: 58362
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

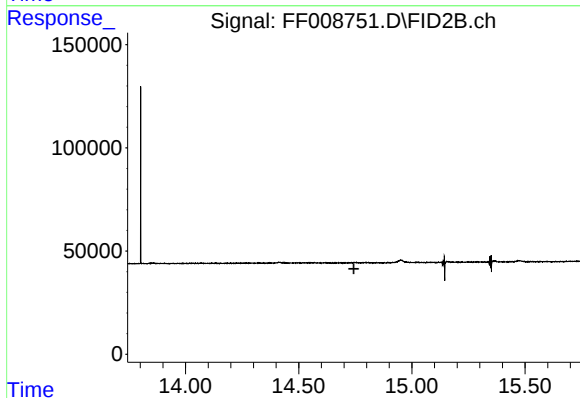


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.744 min
Response: 0
Conc: N.D.

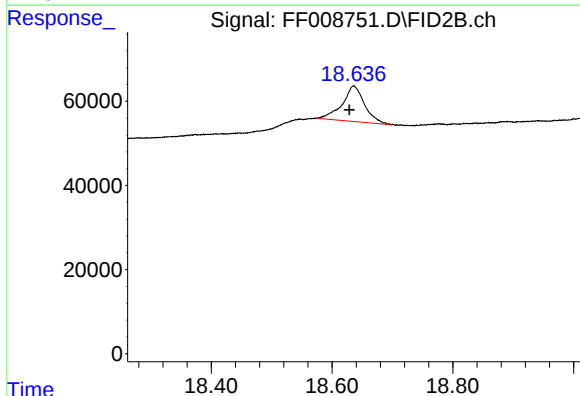


#14 N-DOTRIACONTANE

R.T.: 18.636 min
Delta R.T.: 0.007 min
Response: 217003
Conc: 1.85 ug/ml

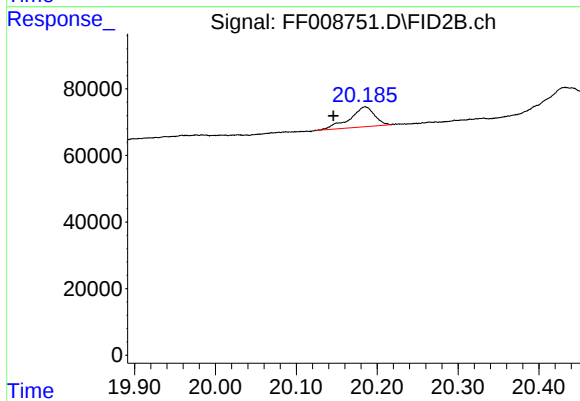

#16 N-HEXATRIACONTANE

R.T.: 20.185 min
Delta R.T.: 0.040 min
Response: 126695
Conc: 1.35 ug/ml

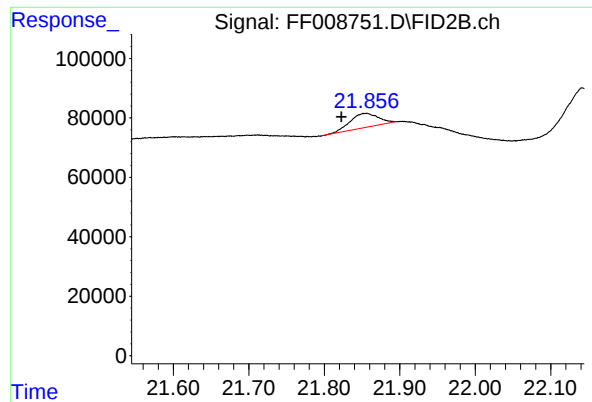

#18 N-TETRACONTANE

R.T.: 21.857 min
Delta R.T.: 0.034 min
Response: 122907
Conc: 1.33 ug/ml

Instrument :
FID_F
ClientSampleId :