

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070921\
 Data File : FF008758.D
 Signal(s) : FID2B.ch
 Acq On : 09 Jul 2021 15:47
 Operator : DD\AJ
 Sample : M2969-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 09 22:47:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	1678950	14.732 ug/ml
Target Compounds			
3) N-DODECANE	6.533	141277	1.039 ug/ml
7) N-EICOSANE	12.610	64408	0.470 ug/ml
10) N-TETRACOSANE	14.945	564919	4.287 ug/ml
12) N-OCTACOSANE	16.944	132936	1.075 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070921\
Data File : FF008758.D
Signal(s) : FID2B.ch
Acq On : 09 Jul 2021 15:47
Operator : DD\AJ
Sample : M2969-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 09 22:47:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

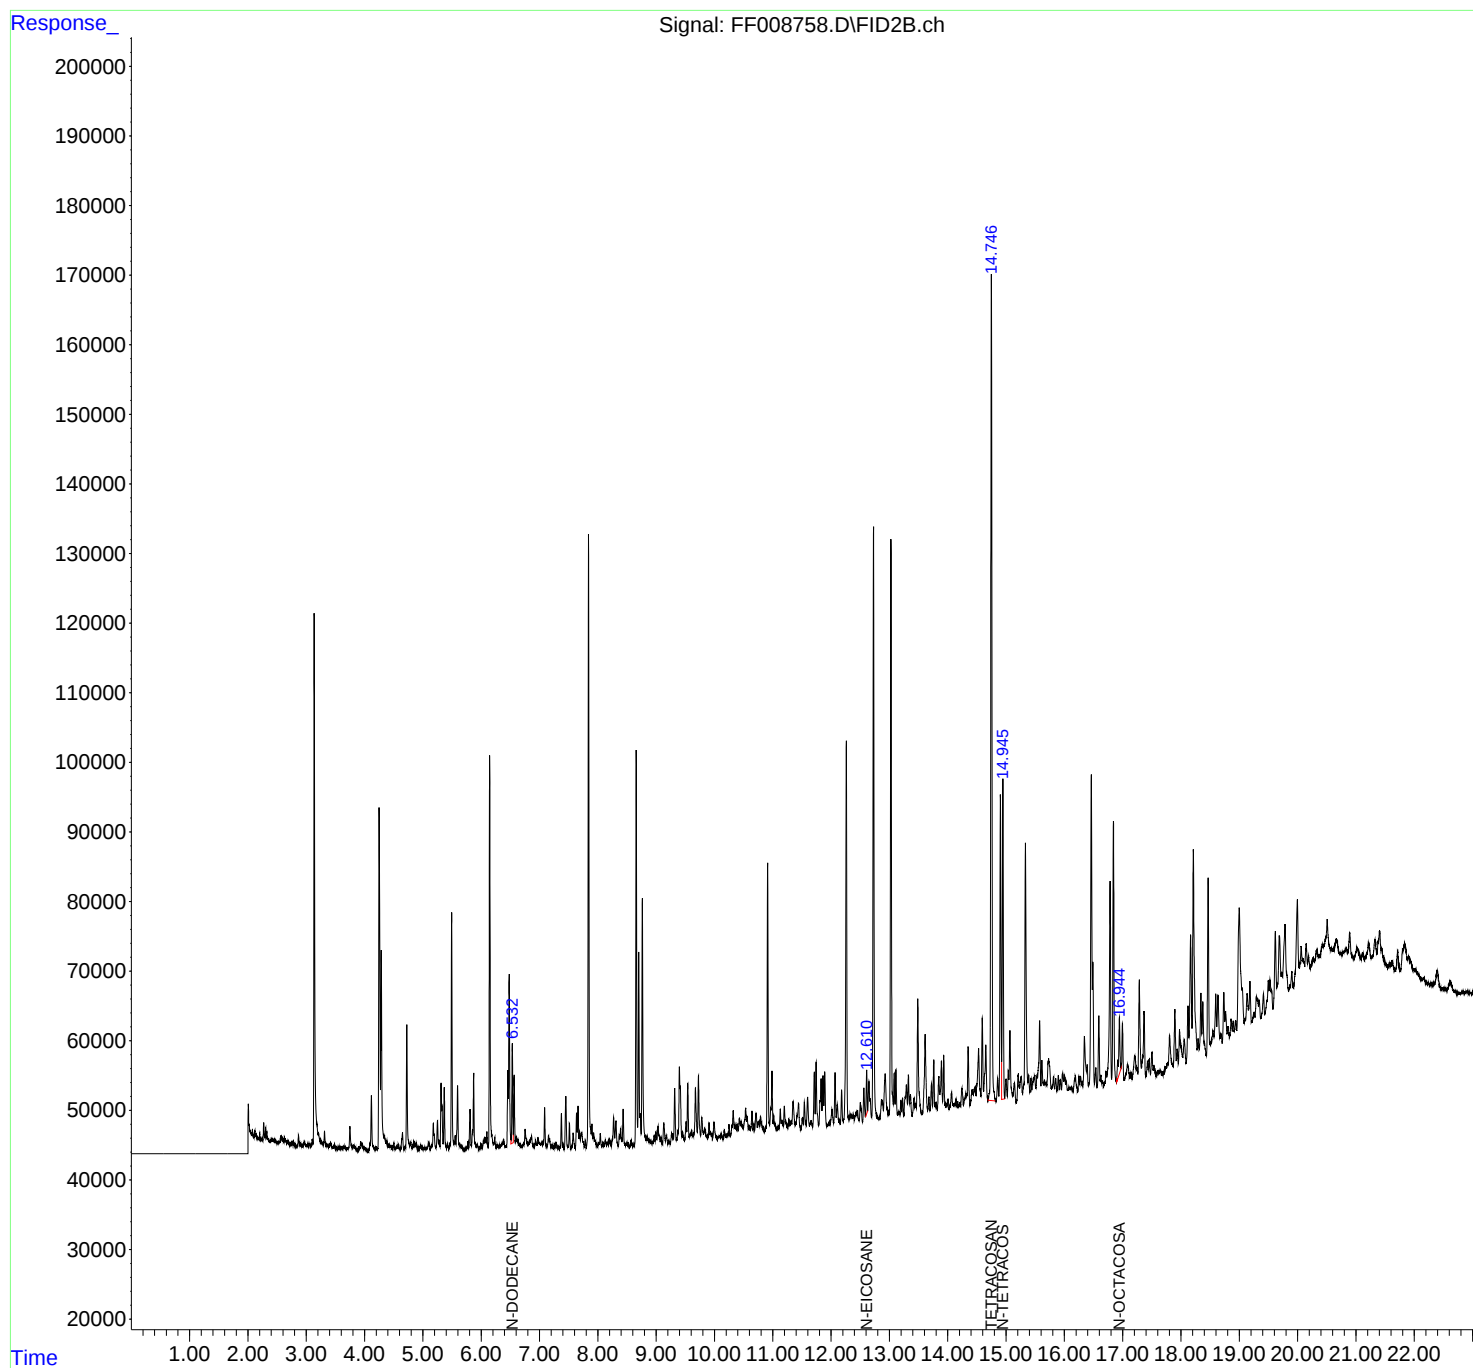


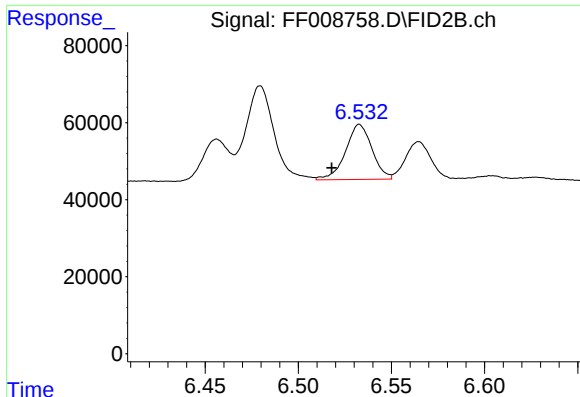

#3 N-DODECANE


R.T.: 6.533 min
Delta R.T.: 0.015 min
Response: 141277
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :

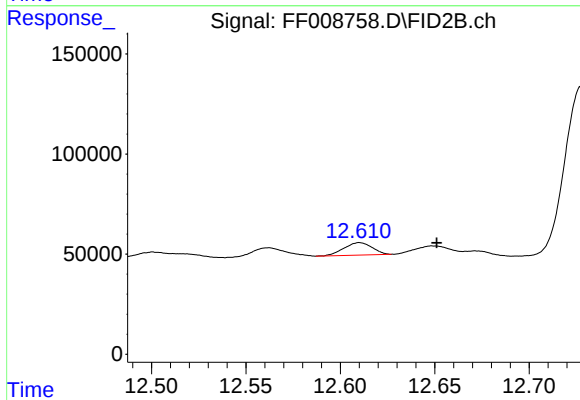


#7 N-EICOSANE

R.T.: 12.610 min
Delta R.T.: -0.041 min
Response: 64408
Conc: 0.47 ug/ml

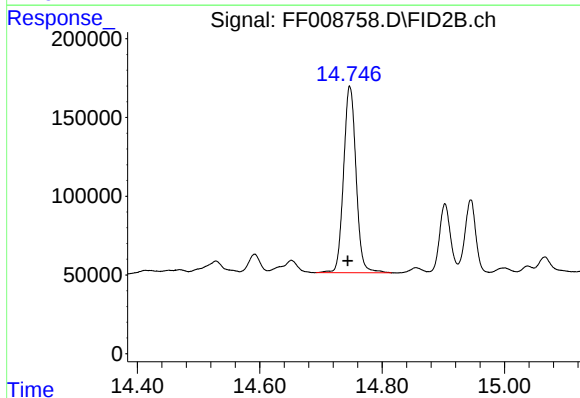


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.747 min
Delta R.T.: 0.003 min
Response: 1678950
Conc: 14.73 ug/ml

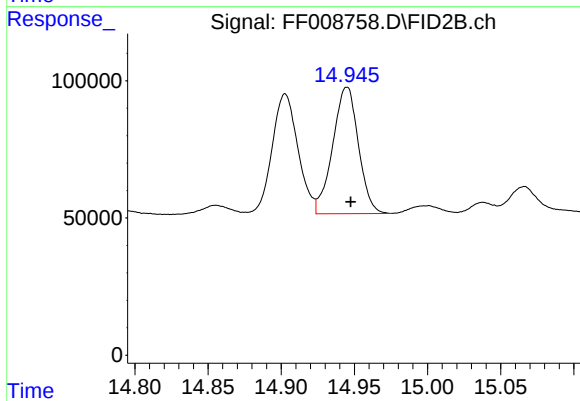

#10 N-TETRACOSANE

R.T.: 14.945 min
Delta R.T.: -0.003 min
Response: 564919
Conc: 4.29 ug/ml

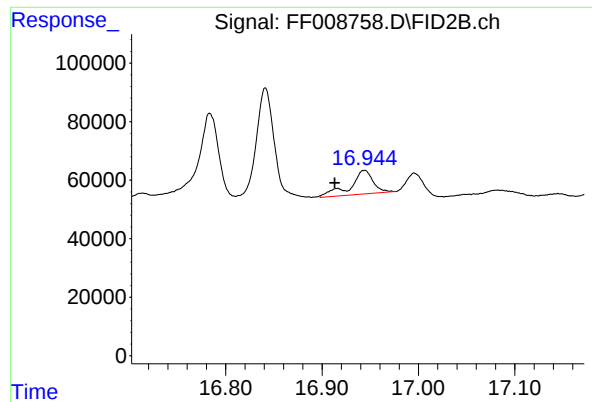

#12 N-OCTACOSANE

R.T.: 16.944 min
Delta R.T.: 0.031 min
Response: 132936
Conc: 1.07 ug/ml

Instrument :
FID_F
ClientSampleId :