

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070921\
Data File : FF008759.D
Signal(s) : FID2B.ch
Acq On : 09 Jul 2021 16:18
Operator : DD\AJ
Sample : M2969-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 09 22:47:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.746	1236293	10.848 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.943	199933	1.517 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070921\
Data File : FF008759.D
Signal(s) : FID2B.ch
Acq On : 09 Jul 2021 16:18
Operator : DD\AJ
Sample : M2969-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 09 22:47:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

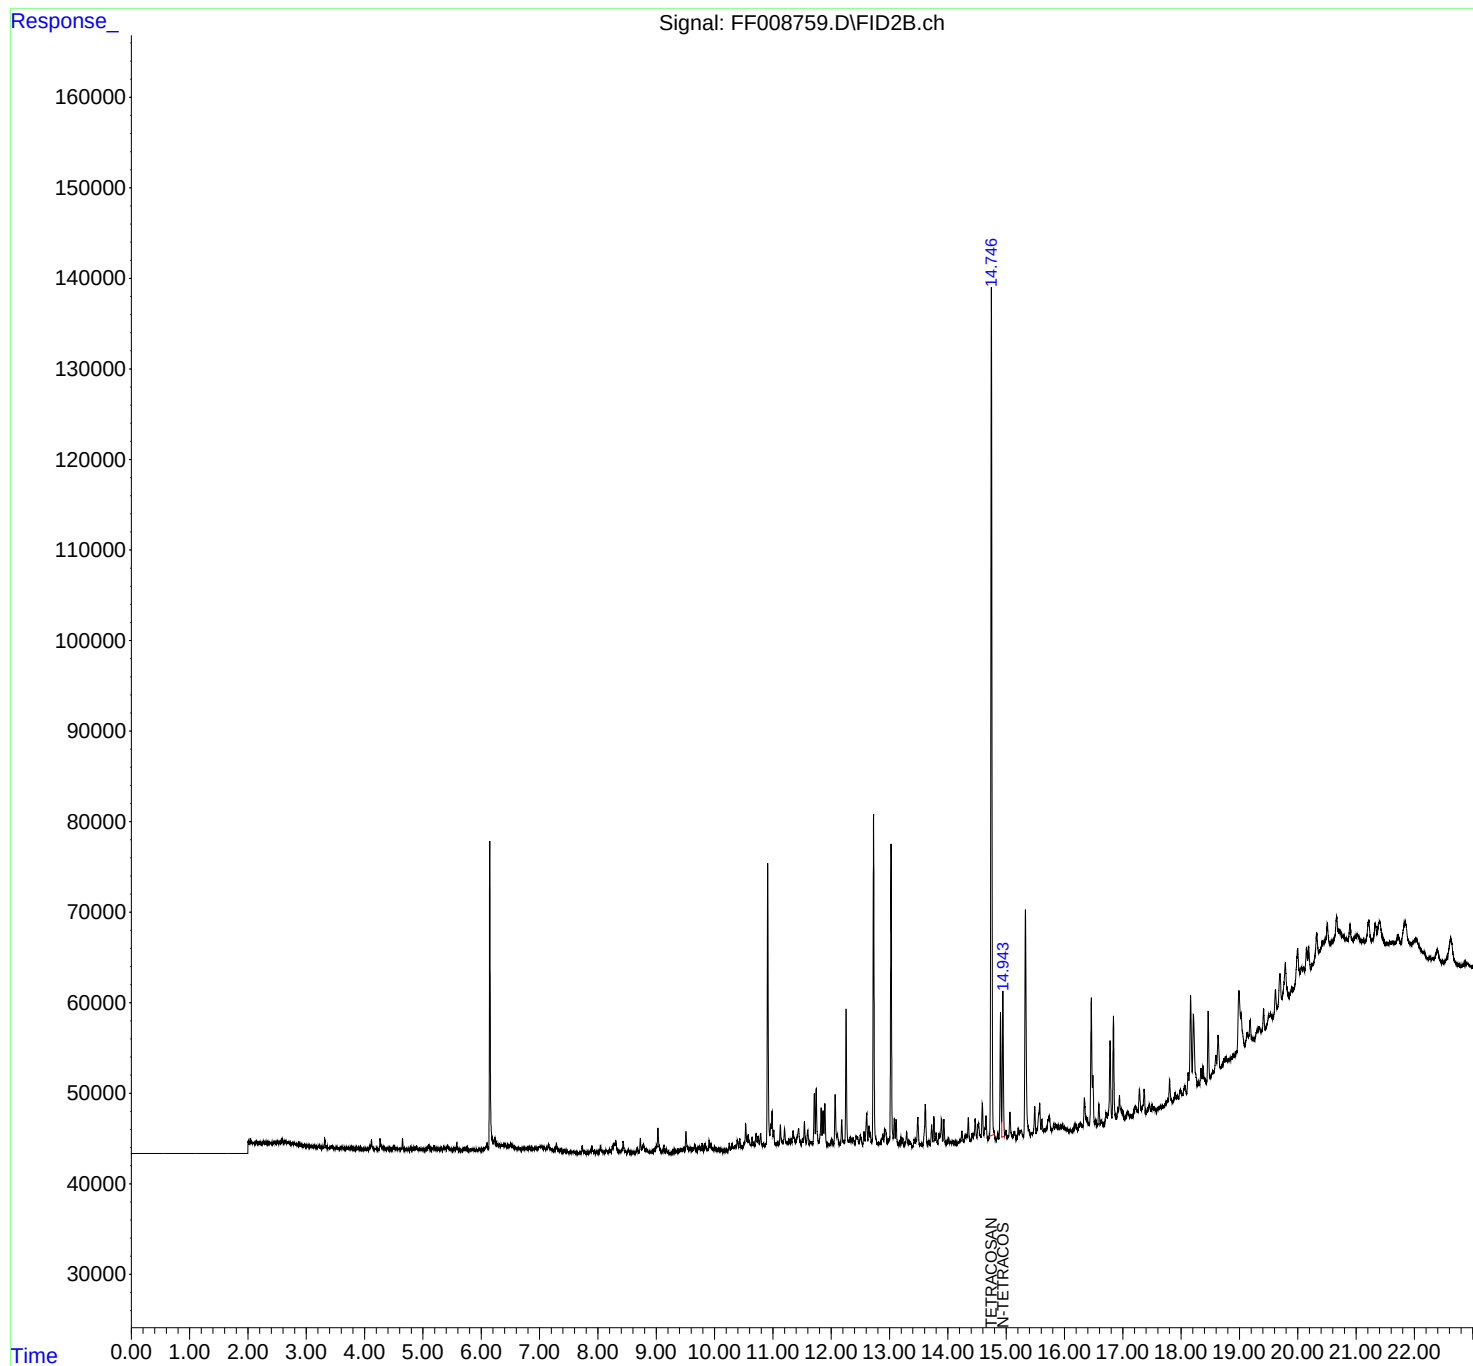


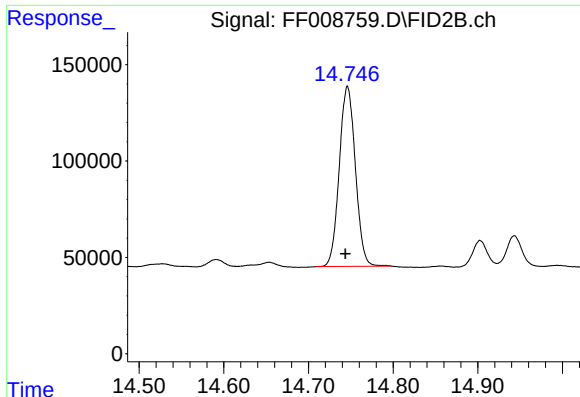

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.746 min
Delta R.T.: 0.002 min
Response: 1236293
Conc: 10.85 ug/ml

Instrument :
FID_F
ClientSampleId :

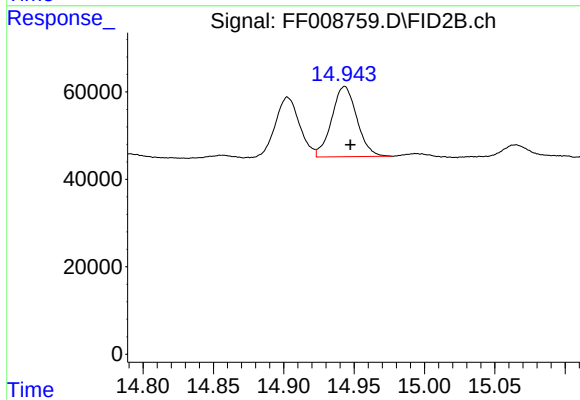

#10 N-TETRACOSANE

R.T.: 14.943 min
Delta R.T.: -0.004 min
Response: 199933
Conc: 1.52 ug/ml