

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070921\
Data File : FF008762.D
Signal(s) : FID2B.ch
Acq On : 09 Jul 2021 17:53
Operator : DD\AJ
Sample : M2969-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 09 22:48:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.747	1662611	14.588 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.632	225241	1.923 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070921\
Data File : FF008762.D
Signal(s) : FID2B.ch
Acq On : 09 Jul 2021 17:53
Operator : DD\AJ
Sample : M2969-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 09 22:48:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

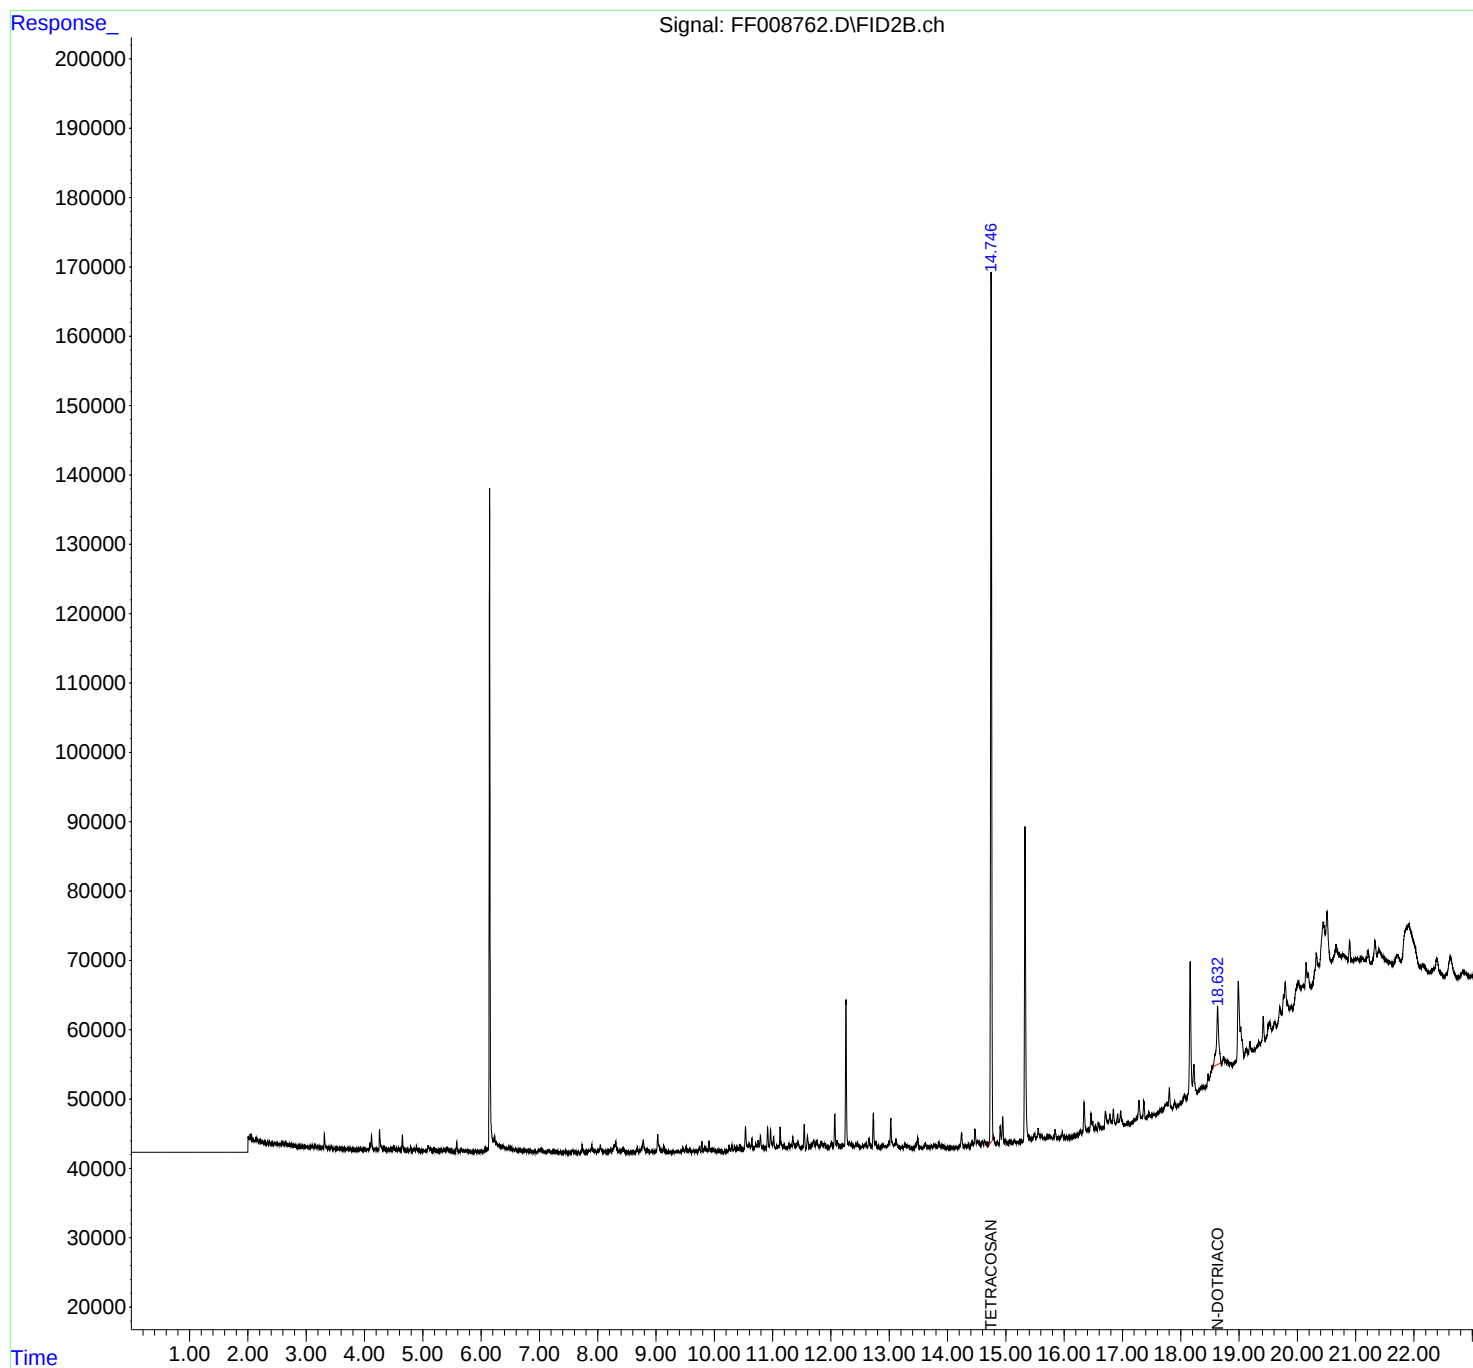


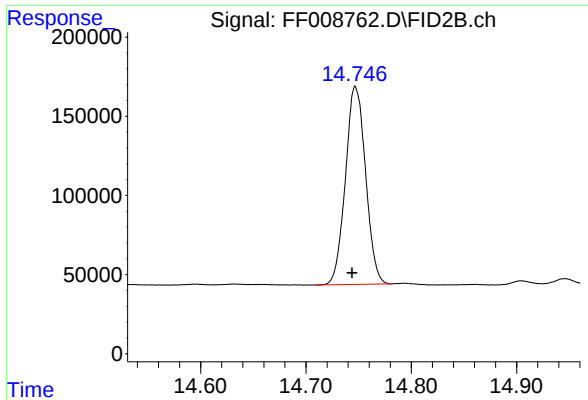

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.747 min
Delta R.T.: 0.003 min
Response: 1662611
Conc: 14.59 ug/ml

Instrument :
FID_F
ClientSampleId :

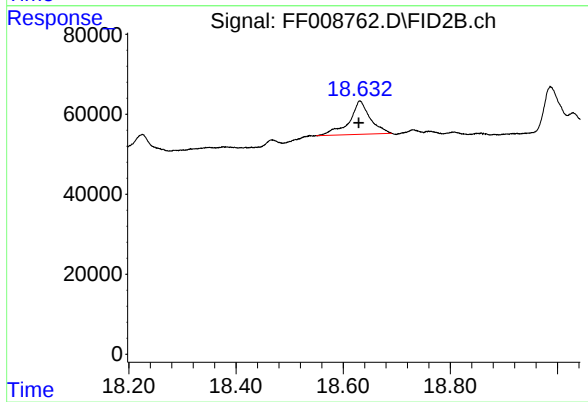

#14 N-DOTRIACONTANE

R.T.: 18.632 min
Delta R.T.: 0.003 min
Response: 225241
Conc: 1.92 ug/ml