

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071019\
 Data File : FF005006.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jul 2019 15:03
 Operator : DD\AJ
 Sample : K3697-02
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 11 00:47:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.680	1921818	19.760 ug/ml
Target Compounds			
4) N-TETRADECANE	8.270	609282	4.869 ug/ml
7) N-EICOSANE	12.576	177778	1.532 ug/ml
8) N-DOCOSANE	13.800	600685	5.339 ug/ml
10) N-TETRACOSANE	14.859	1656748	14.883 ug/ml
11) N-HEXACOSANE	15.913	237242	2.145 ug/ml
12) N-OCTACOSANE	16.867	722993	6.482 ug/ml
13) N-TRIACONTANE	17.758	641572	5.711 ug/ml
14) N-DOTRIACONTANE	18.596	275309	2.417 ug/ml
16) N-HEXATRIACONTANE	20.176	193043	1.864 ug/ml
18) N-TETRACONTANE	21.854	695857	5.986 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071019\
Data File : FF005006.D
Signal(s) : FID2B.ch
Acq On : 10 Jul 2019 15:03
Operator : DD\AJ
Sample : K3697-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 11 00:47:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

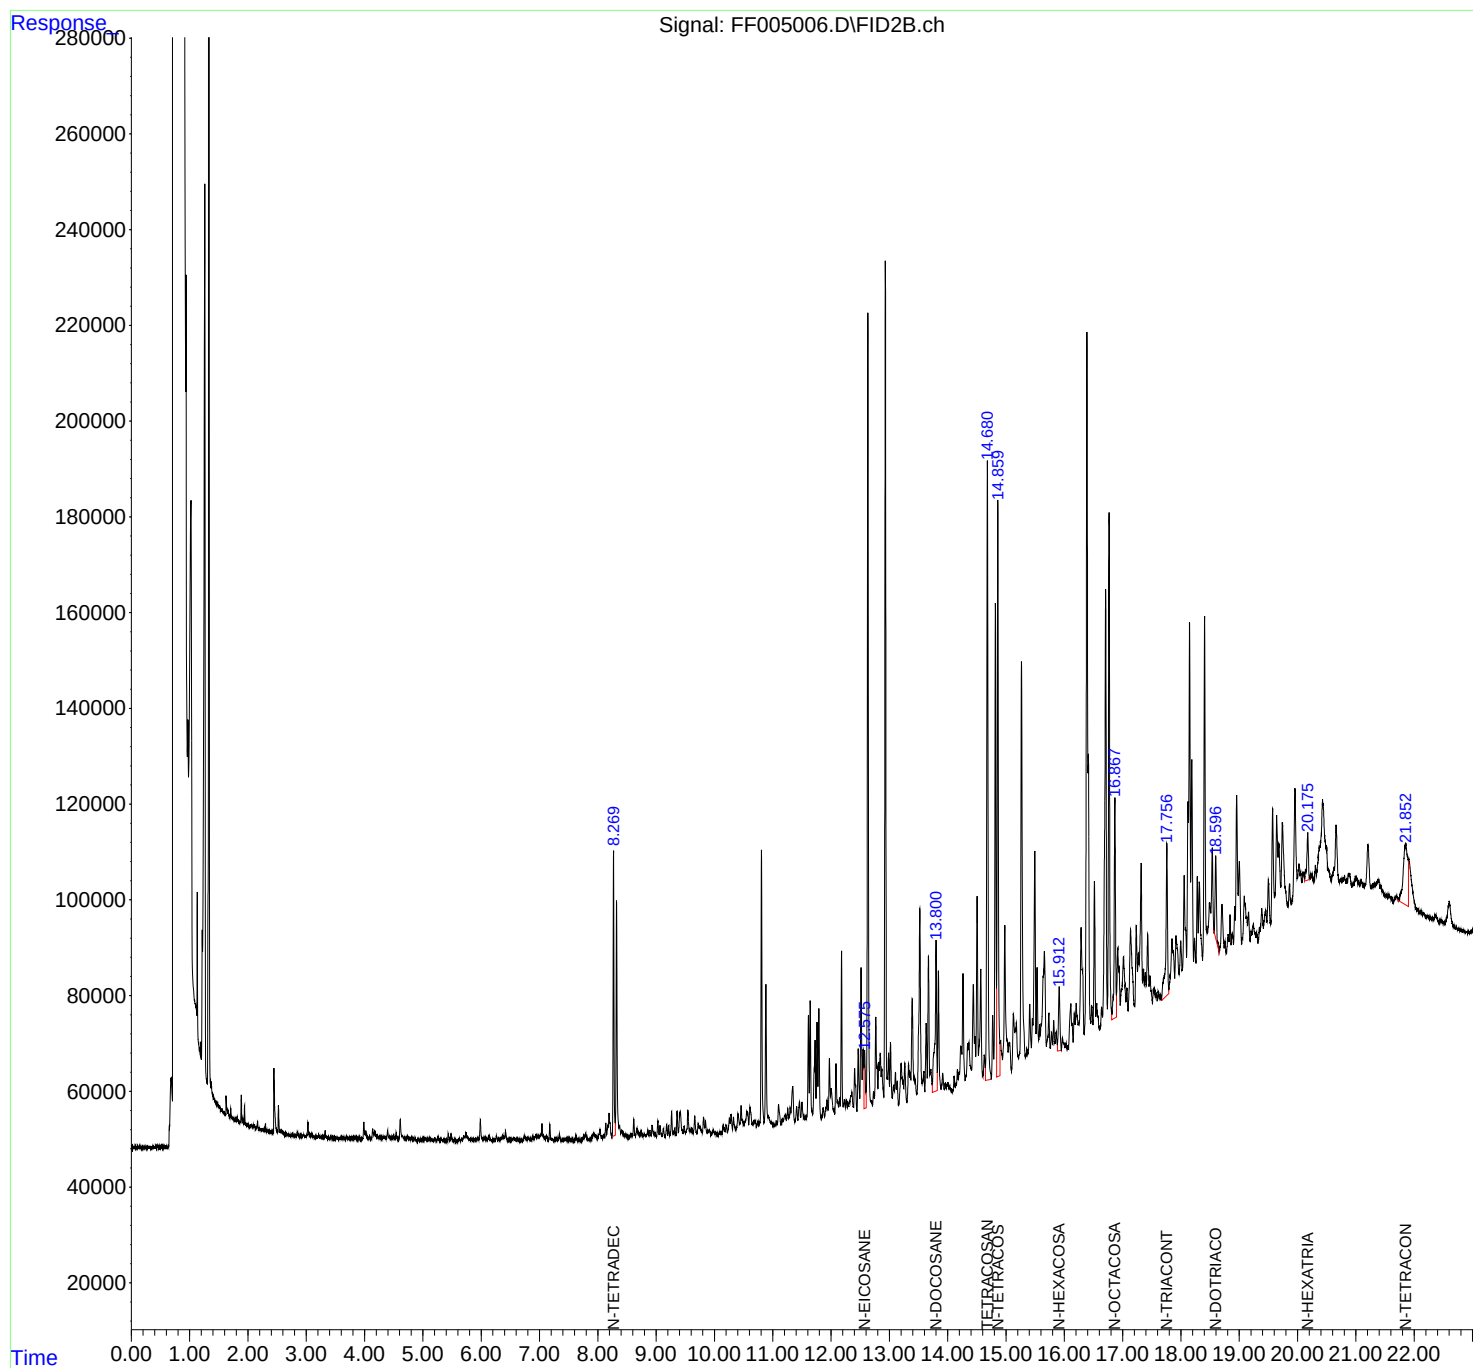

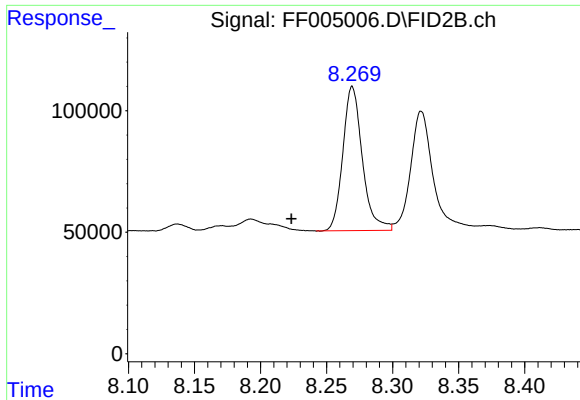


#4 N-TETRADECANE

R.T.: 8.270 min
Delta R.T.: 0.046 min
Response: 609282
Conc: 4.87 ug/ml

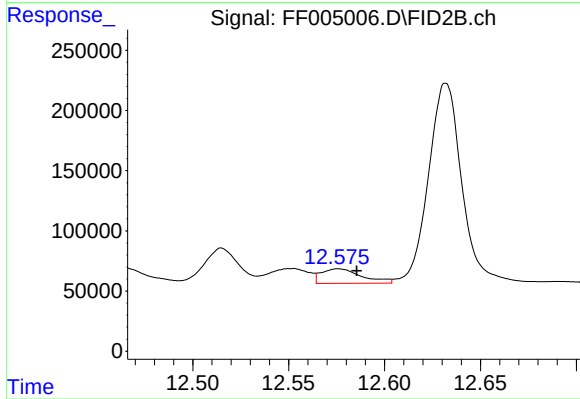


#7 N-EICOSANE

R.T.: 12.576 min
Delta R.T.: -0.010 min
Response: 177778
Conc: 1.53 ug/ml

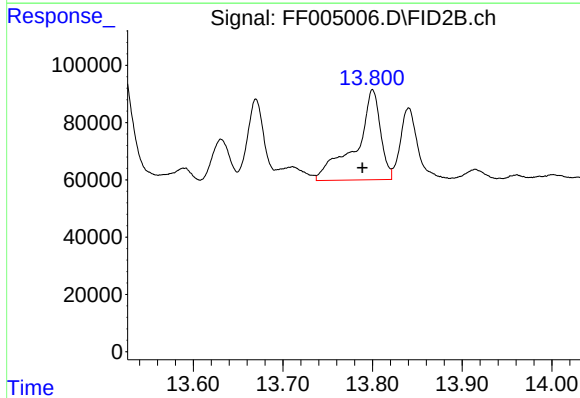


#8 N-DOCOSANE

R.T.: 13.800 min
Delta R.T.: 0.011 min
Response: 600685
Conc: 5.34 ug/ml

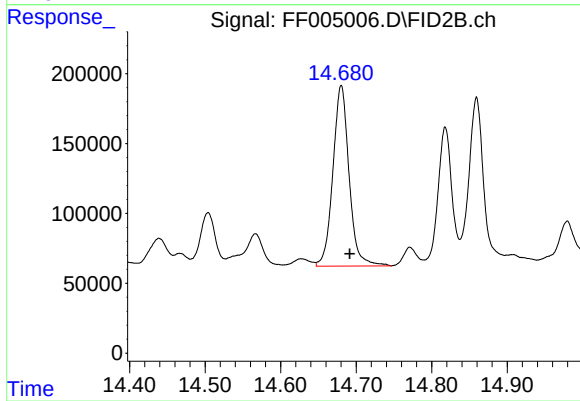


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.680 min
Delta R.T.: -0.011 min
Response: 1921818
Conc: 19.76 ug/ml

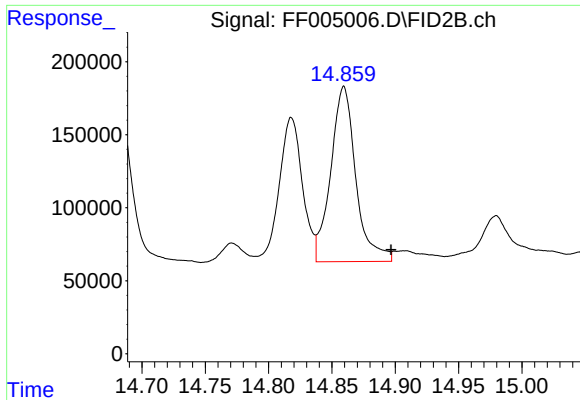


#10 N-TETRACOSANE

R.T.: 14.859 min
Delta R.T.: -0.037 min
Response: 1656748
Conc: 14.88 ug/ml

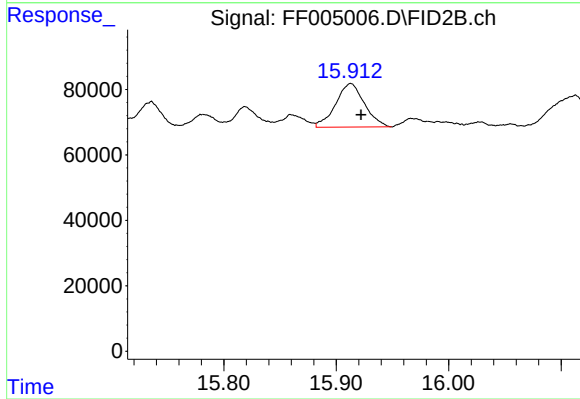


#11 N-HEXACOSANE

R.T.: 15.913 min
Delta R.T.: -0.009 min
Response: 237242
Conc: 2.14 ug/ml

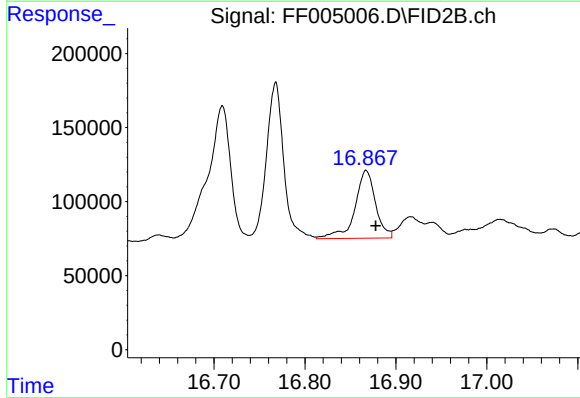


#12 N-OCTACOSANE

R.T.: 16.867 min
Delta R.T.: -0.010 min
Response: 722993
Conc: 6.48 ug/ml

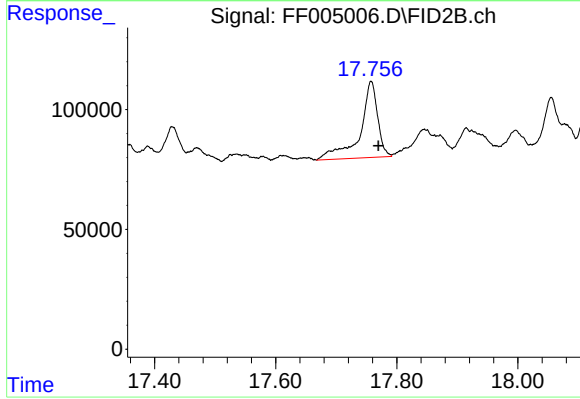


#13 N-TRIACONTANE

R.T.: 17.758 min
Delta R.T.: -0.012 min
Response: 641572
Conc: 5.71 ug/ml

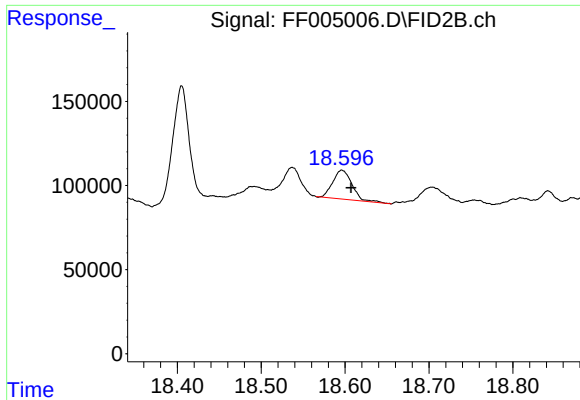


#14 N-DOTRIACONTANE

R.T.: 18.596 min
Delta R.T.: -0.011 min
Response: 275309
Conc: 2.42 ug/ml

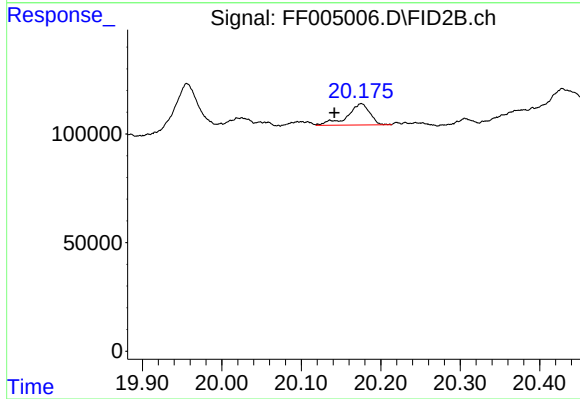

#16 N-HEXATRIACONTANE

R.T.: 20.176 min
Delta R.T.: 0.034 min
Response: 193043
Conc: 1.86 ug/ml

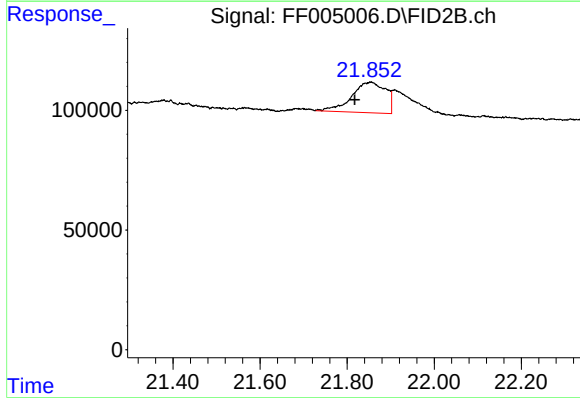

#18 N-TETRACONTANE

R.T.: 21.854 min
Delta R.T.: 0.036 min
Response: 695857
Conc: 5.99 ug/ml