

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071118\
 Data File : FF001278.D
 Signal(s) : FID2B.ch
 Acq On : 12 Jul 2018 01:30
 Operator : AJ\SJ
 Sample : J3832-01 5X
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 12 05:11:34 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.461	600539	5.575 ug/ml
Target Compounds				
4)	N-TETRADECANE	7.993	253252	2.014 ug/ml
7)	N-EICOSANE	12.418	634259	5.099 ug/ml
8)	N-DOCOSANE	13.605	532110	4.315 ug/ml
10)	N-TETRACOSANE	14.656	1735507	14.236 ug/ml
12)	N-OCTACOSANE	16.633	373158	3.097 ug/ml
13)	N-TRIACONTANE	17.517	638367	5.310 ug/ml
14)	N-DOTRIACONTANE	18.347	591803	5.019 ug/ml
15)	N-TETRATRIACONTANE	19.140	398642	3.392 ug/ml
16)	N-HEXATRIACONTANE	19.862	375599	3.307 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071118\
Data File : FF001278.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 01:30
Operator : AJ\SJ
Sample : J3832-01 5X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 12 05:11:34 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

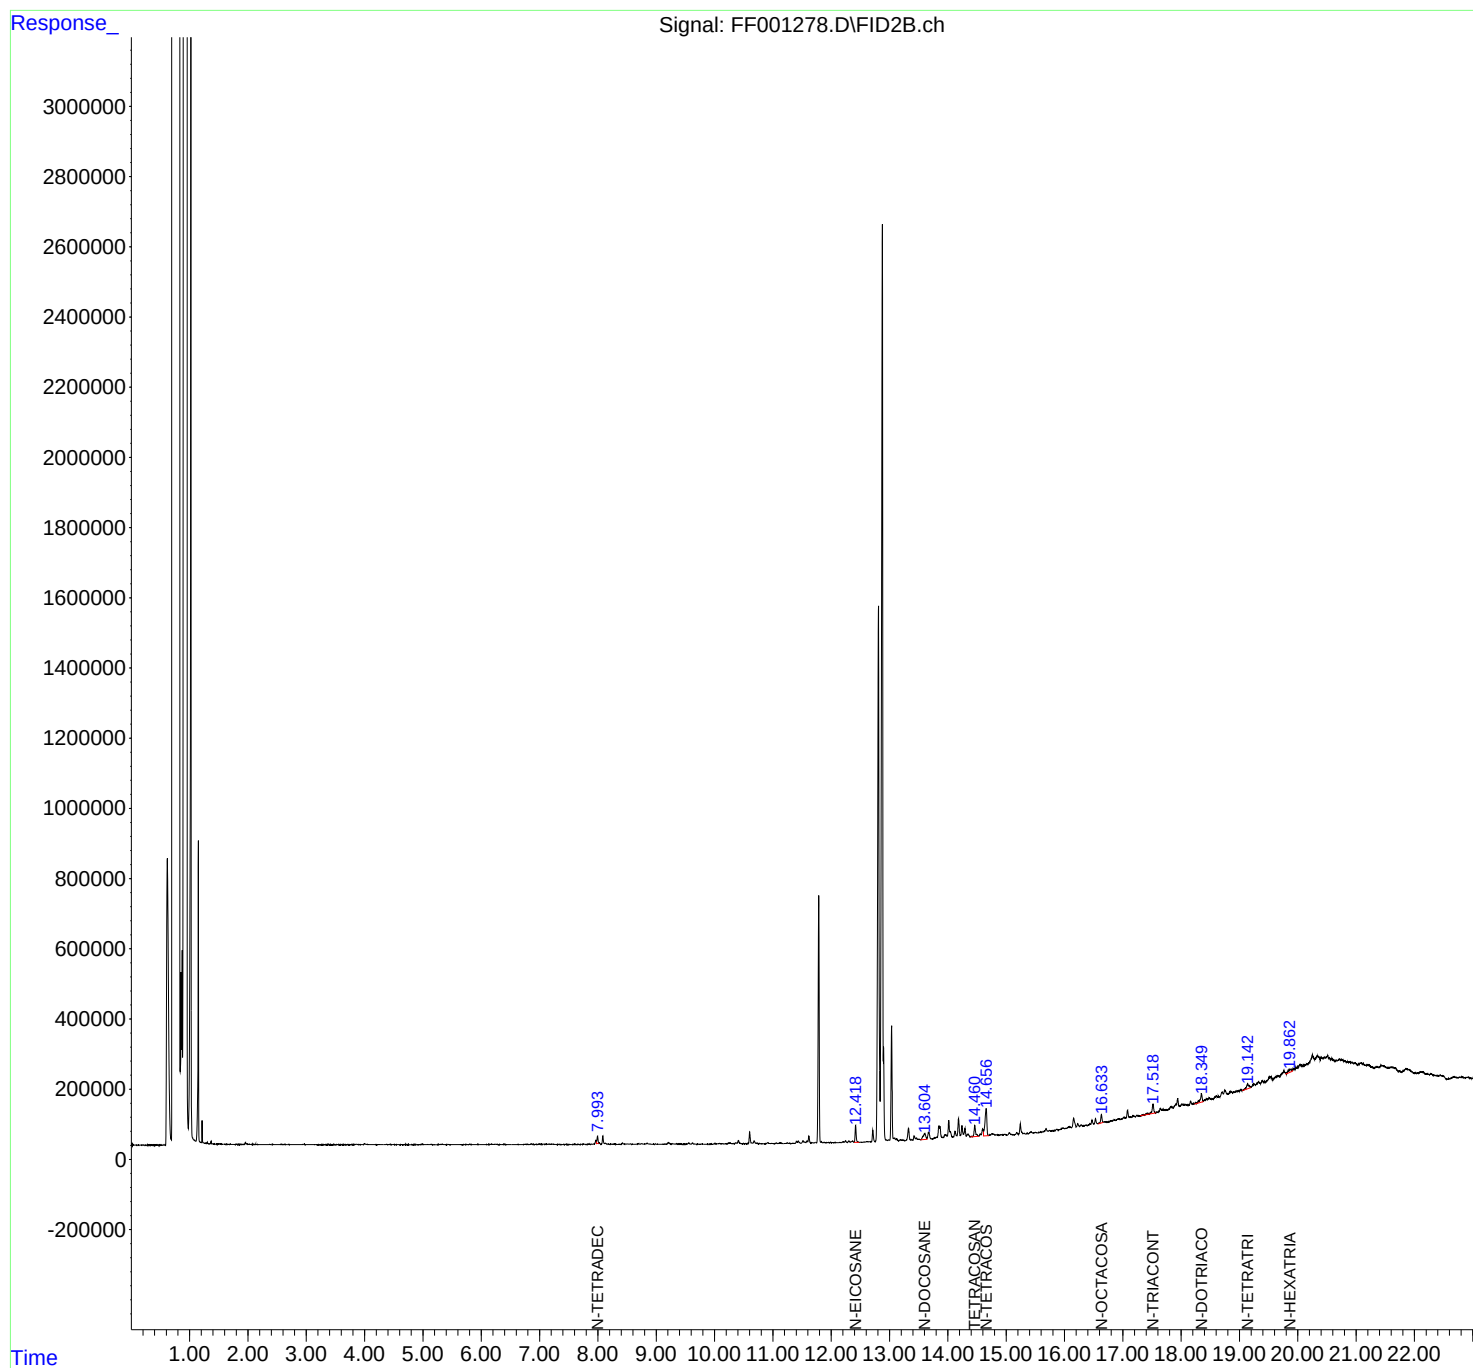

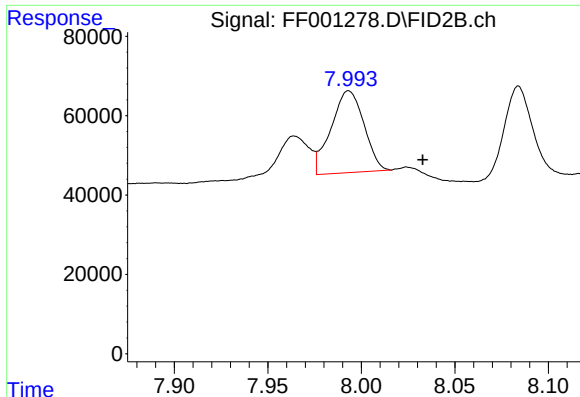


#4 N-TETRADECANE

R.T.: 7.993 min
Delta R.T.: -0.040 min
Response: 253252
Conc: 2.01 ug/ml

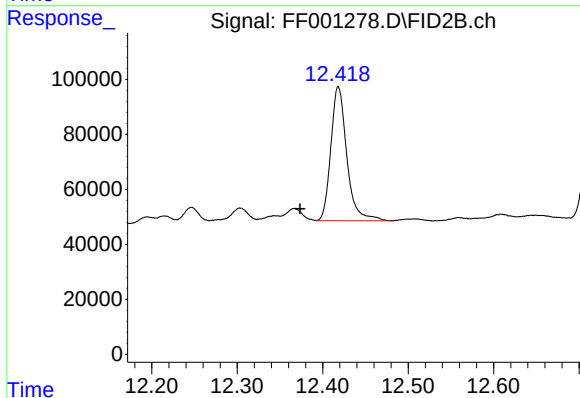


#7 N-EICOSANE

R.T.: 12.418 min
Delta R.T.: 0.045 min
Response: 634259
Conc: 5.10 ug/ml

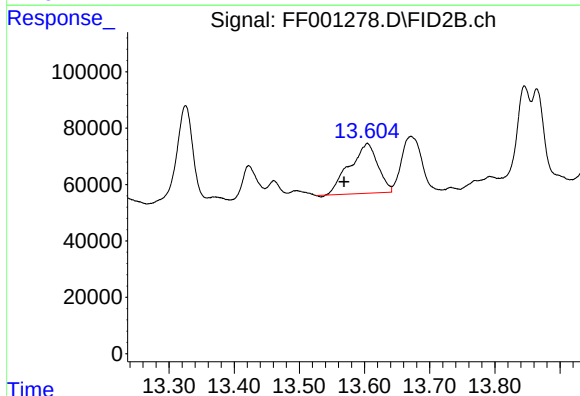


#8 N-DOCOSANE

R.T.: 13.605 min
Delta R.T.: 0.036 min
Response: 532110
Conc: 4.32 ug/ml

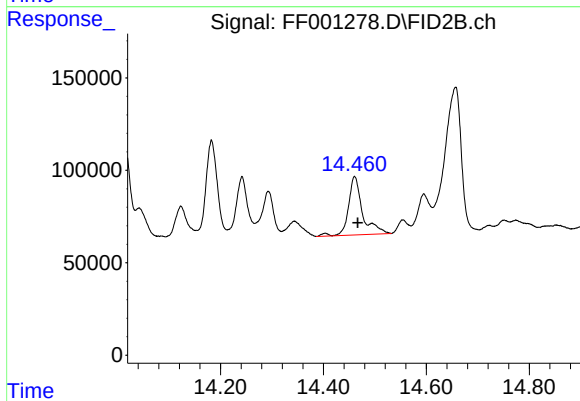


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.461 min
Delta R.T.: -0.006 min
Response: 600539
Conc: 5.57 ug/ml

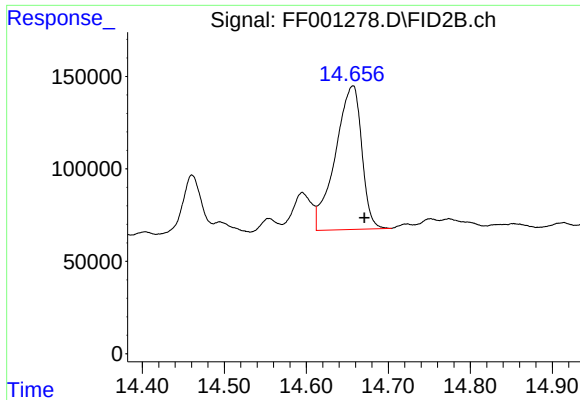


#10 N-TETRACOSANE

R.T.: 14.656 min
Delta R.T.: -0.015 min
Response: 1735507
Conc: 14.24 ug/ml

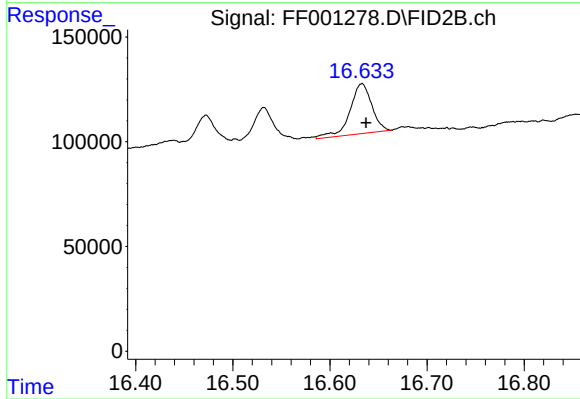


#12 N-OCTACOSANE

R.T.: 16.633 min
Delta R.T.: -0.004 min
Response: 373158
Conc: 3.10 ug/ml

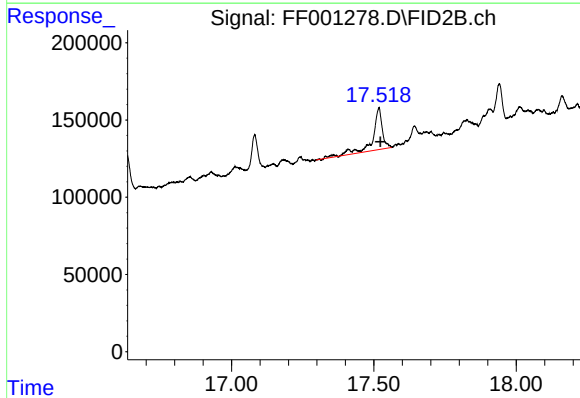


#13 N-TRIACONTANE

R.T.: 17.517 min
Delta R.T.: -0.005 min
Response: 638367
Conc: 5.31 ug/ml

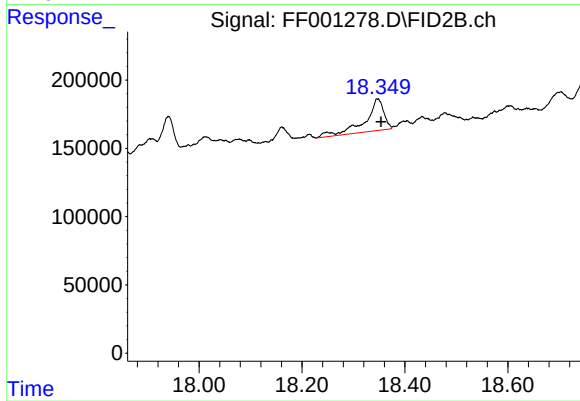

#14 N-DOTRIACONTANE

R.T.: 18.347 min
Delta R.T.: -0.006 min
Response: 591803
Conc: 5.02 ug/ml

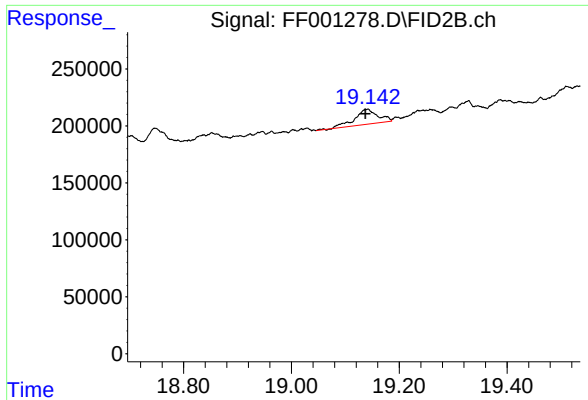


#15 N-TETRATRIACONTANE

R.T.: 19.140 min

Delta R.T.: 0.003 min

Response: 398642

Conc: 3.39 ug/ml

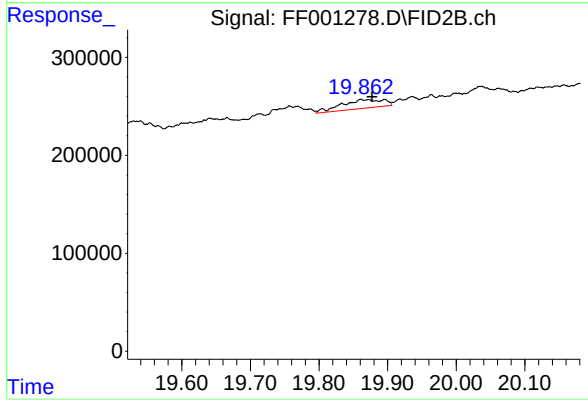

#16 N-HEXATRIACONTANE

R.T.: 19.862 min

Delta R.T.: -0.016 min

Response: 375599

Conc: 3.31 ug/ml