

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071118\
 Data File : FF001252.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jul 2018 11:00
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 12 05:03:50 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.461	5401384	50.141 ug/ml
Target Compounds			
2) N-DECANE	4.227	6511774	52.448 ug/ml
3) N-DODECANE	6.239	6535567	52.158 ug/ml
4) N-TETRADECANE	8.027	6542368	52.019 ug/ml
5) N-HEXADECANE	9.622	6513733	52.133 ug/ml
6) N-OCTADECANE	11.060	6469113	51.620 ug/ml
7) N-EICOSANE	12.367	6323229	50.834 ug/ml
8) N-DOCOSANE	13.564	6170304	50.039 ug/ml
10) N-TETRACOSANE	14.664	6018591	49.370 ug/ml
11) N-HEXACOSANE	15.682	5888145	48.577 ug/ml
12) N-OCTACOSANE	16.631	5831541	48.406 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071118\
Data File : FF001252.D
Signal(s) : FID2B.ch
Acq On : 11 Jul 2018 11:00
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 12 05:03:50 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

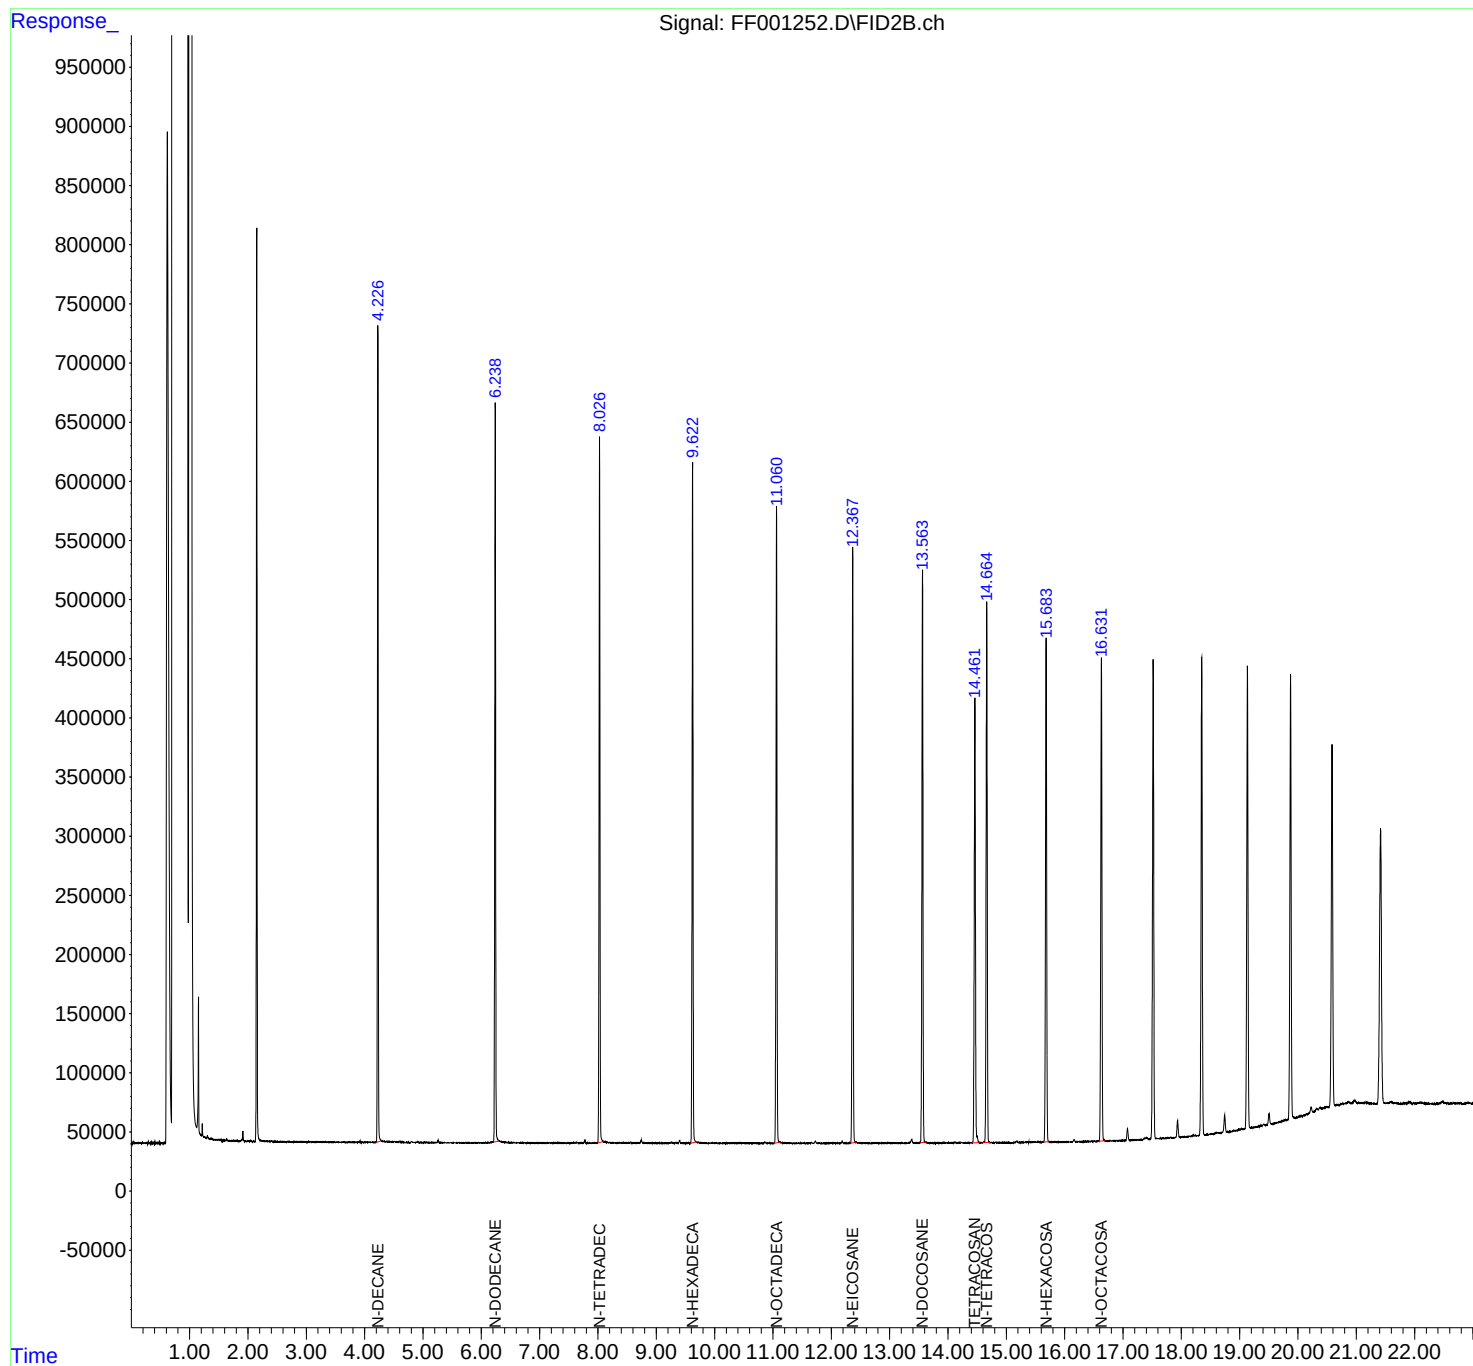

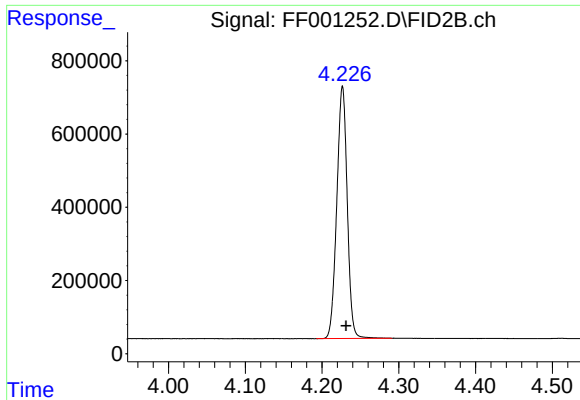


#2 N-DECANE

R.T.: 4.227 min
Delta R.T.: -0.005 min
Response: 6511774
Conc: 52.45 ug/ml

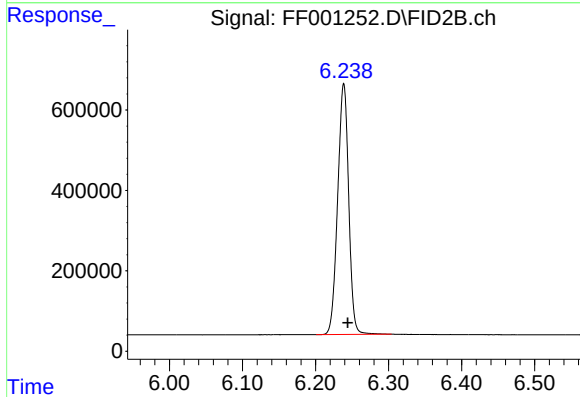


#3 N-DODECANE

R.T.: 6.239 min
Delta R.T.: -0.005 min
Response: 6535567
Conc: 52.16 ug/ml

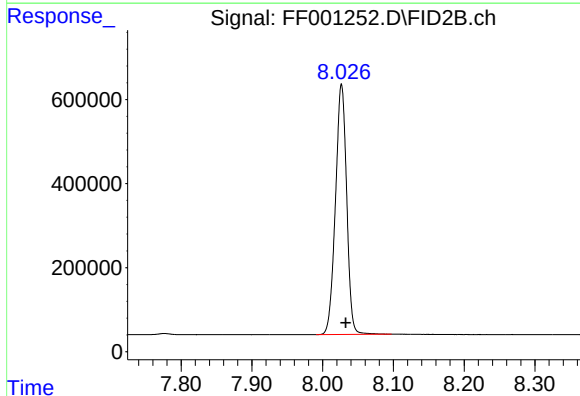


#4 N-TETRADECANE

R.T.: 8.027 min
Delta R.T.: -0.006 min
Response: 6542368
Conc: 52.02 ug/ml

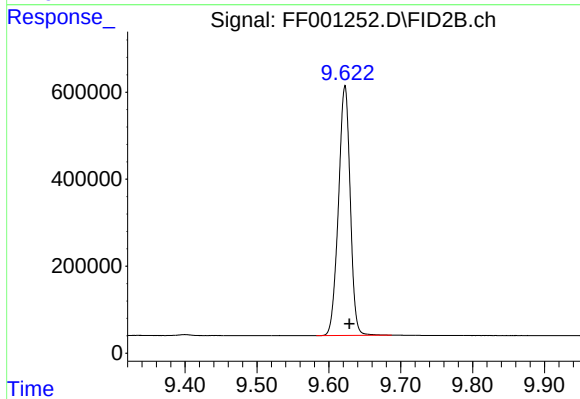


#5 N-HEXADECANE

R.T.: 9.622 min
Delta R.T.: -0.006 min
Response: 6513733
Conc: 52.13 ug/ml

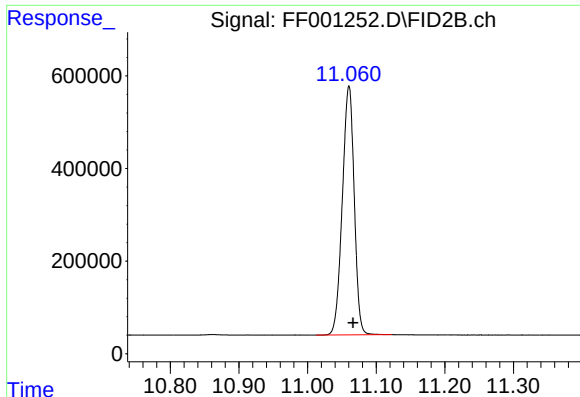


#6 N-OCTADECANE

R.T.: 11.060 min
Delta R.T.: -0.006 min
Response: 6469113
Conc: 51.62 ug/ml

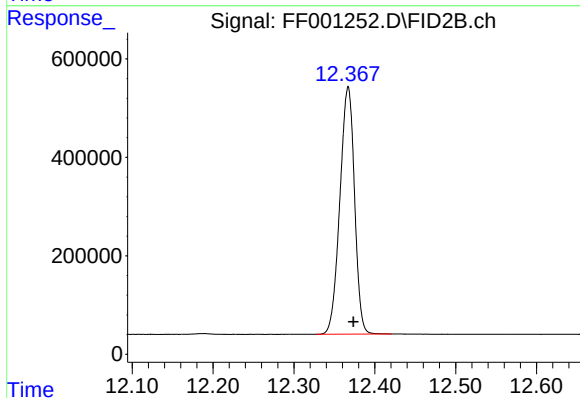


#7 N-EICOSANE

R.T.: 12.367 min
Delta R.T.: -0.006 min
Response: 6323229
Conc: 50.83 ug/ml

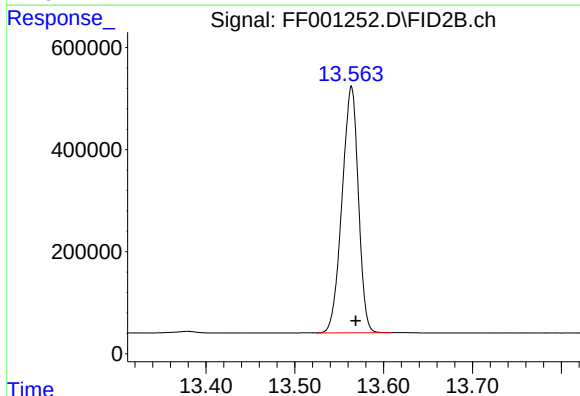


#8 N-DOCOSANE

R.T.: 13.564 min
Delta R.T.: -0.005 min
Response: 6170304
Conc: 50.04 ug/ml

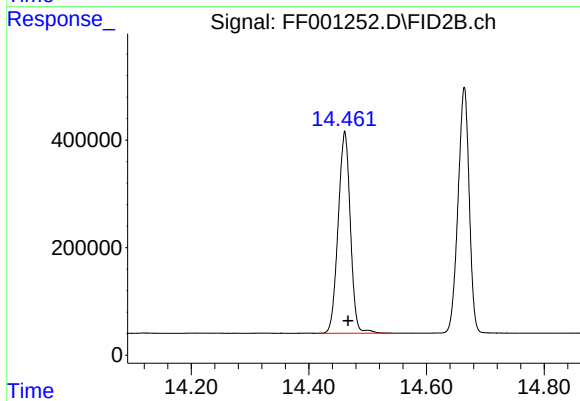


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.461 min
Delta R.T.: -0.006 min
Response: 5401384
Conc: 50.14 ug/ml

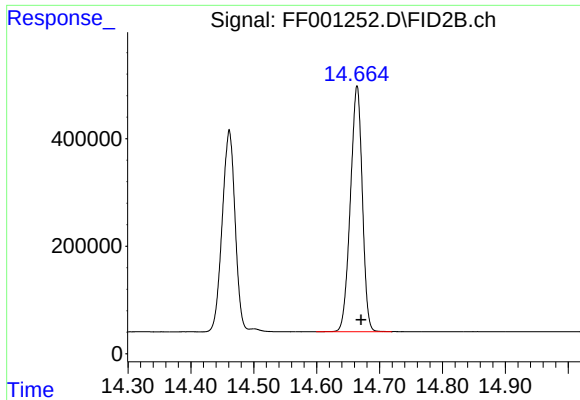


#10 N-TETRACOSANE

R.T.: 14.664 min
Delta R.T.: -0.006 min
Response: 6018591
Conc: 49.37 ug/ml

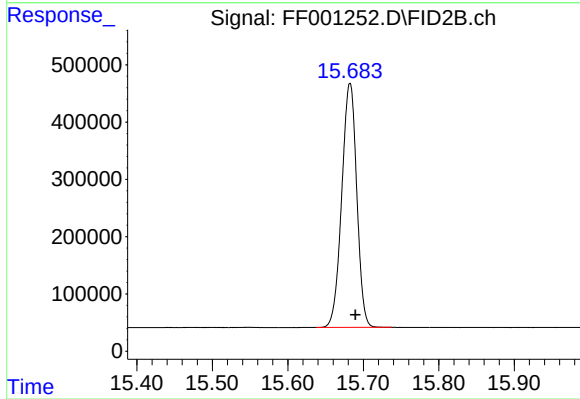

#11 N-HEXACOSANE

R.T.: 15.682 min
Delta R.T.: -0.007 min
Response: 5888145
Conc: 48.58 ug/ml

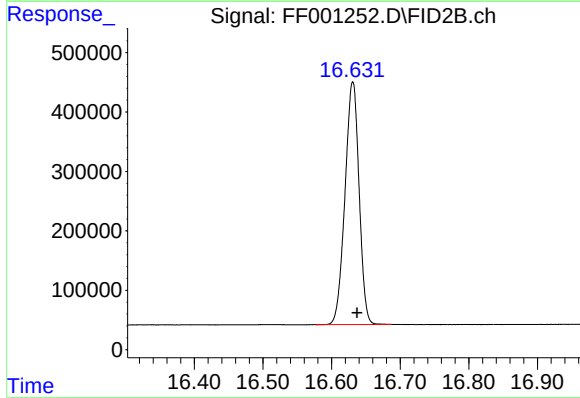

#12 N-OCTACOSANE

R.T.: 16.631 min
Delta R.T.: -0.006 min
Response: 5831541
Conc: 48.41 ug/ml