

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001285.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 12:40
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:36:11 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.234	3852367	30.744 ug/ml
12) N-OCTACOSANE	16.632	3542103	29.402 ug/ml
13) N-TRIACONTANE	17.515	281506	2.342 ug/ml
14) N-DOTRIACONTANE	18.348	406134	3.445 ug/ml
15) N-TETRATRIACONTANE	19.132	304342	2.589 ug/ml
16) N-HEXATRIACONTANE	19.873	191624	1.687 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001285.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 12:40
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:36:11 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

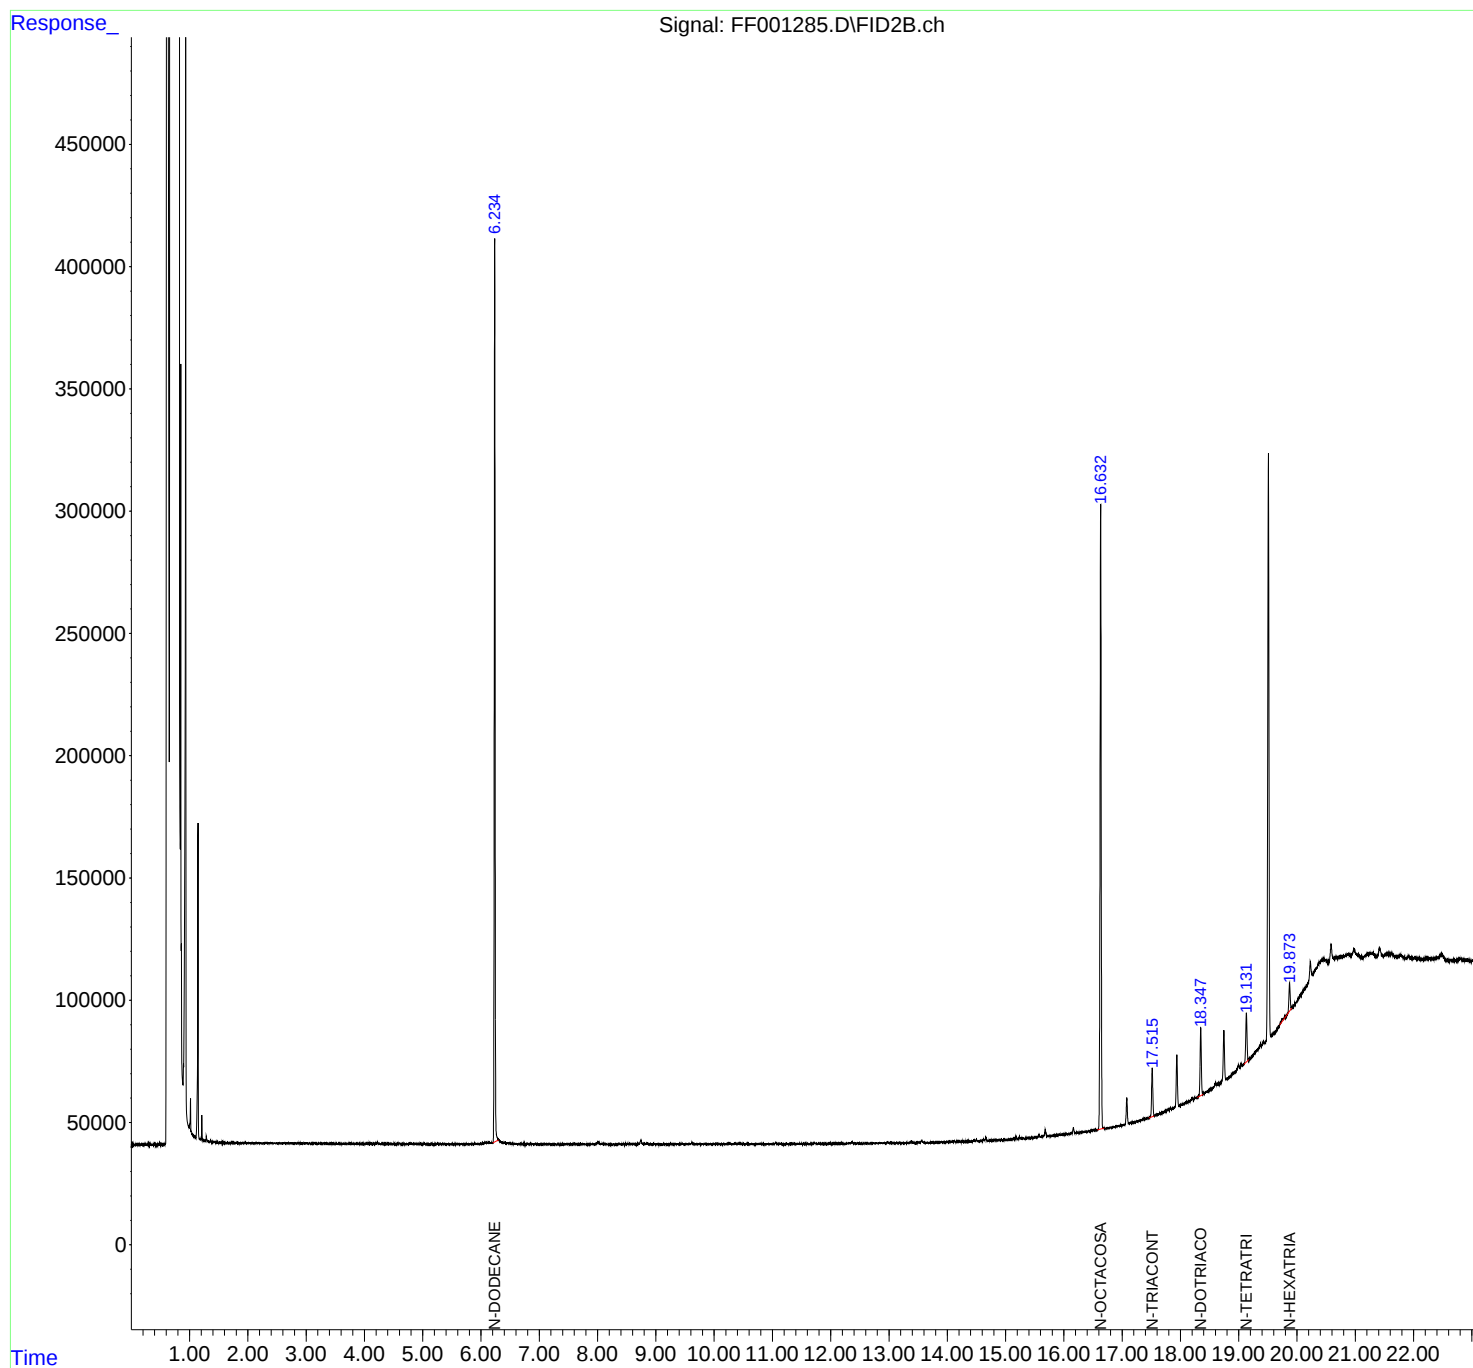


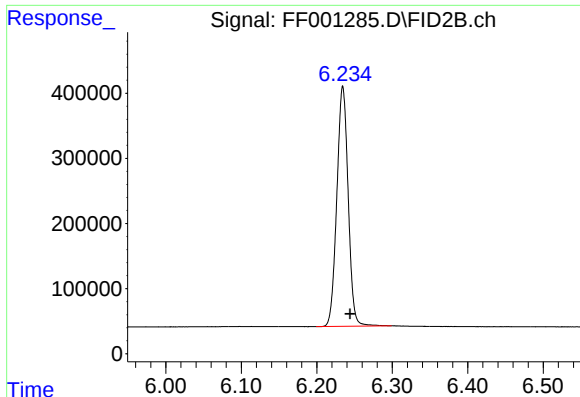

#3 N-DODECANE


R.T.: 6.234 min
Delta R.T.: -0.010 min
Response: 3852367
Conc: 30.74 ug/ml

Instrument :
FID_F
ClientSampleId :

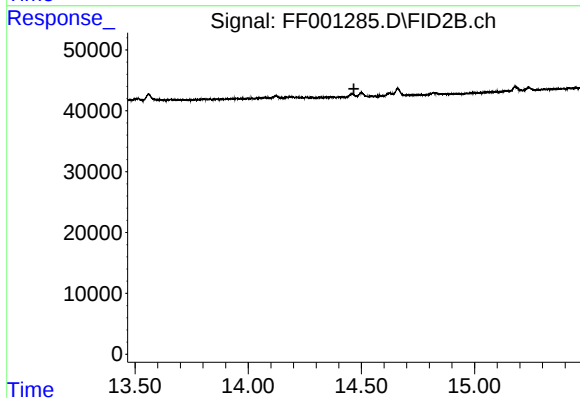


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.467 min
Response: 0
Conc: N.D.

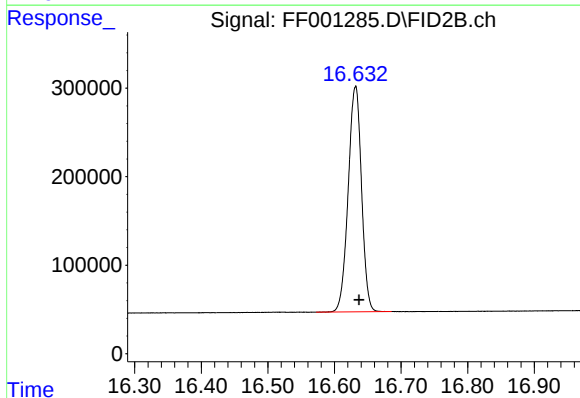


#12 N-OCTACOSANE

R.T.: 16.632 min
Delta R.T.: -0.005 min
Response: 3542103
Conc: 29.40 ug/ml

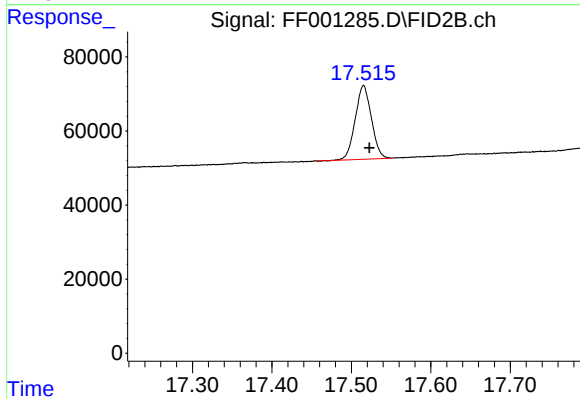

#13 N-TRIACONTANE


R.T.: 17.515 min
Delta R.T.: -0.007 min
Response: 281506
Conc: 2.34 ug/ml

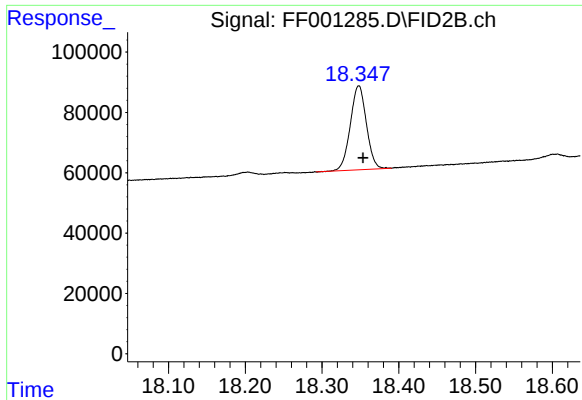

#14 N-DOTRIACONTANE


R.T.: 18.348 min
Delta R.T.: -0.005 min
Response: 406134
Conc: 3.44 ug/ml

Instrument :
FID_F
ClientSampleId :

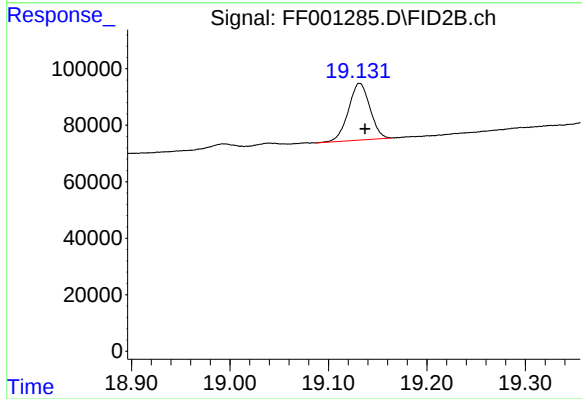

#15 N-TETRATRIACONTANE

R.T.: 19.132 min
Delta R.T.: -0.005 min
Response: 304342
Conc: 2.59 ug/ml

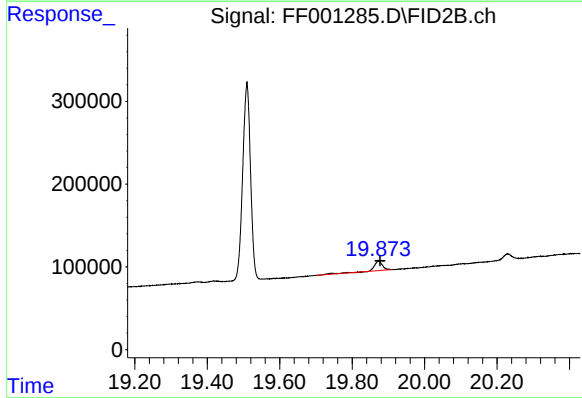

#16 N-HEXATRIACONTANE

R.T.: 19.873 min
Delta R.T.: -0.005 min
Response: 191624
Conc: 1.69 ug/ml