

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001286.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 13:23
Operator : AJ\SJ
Sample : J3926-01RE
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:36:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.458	3266912	30.327 ug/ml
Target Compounds			
4) N-TETRADECANE	8.078	2033007	16.165 ug/ml
11) N-HEXACOSANE	15.679	289113	2.385 ug/ml
12) N-OCTACOSANE	16.628	432512	3.590 ug/ml
13) N-TRIACONTANE	17.516	489750	4.074 ug/ml
14) N-DOTRIACONTANE	18.348	371441	3.150 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001286.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 13:23
Operator : AJ\SJ
Sample : J3926-01RE
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:36:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

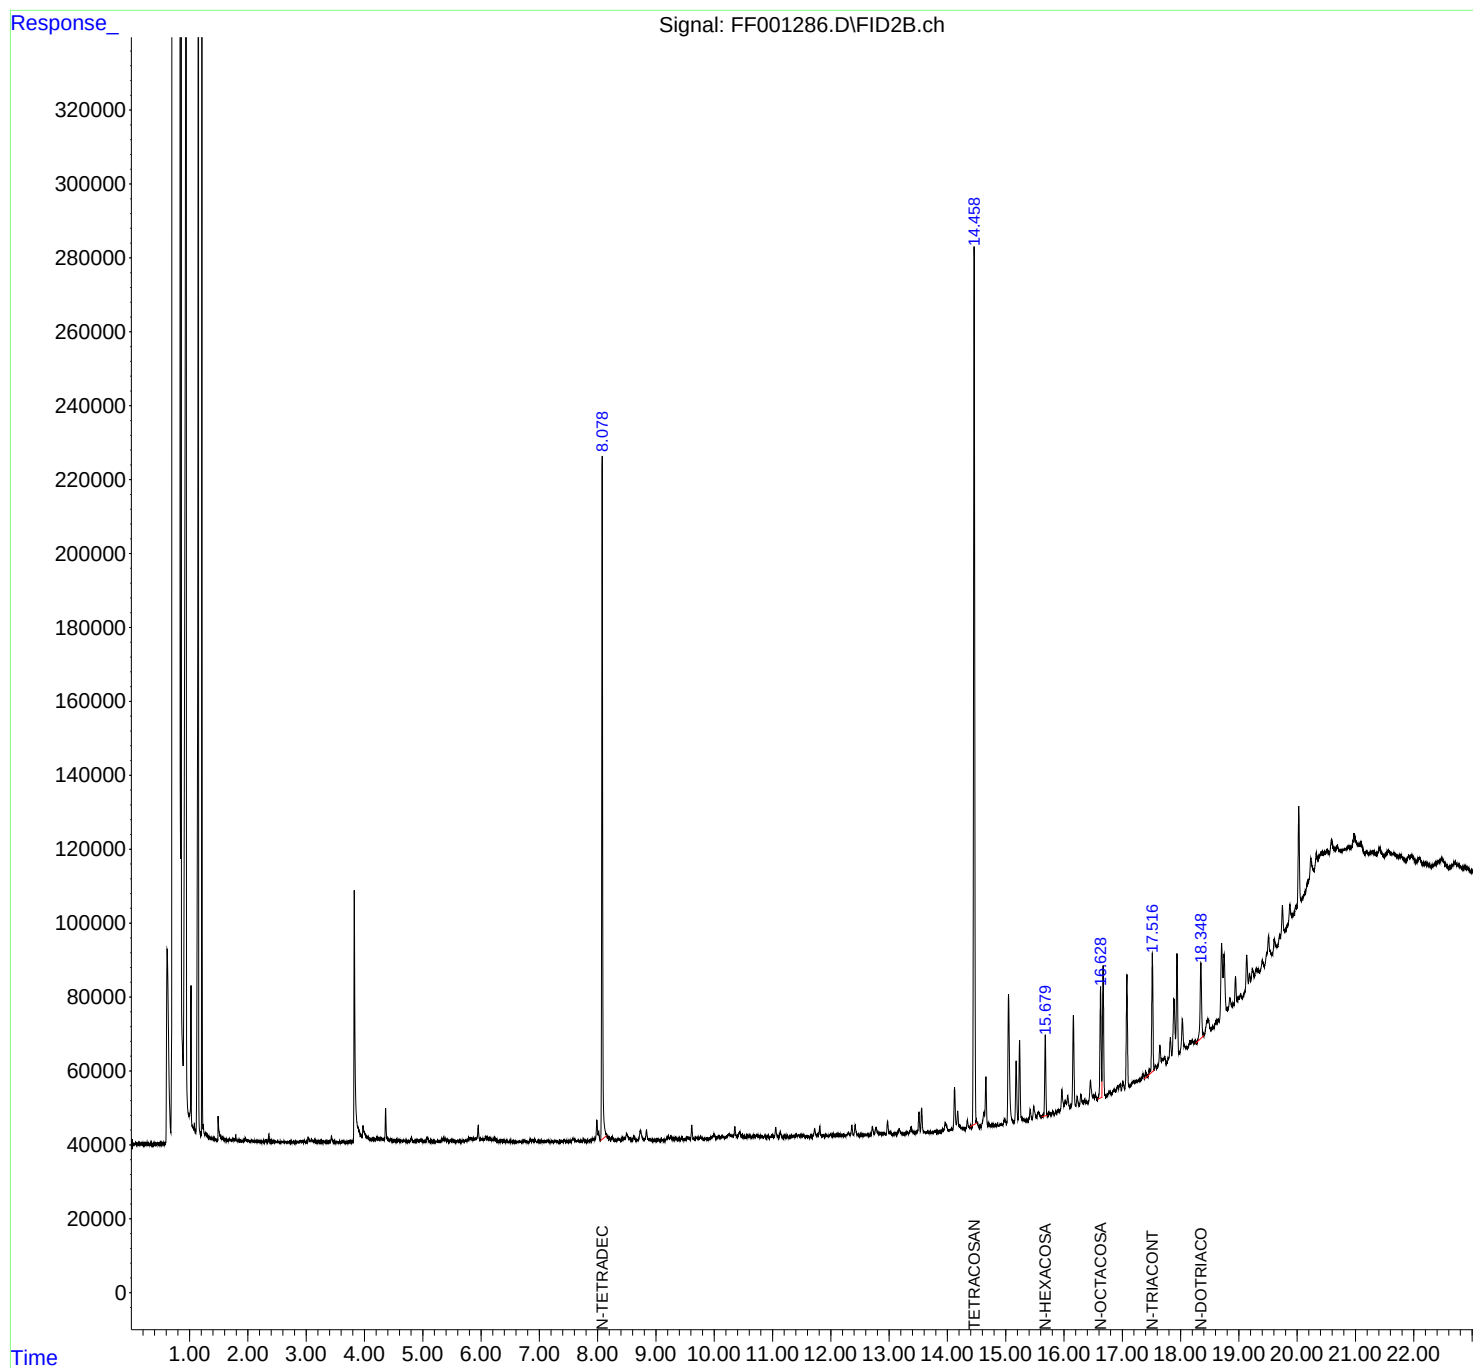


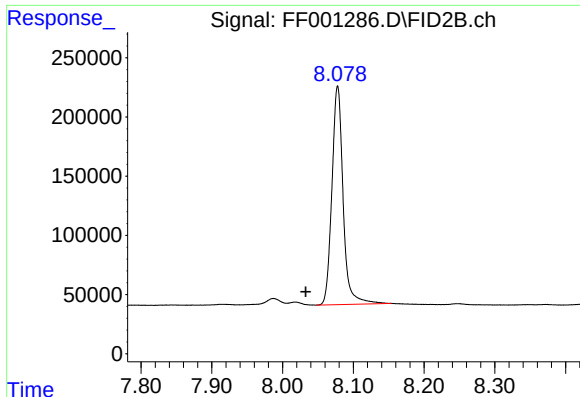

#4 N-TETRADECANE


R.T.: 8.078 min
Delta R.T.: 0.045 min
Response: 2033007
Conc: 16.16 ug/ml

Instrument :
FID_F
ClientSampleId :

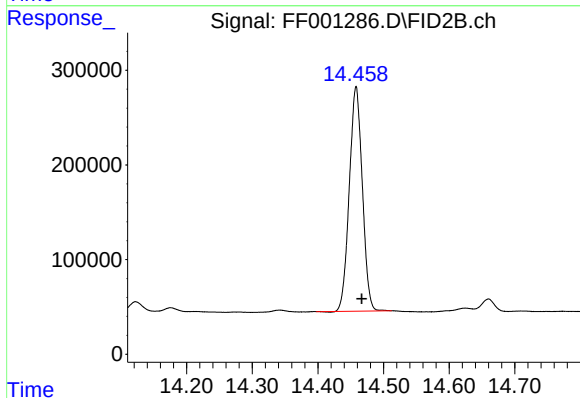


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.458 min
Delta R.T.: -0.008 min
Response: 3266912
Conc: 30.33 ug/ml

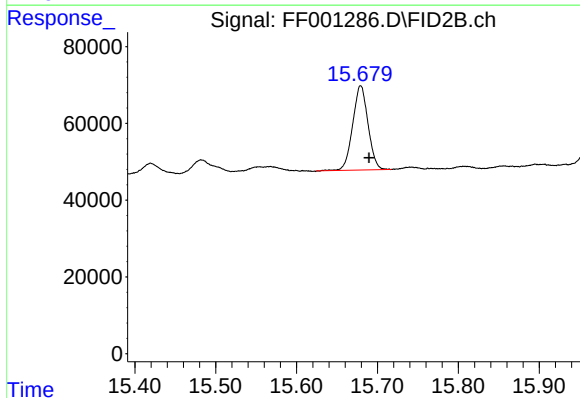


#11 N-HEXACOSANE

R.T.: 15.679 min
Delta R.T.: -0.010 min
Response: 289113
Conc: 2.39 ug/ml

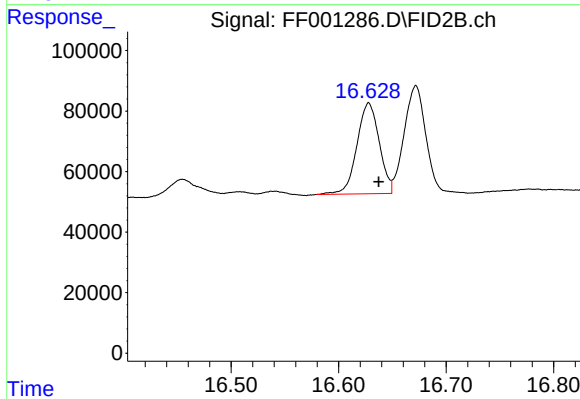

#12 N-OCTACOSANE


R.T.: 16.628 min
Delta R.T.: -0.009 min
Response: 432512
Conc: 3.59 ug/ml

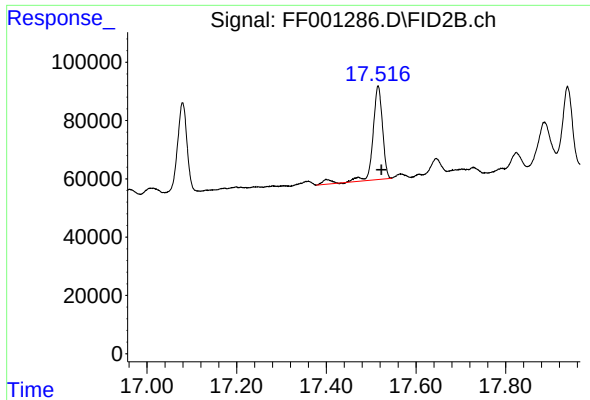

#13 N-TRIACONTANE

R.T.: 17.516 min
Delta R.T.: -0.007 min
Response: 489750
Conc: 4.07 ug/ml

Instrument :
FID_F
ClientSampleId :

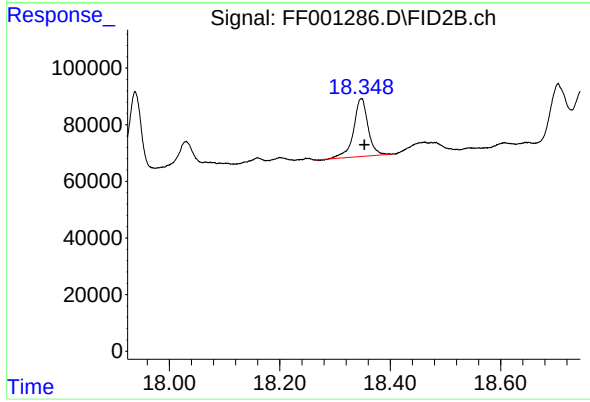

#14 N-DOTRIACONTANE

R.T.: 18.348 min
Delta R.T.: -0.006 min
Response: 371441
Conc: 3.15 ug/ml