

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001287.D
 Signal(s) : FID2B.ch
 Acq On : 12 Jul 2018 13:59
 Operator : AJ\SJ
 Sample : J3926-02RE
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 02:36:40 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.459	3221236	29.903 ug/ml
Target Compounds			
4) N-TETRADECANE	8.080	1970337	15.666 ug/ml
11) N-HEXACOSANE	15.680	283237	2.337 ug/ml
12) N-OCTACOSANE	16.629	387458	3.216 ug/ml
13) N-TRIACONTANE	17.515	464239	3.862 ug/ml
14) N-DOTRIACONTANE	18.345	383748	3.255 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001287.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 13:59
Operator : AJ\SJ
Sample : J3926-02RE
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:36:40 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

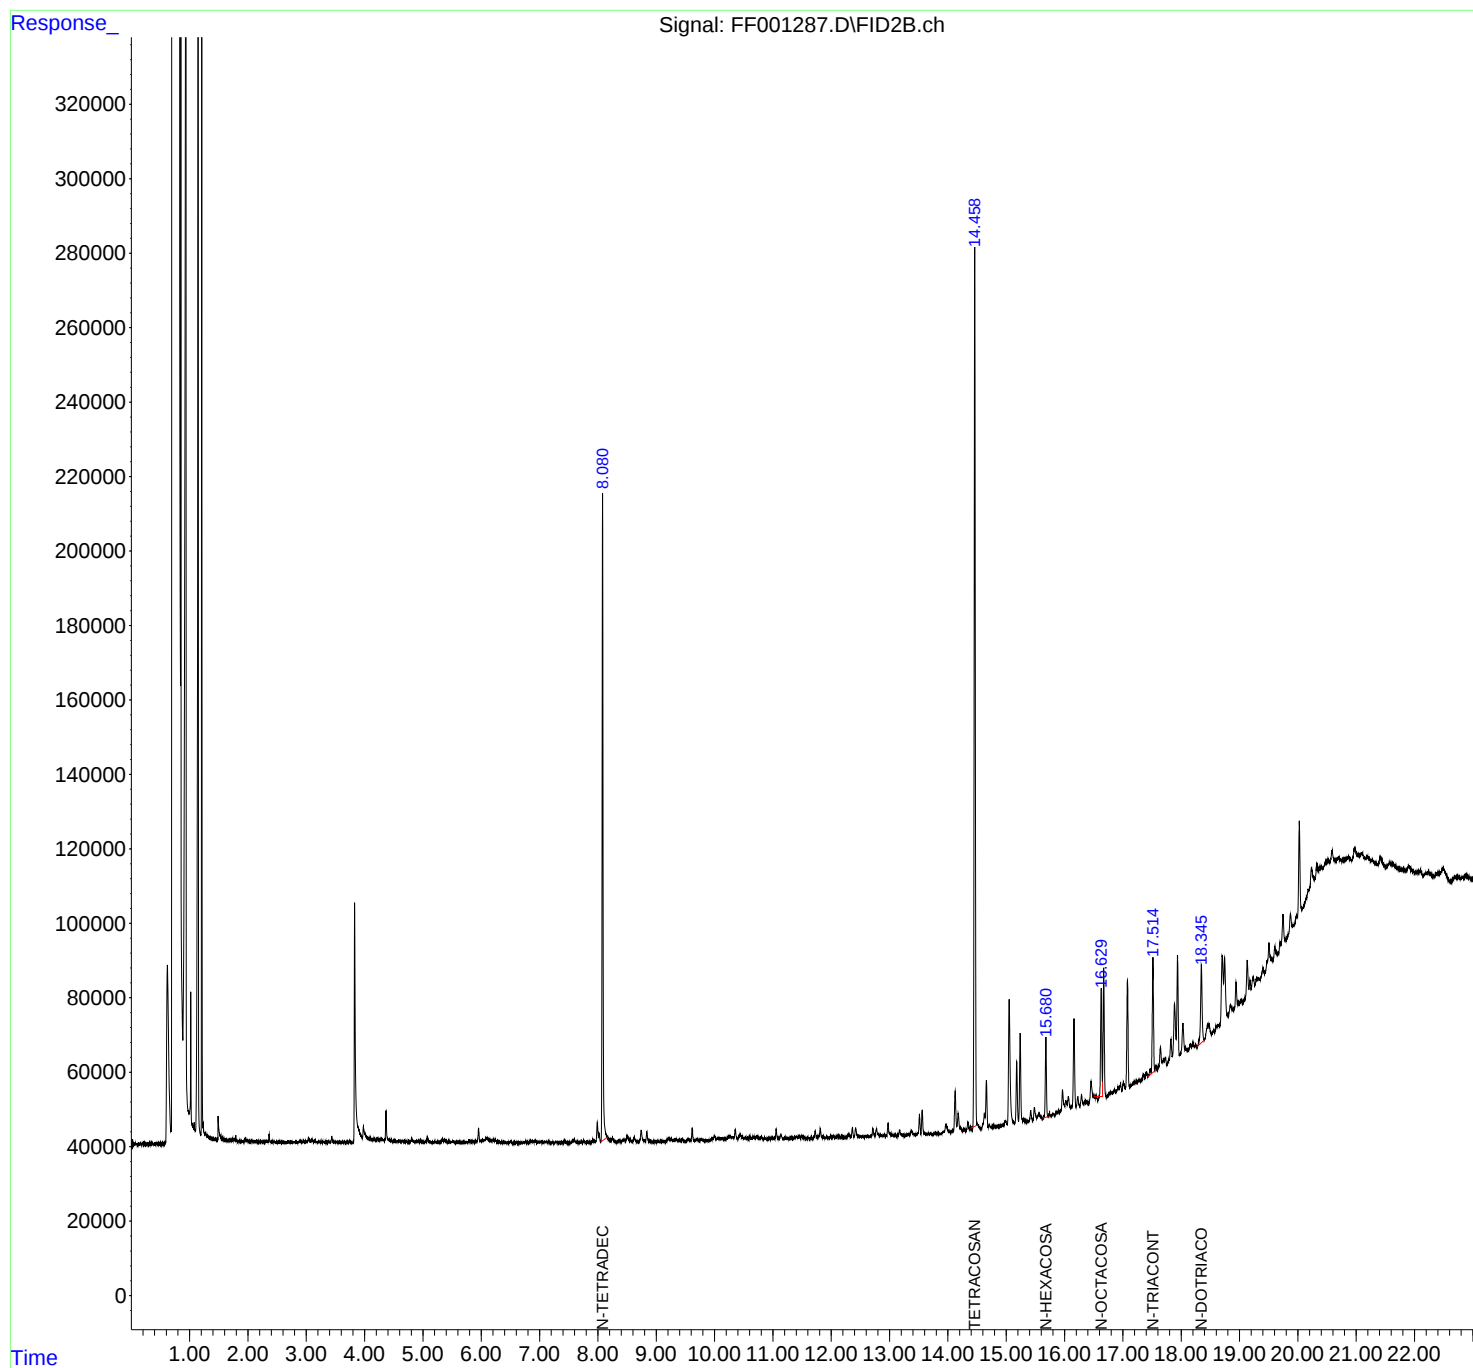


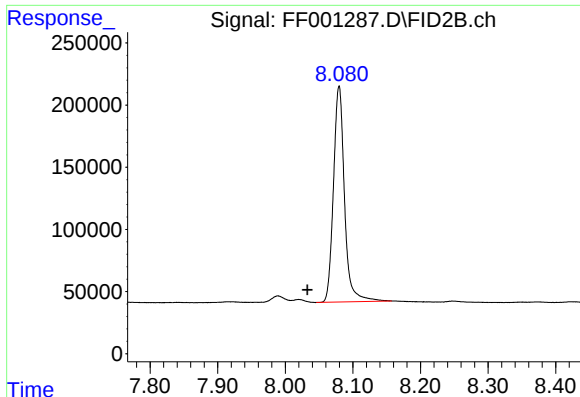

#4 N-TETRADECANE


R.T.: 8.080 min
Delta R.T.: 0.047 min
Response: 1970337
Conc: 15.67 ug/ml

Instrument :
FID_F
ClientSampleId :

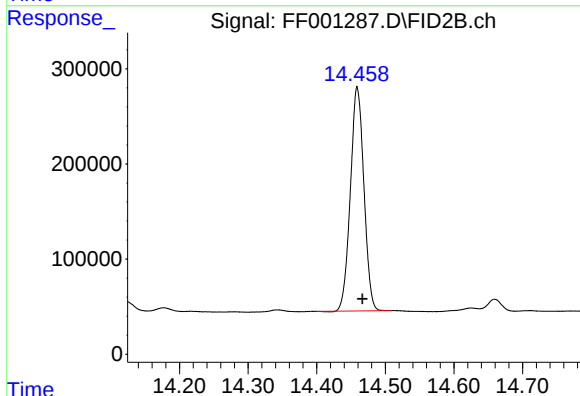


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.459 min
Delta R.T.: -0.008 min
Response: 3221236
Conc: 29.90 ug/ml

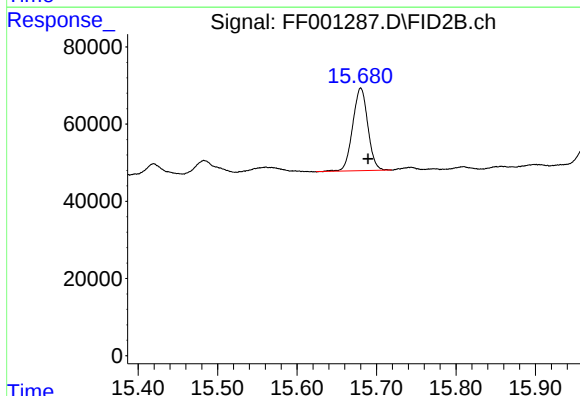


#11 N-HEXACOSANE

R.T.: 15.680 min
Delta R.T.: -0.009 min
Response: 283237
Conc: 2.34 ug/ml

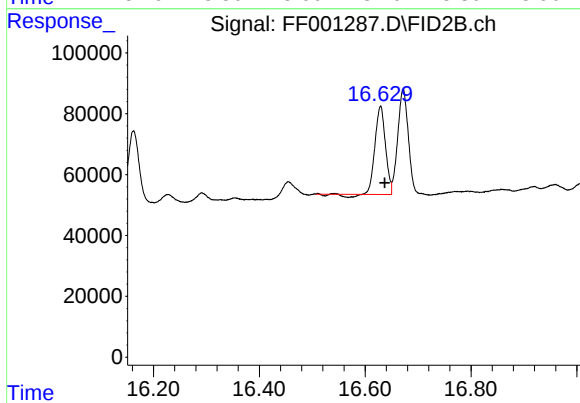

#12 N-OCTACOSANE


R.T.: 16.629 min
Delta R.T.: -0.008 min
Response: 387458
Conc: 3.22 ug/ml

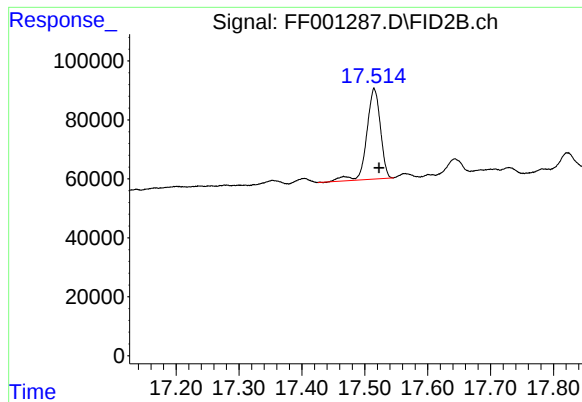

#13 N-TRIACONTANE

R.T.: 17.515 min
Delta R.T.: -0.008 min
Response: 464239
Conc: 3.86 ug/ml

Instrument :
FID_F
ClientSampleId :

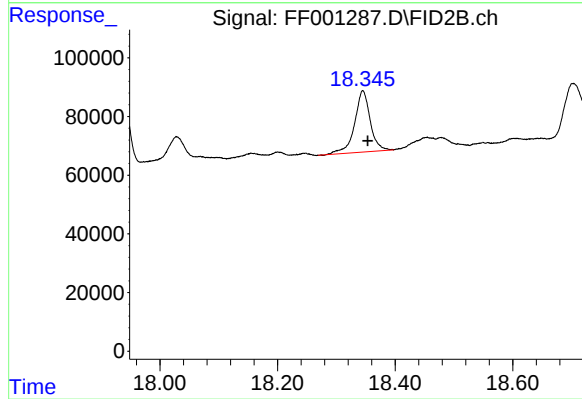

#14 N-DOTRIACONTANE

R.T.: 18.345 min
Delta R.T.: -0.008 min
Response: 383748
Conc: 3.25 ug/ml