

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001288.D
 Signal(s) : FID2B.ch
 Acq On : 12 Jul 2018 16:28
 Operator : AJ\SJ
 Sample : J3930-01 2X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 02:36:54 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.460	1016481	9.436 ug/ml
Target Compounds			
4) N-TETRADECANE	8.082	586606	4.664 ug/ml
7) N-EICOSANE	12.415	704916	5.667 ug/ml
10) N-TETRACOSANE	14.631	430450	3.531 ug/ml
11) N-HEXACOSANE	15.756f	620961	5.123 ug/ml
12) N-OCTACOSANE	16.631	525019	4.358 ug/ml
13) N-TRIACONTANE	17.518	400442	3.331 ug/ml
14) N-DOTRIACONTANE	18.347	319921	2.713 ug/ml
15) N-TETRATRIACONTANE	19.139	251257	2.138 ug/ml
16) N-HEXATRIACONTANE	19.870	97287	0.856 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001288.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 16:28
Operator : AJ\SJ
Sample : J3930-01 2X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:36:54 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

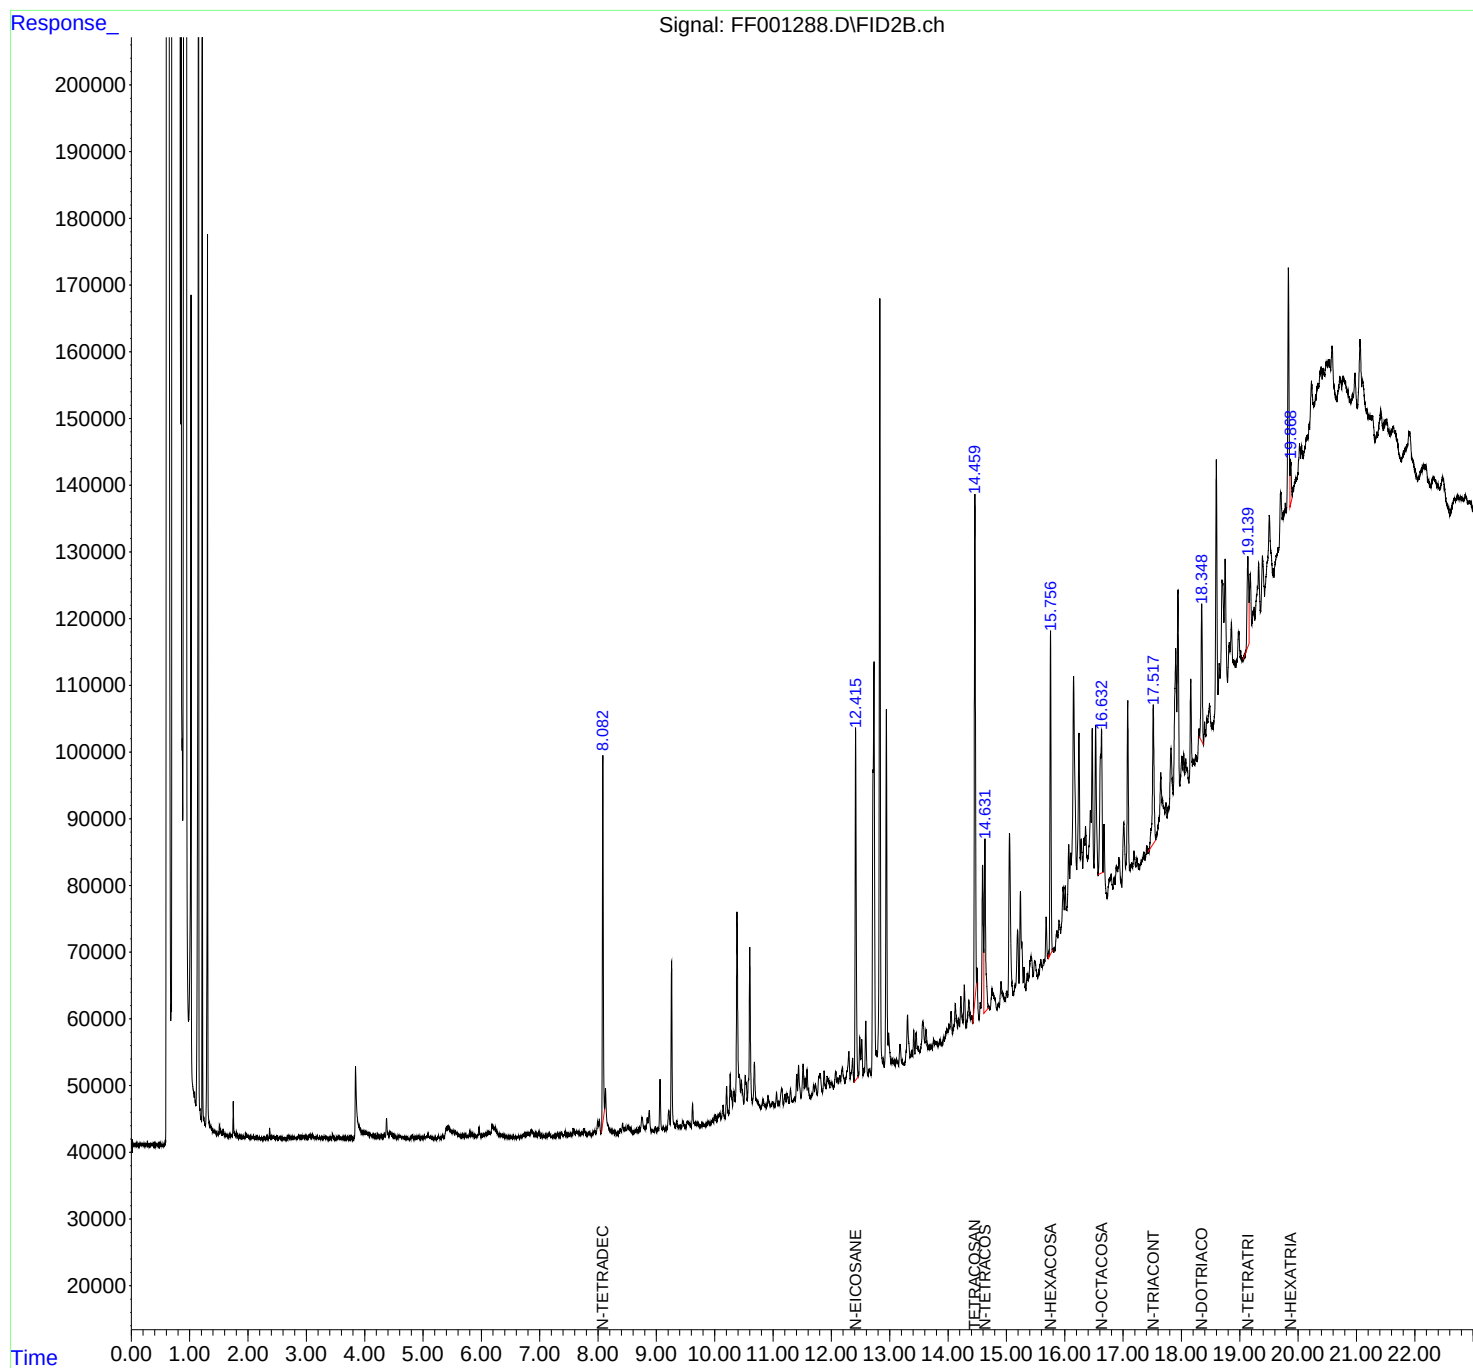


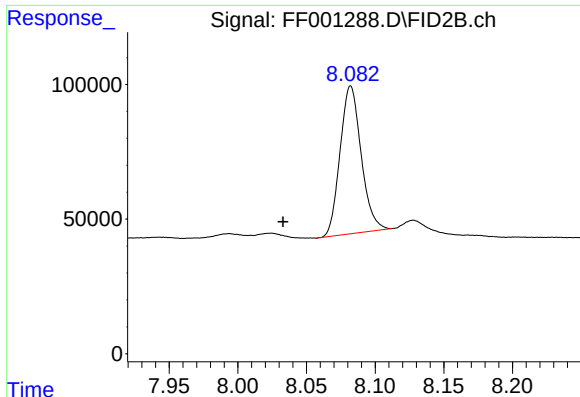

#4 N-TETRADECANE


R.T.: 8.082 min
Delta R.T.: 0.049 min
Response: 586606
Conc: 4.66 ug/ml

Instrument :
FID_F
ClientSampleId :

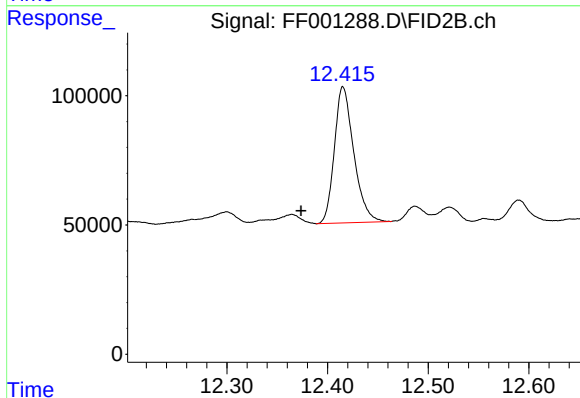


#7 N-EICOSANE

R.T.: 12.415 min
Delta R.T.: 0.042 min
Response: 704916
Conc: 5.67 ug/ml

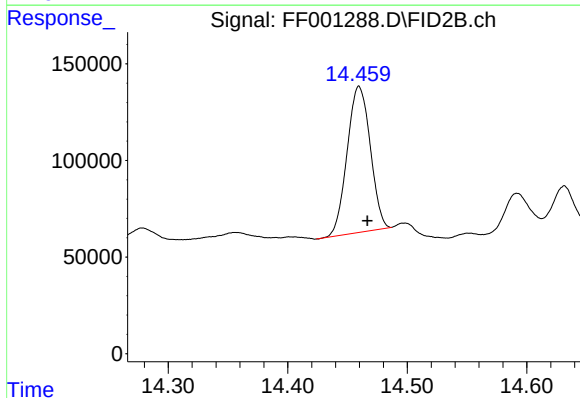


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.460 min
Delta R.T.: -0.007 min
Response: 1016481
Conc: 9.44 ug/ml

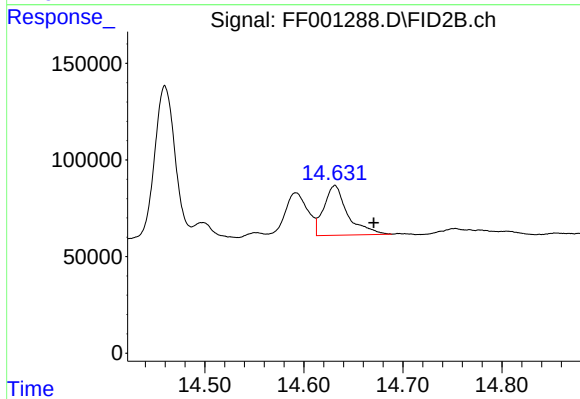

#10 N-TETRACOSANE


R.T.: 14.631 min
Delta R.T.: -0.039 min
Response: 430450
Conc: 3.53 ug/ml

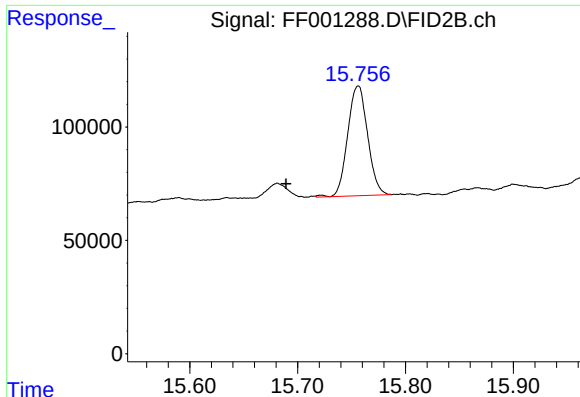

#11 N-HEXACOSANE


R.T.: 15.756 min
Delta R.T.: 0.067 min
Response: 620961
Conc: 5.12 ug/ml

Instrument :
FID_F
ClientSampleId :

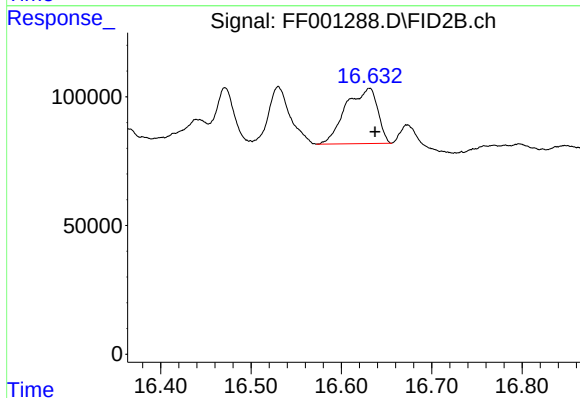


#12 N-OCTACOSANE

R.T.: 16.631 min
Delta R.T.: -0.006 min
Response: 525019
Conc: 4.36 ug/ml

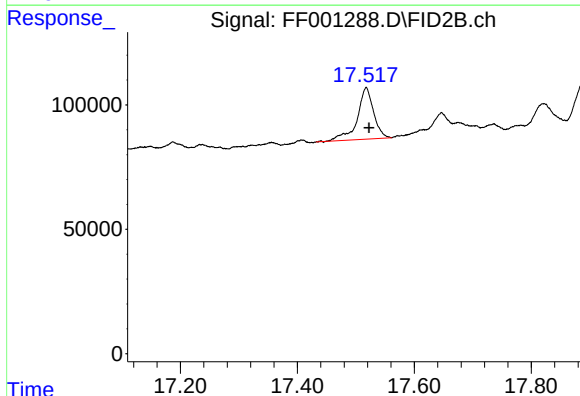


#13 N-TRIACONTANE

R.T.: 17.518 min
Delta R.T.: -0.005 min
Response: 400442
Conc: 3.33 ug/ml

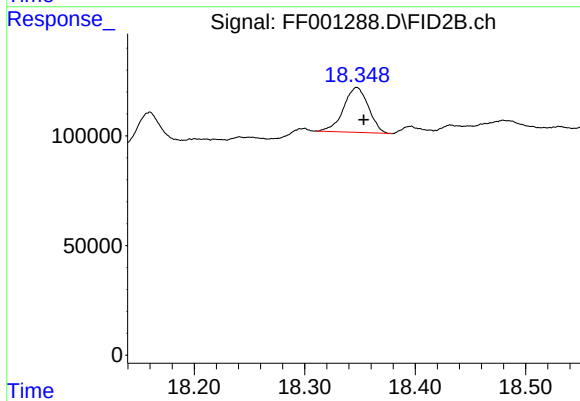

#14 N-DOTRIACONTANE


R.T.: 18.347 min
Delta R.T.: -0.006 min
Response: 319921
Conc: 2.71 ug/ml

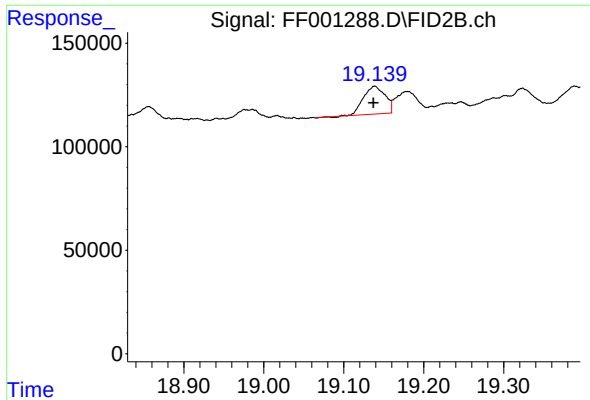

#15 N-TETRATRIACONTANE

R.T.: 19.139 min
Delta R.T.: 0.002 min
Response: 251257
Conc: 2.14 ug/ml

Instrument :
FID_F
ClientSampleId :

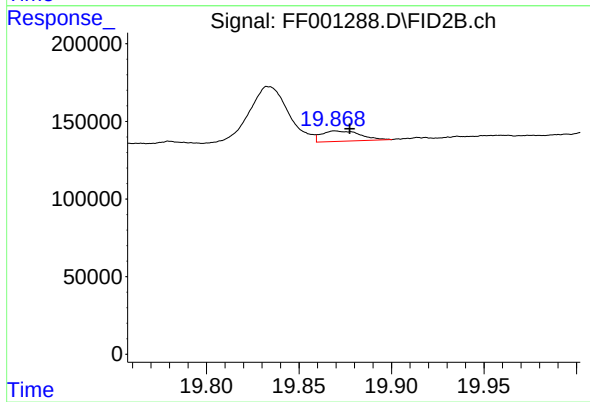

#16 N-HEXATRIACONTANE

R.T.: 19.870 min
Delta R.T.: -0.008 min
Response: 97287
Conc: 0.86 ug/ml