

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF071218\  
Data File : FF001290.D  
Signal(s) : FID2B.ch  
Acq On : 12 Jul 2018 17:29  
Operator : AJ\SJ  
Sample : J3828-03 10X  
Misc :  
ALS Vial : 59 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 13 02:37:25 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_F\Method\FF070218.M  
Quant Title :  
QLast Update : Mon Jul 02 13:42:46 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 5) N-HEXADECANE             | 9.620  | 185294   | 1.483 ug/ml |
| 6) N-OCTADECANE             | 11.059 | 168061   | 1.341 ug/ml |
| 12) N-OCTACOSANE            | 16.636 | 122116   | 1.014 ug/ml |
| 13) N-TRIACONTANE           | 17.509 | 436501   | 3.631 ug/ml |
| 15) N-TETRATRIACONTANE      | 19.137 | 225825   | 1.921 ug/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF071218\  
Data File : FF001290.D  
Signal(s) : FID2B.ch  
Acq On : 12 Jul 2018 17:29  
Operator : AJ\SJ  
Sample : J3828-03 10X  
Misc :  
ALS Vial : 59 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 13 02:37:25 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_F\Method\FF070218.M  
Quant Title :  
QLast Update : Mon Jul 02 13:42:46 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

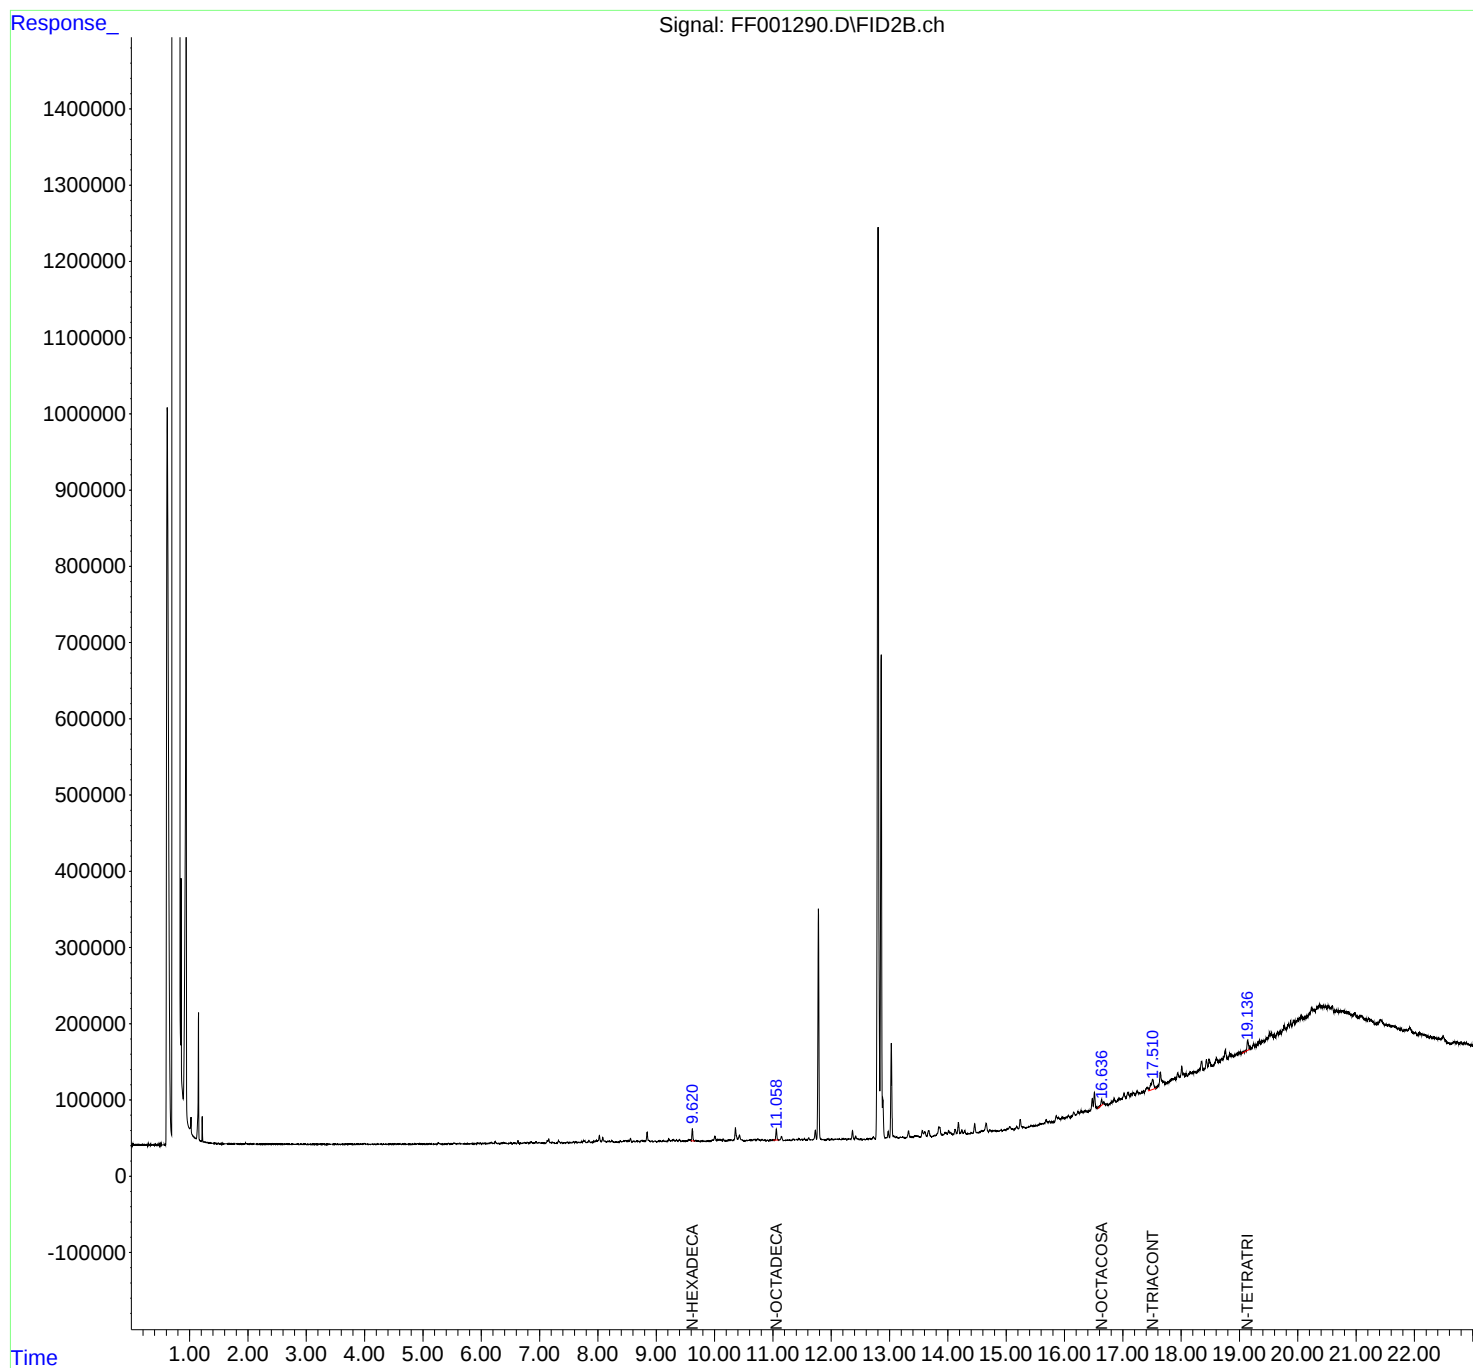


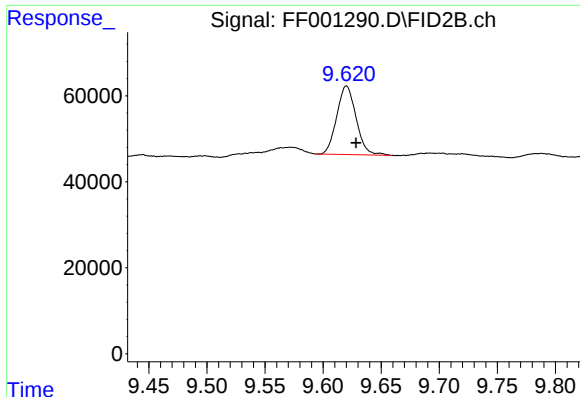

#5 N-HEXADECANE


R.T.: 9.620 min  
Delta R.T.: -0.008 min  
Response: 185294  
Conc: 1.48 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

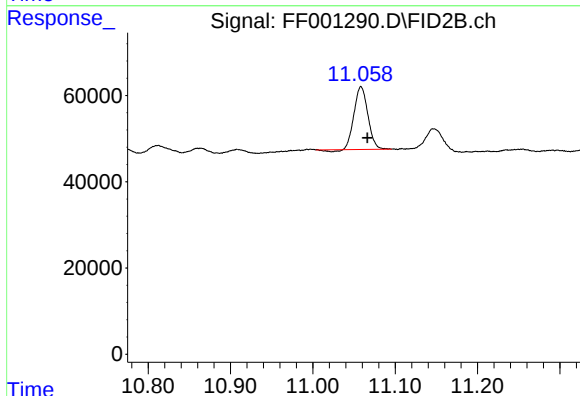


#6 N-OCTADECANE

R.T.: 11.059 min  
Delta R.T.: -0.008 min  
Response: 168061  
Conc: 1.34 ug/ml

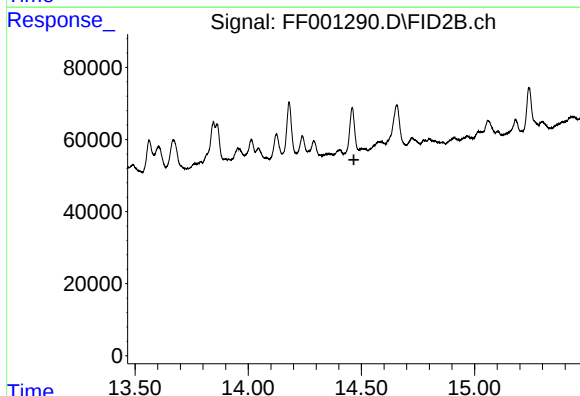


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.467 min  
Response: 0  
Conc: N.D.

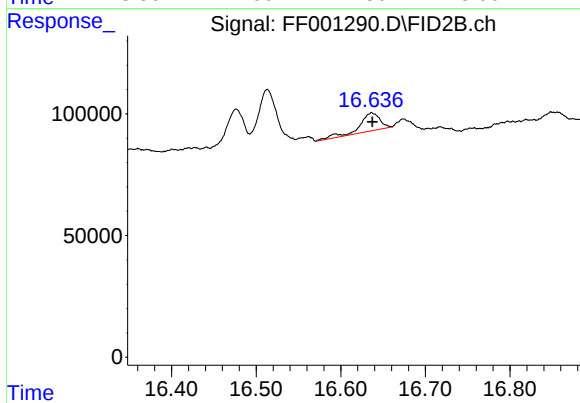

#12 N-OCTACOSANE


R.T.: 16.636 min  
Delta R.T.: 0.000 min  
Response: 122116  
Conc: 1.01 ug/ml

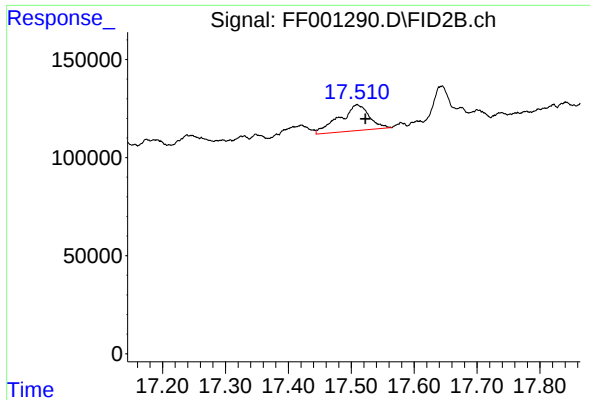

#13 N-TRIACONTANE

R.T.: 17.509 min  
Delta R.T.: -0.013 min  
Response: 436501  
Conc: 3.63 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

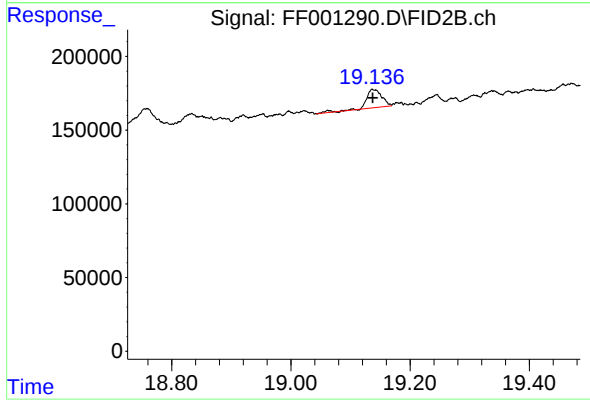

#15 N-TETRATRIACONTANE

R.T.: 19.137 min  
Delta R.T.: 0.000 min  
Response: 225825  
Conc: 1.92 ug/ml