

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001292.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 18:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:37:53 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.460	2570351	23.861 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.345	233035	1.976 ug/ml
15) N-TETRATRIACONTANE	19.129	112136	0.954 ug/ml
16) N-HEXATRIACONTANE	19.870	417961	3.679 ug/ml
17) N-OCTATRIACONTANE	20.582	97075	0.940 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001292.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 18:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:37:53 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

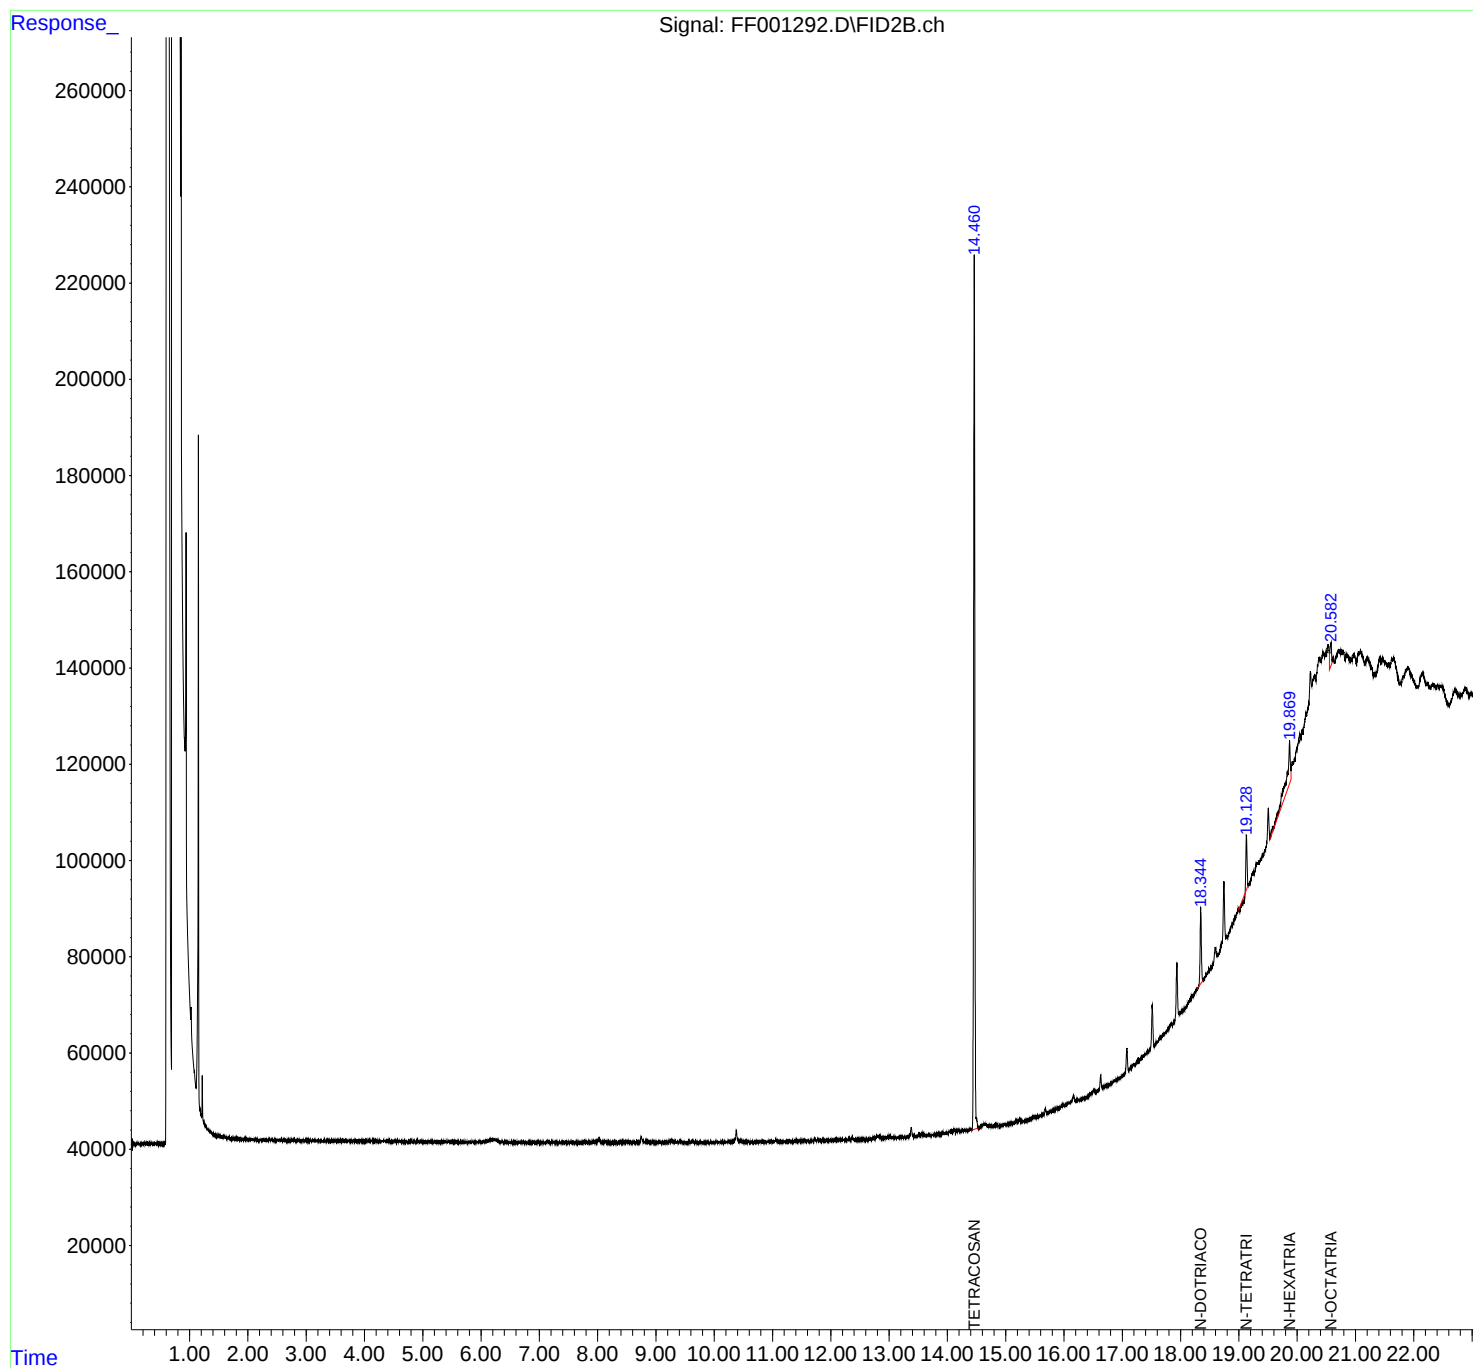


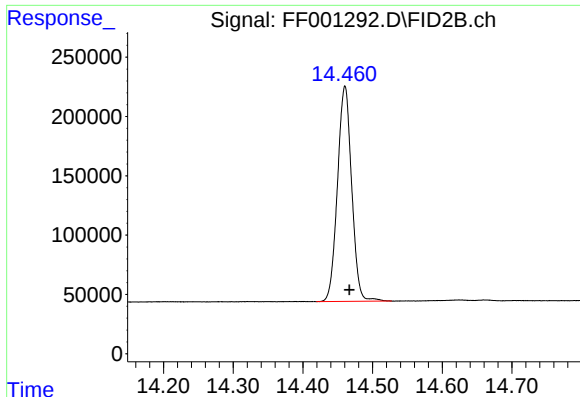

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.460 min
Delta R.T.: -0.006 min
Response: 2570351
Conc: 23.86 ug/ml

Instrument :
FID_F
ClientSampleId :

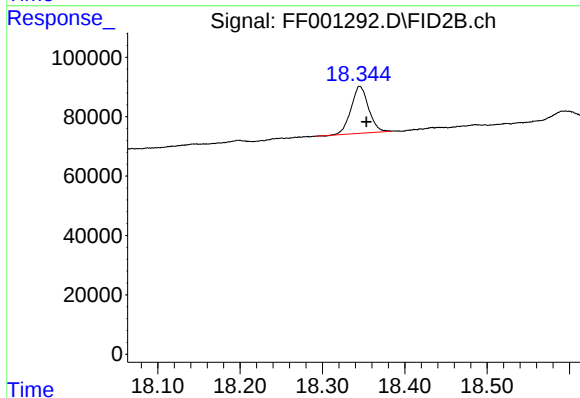


#14 N-DOTRIACONTANE

R.T.: 18.345 min
Delta R.T.: -0.008 min
Response: 233035
Conc: 1.98 ug/ml

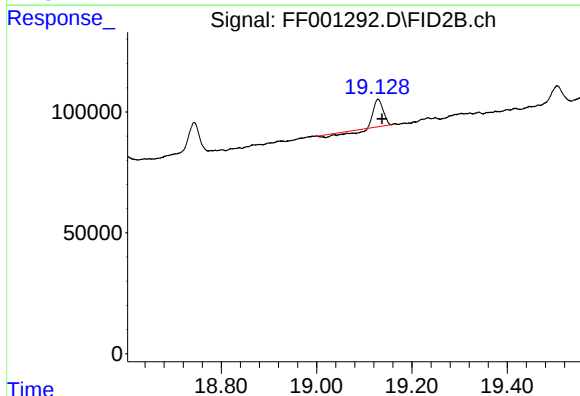


#15 N-TETRATRIACONTANE

R.T.: 19.129 min
Delta R.T.: -0.008 min
Response: 112136
Conc: 0.95 ug/ml

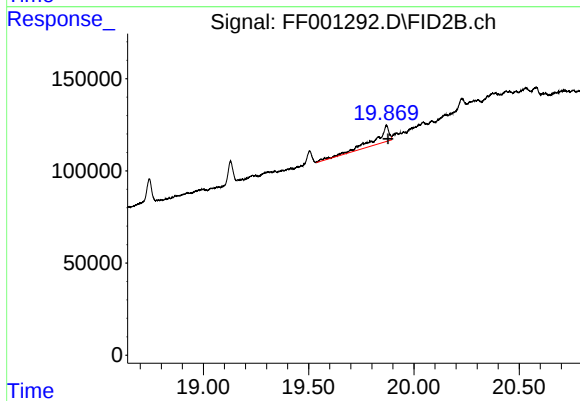

#16 N-HEXATRIACONTANE

R.T.: 19.870 min
Delta R.T.: -0.008 min
Response: 417961
Conc: 3.68 ug/ml

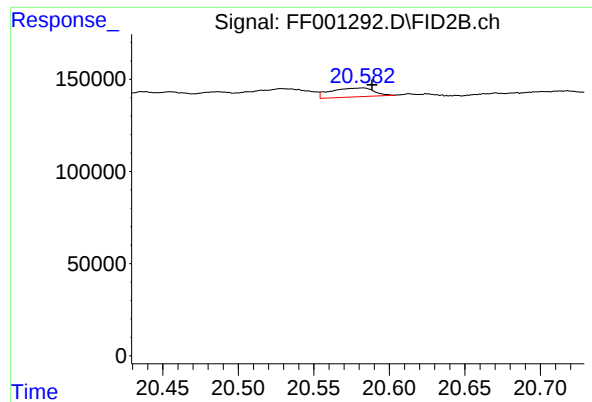

#17 N-OCTATRIACONTANE

R.T.: 20.582 min
Delta R.T.: -0.006 min
Response: 97075
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :