

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001297.D
 Signal(s) : FID2B.ch
 Acq On : 12 Jul 2018 20:59
 Operator : AJ\SJ
 Sample : J3927-02 2X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 02:39:10 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.458	1137112	10.556 ug/ml
Target Compounds			
4) N-TETRADECANE	8.081	507288	4.034 ug/ml
7) N-EICOSANE	12.413	782994	6.295 ug/ml
10) N-TETRACOSANE	14.629	564876	4.634 ug/ml
12) N-OCTACOSANE	16.630	366425	3.042 ug/ml
13) N-TRIACONTANE	17.515	516986	4.301 ug/ml
14) N-DOTRIACONTANE	18.344	460875	3.909 ug/ml
15) N-TETRATRIACONTANE	19.132	230115	1.958 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001297.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2018 20:59
Operator : AJ\SJ
Sample : J3927-02 2X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 02:39:10 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

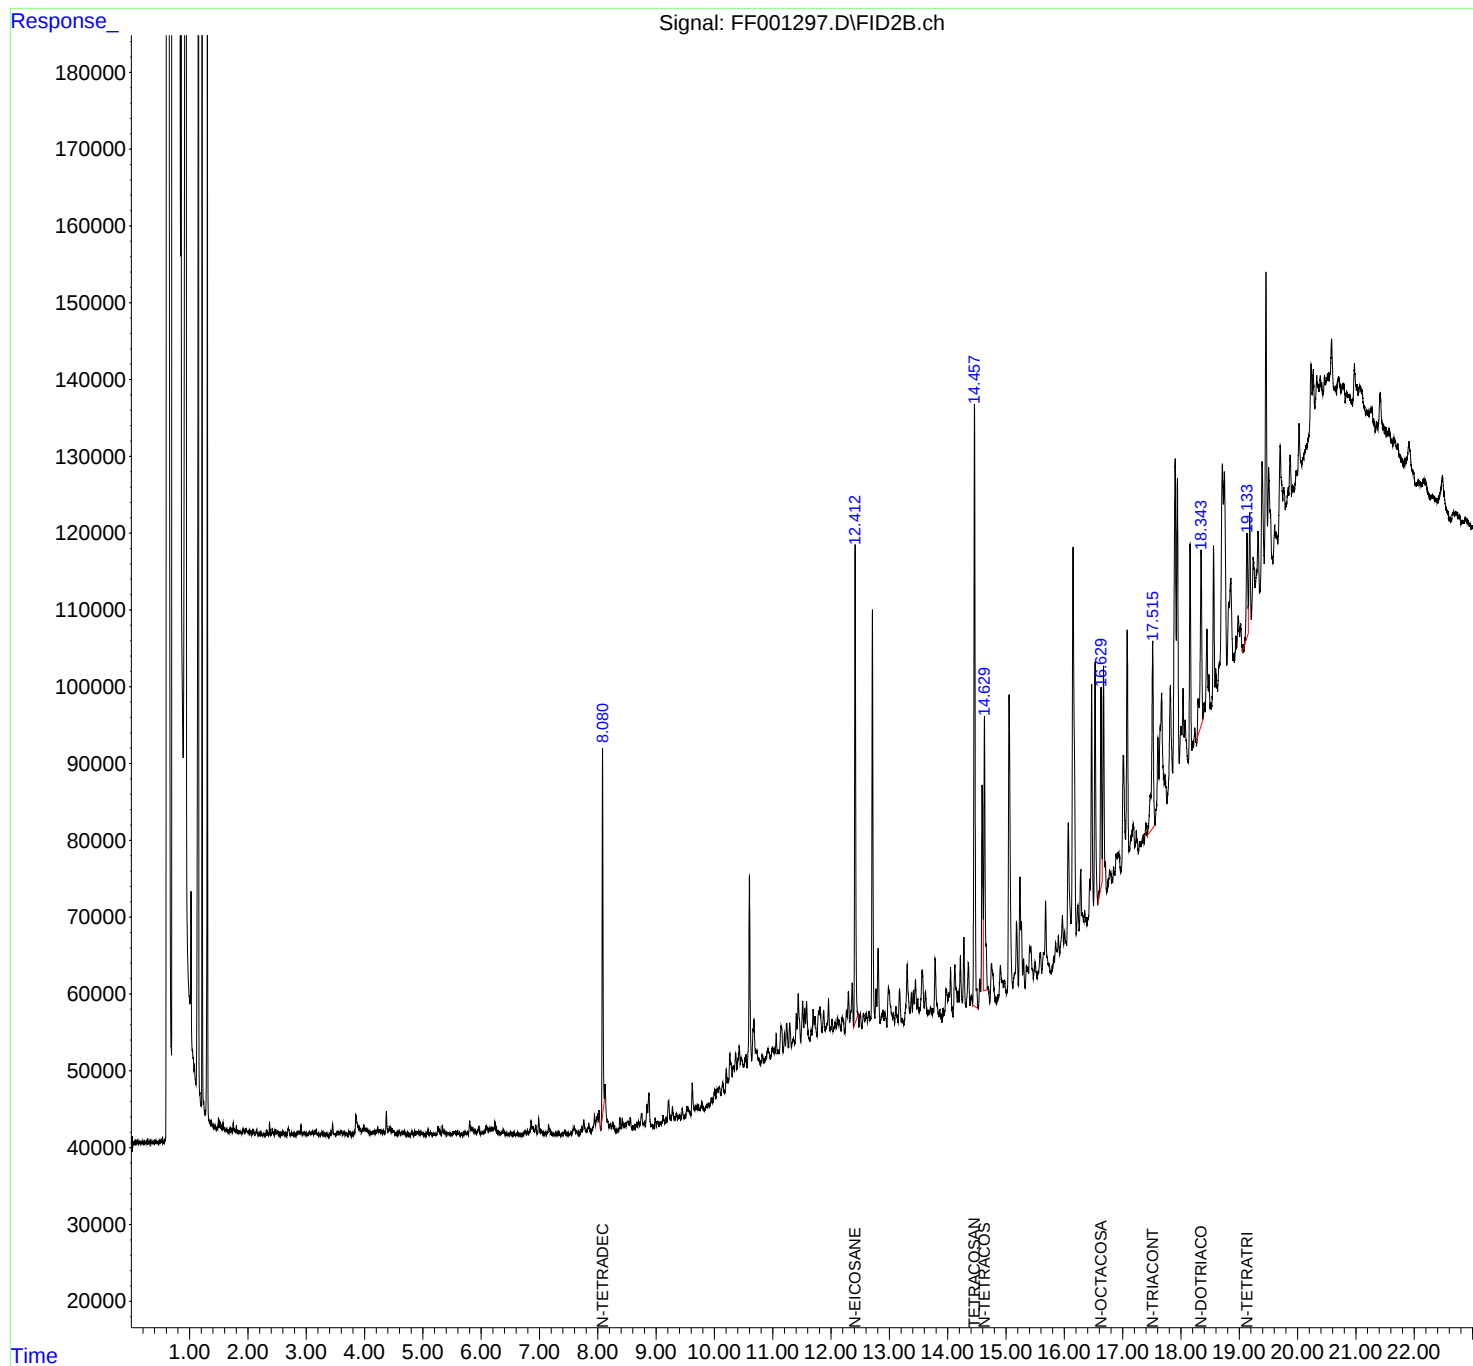


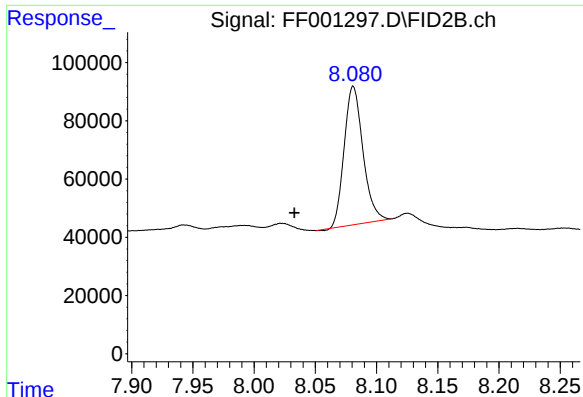

#4 N-TETRADECANE


R.T.: 8.081 min
Delta R.T.: 0.048 min
Response: 507288
Conc: 4.03 ug/ml

Instrument :
FID_F
ClientSampleId :

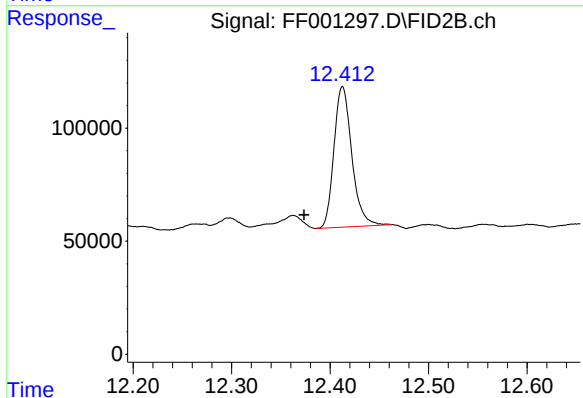


#7 N-EICOSANE

R.T.: 12.413 min
Delta R.T.: 0.039 min
Response: 782994
Conc: 6.29 ug/ml

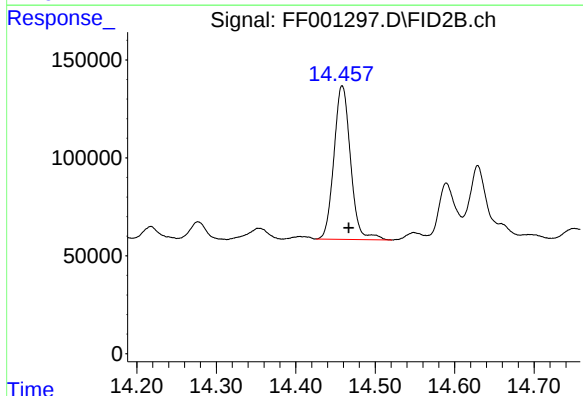


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.458 min
Delta R.T.: -0.008 min
Response: 1137112
Conc: 10.56 ug/ml

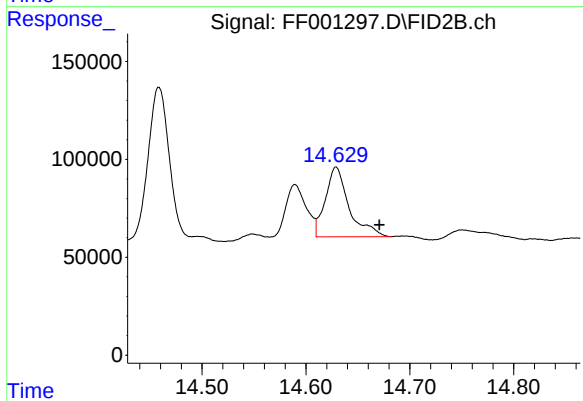

#10 N-TETRACOSANE


R.T.: 14.629 min
Delta R.T.: -0.042 min
Response: 564876
Conc: 4.63 ug/ml

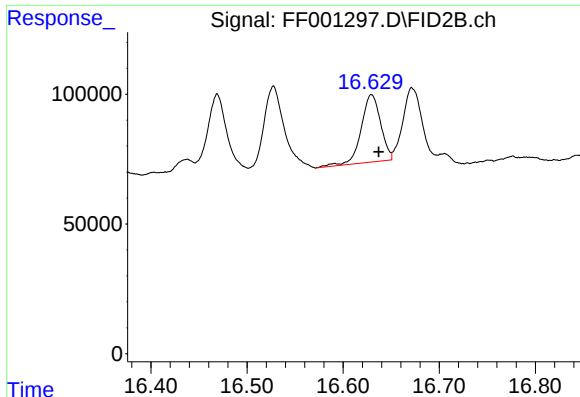

#12 N-OCTACOSANE


R.T.: 16.630 min
Delta R.T.: -0.008 min
Response: 366425
Conc: 3.04 ug/ml

Instrument :
FID_F
ClientSampleId :

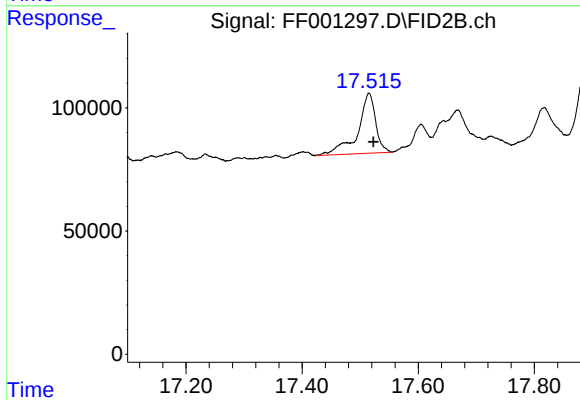


#13 N-TRIACONTANE

R.T.: 17.515 min
Delta R.T.: -0.008 min
Response: 516986
Conc: 4.30 ug/ml

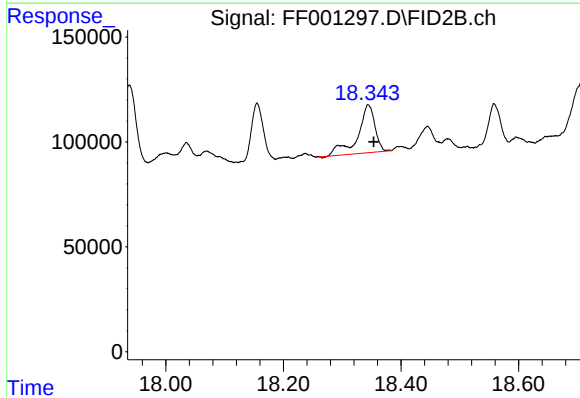

#14 N-DOTRIACONTANE

R.T.: 18.344 min
Delta R.T.: -0.009 min
Response: 460875
Conc: 3.91 ug/ml

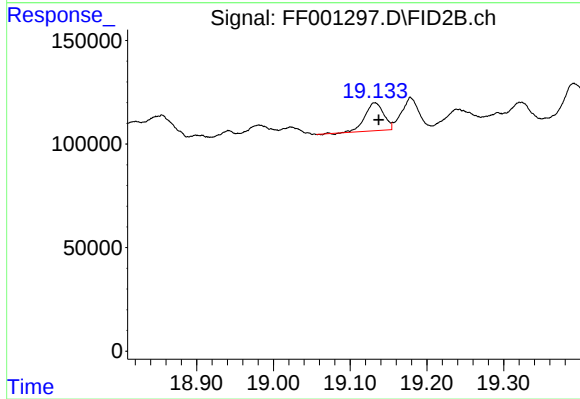

#15 N-TETRATRIACONTANE

R.T.: 19.132 min
Delta R.T.: -0.005 min
Response: 230115
Conc: 1.96 ug/ml