

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001308.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 02:28
 Operator : AJ\SJ
 Sample : J3947-01
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 05:28:09 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.459	2339788	21.720 ug/ml
Target Compounds			
4) N-TETRADECANE	8.082	1622054	12.897 ug/ml
10) N-TETRACOSANE	14.659	190268	1.561 ug/ml
11) N-HEXACOSANE	15.678	264089	2.179 ug/ml
12) N-OCTACOSANE	16.627	313836	2.605 ug/ml
13) N-TRIACONTANE	17.512	400320	3.330 ug/ml
14) N-DOTRIACONTANE	18.342	377769	3.204 ug/ml
18) N-TETRACONTANE	21.407	370526	3.618 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001308.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 02:28
Operator : AJ\SJ
Sample : J3947-01
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 05:28:09 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

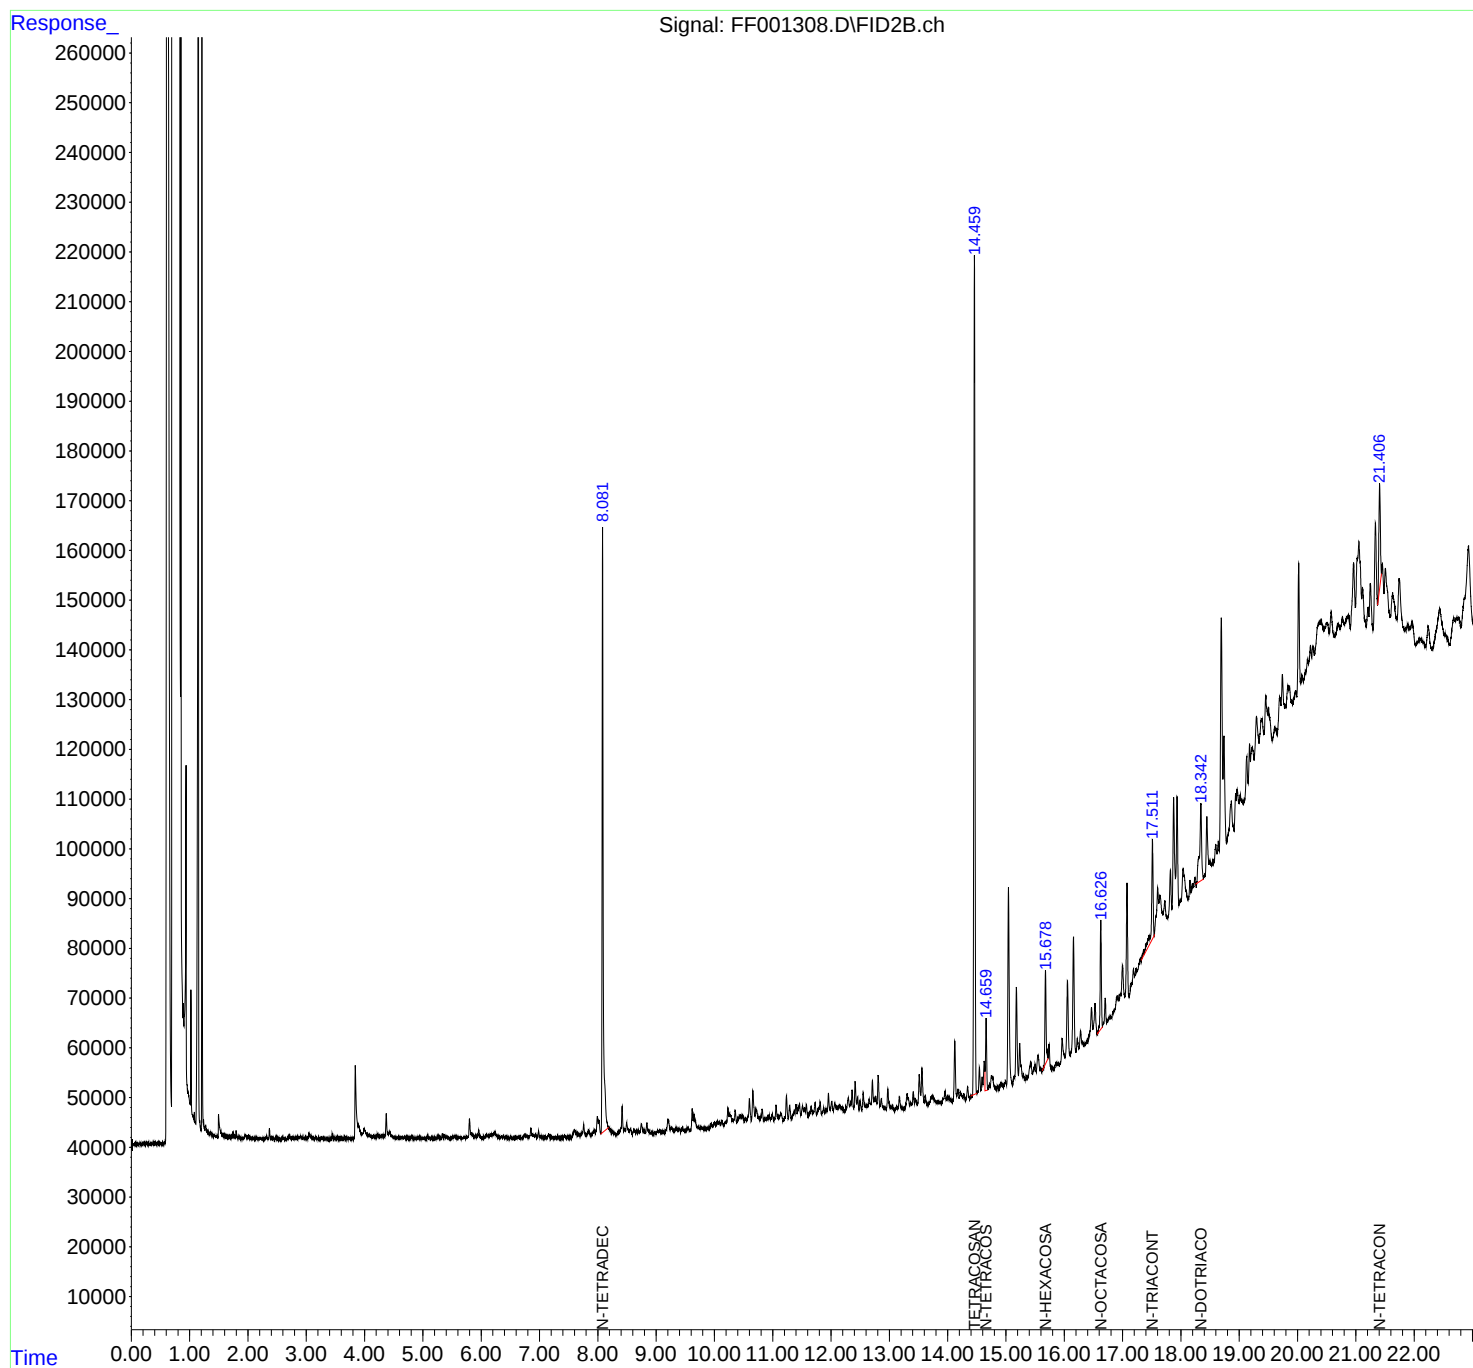


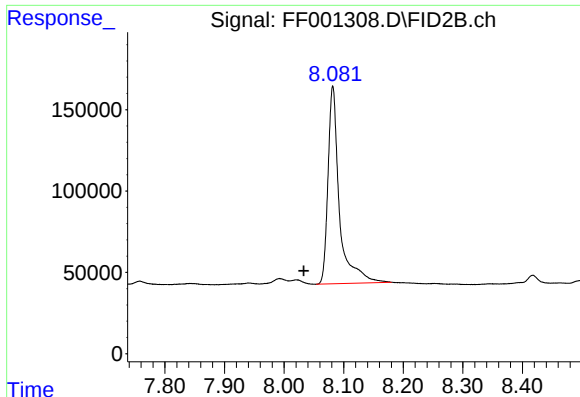

#4 N-TETRADECANE


R.T.: 8.082 min
Delta R.T.: 0.049 min
Response: 1622054
Conc: 12.90 ug/ml

Instrument :
FID_F
ClientSampleId :

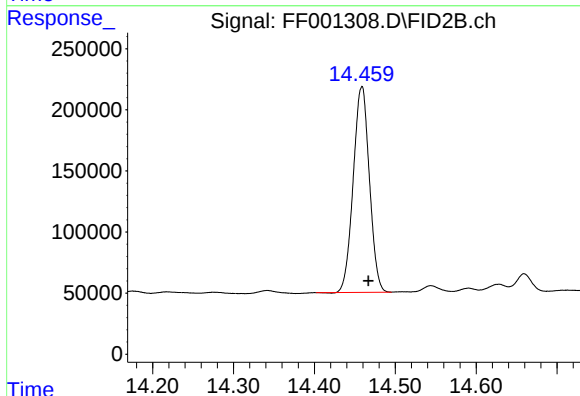


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.459 min
Delta R.T.: -0.008 min
Response: 2339788
Conc: 21.72 ug/ml

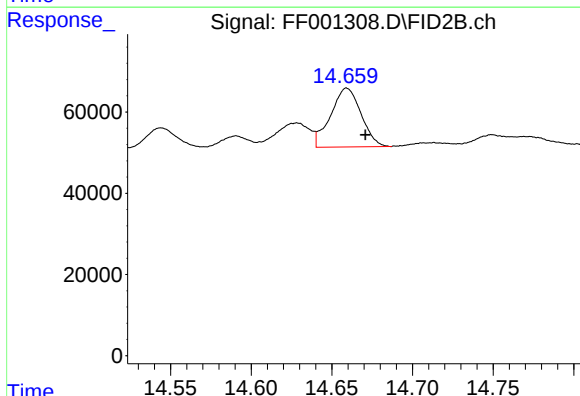


#10 N-TETRACOSANE

R.T.: 14.659 min
Delta R.T.: -0.011 min
Response: 190268
Conc: 1.56 ug/ml

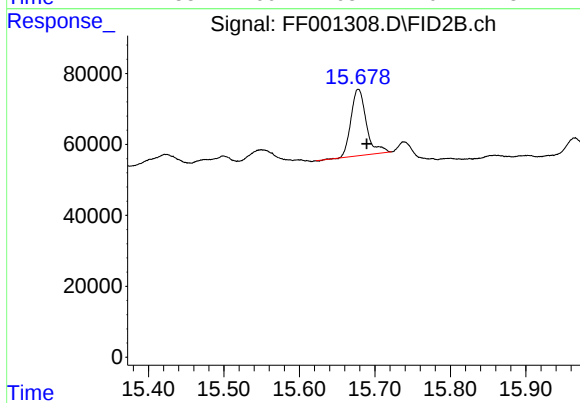

#11 N-HEXACOSANE


R.T.: 15.678 min
Delta R.T.: -0.011 min
Response: 264089
Conc: 2.18 ug/ml

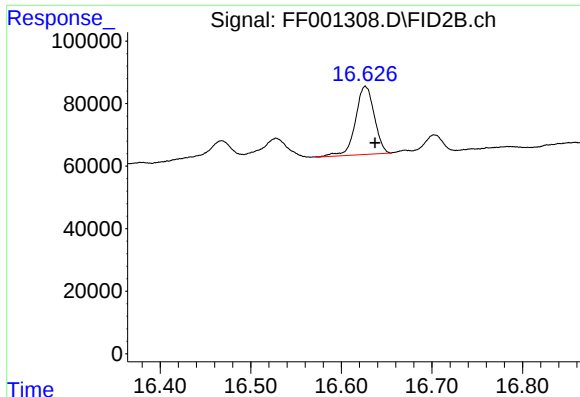

#12 N-OCTACOSANE


R.T.: 16.627 min
Delta R.T.: -0.011 min
Response: 313836
Conc: 2.61 ug/ml

Instrument :
FID_F
ClientSampleId :

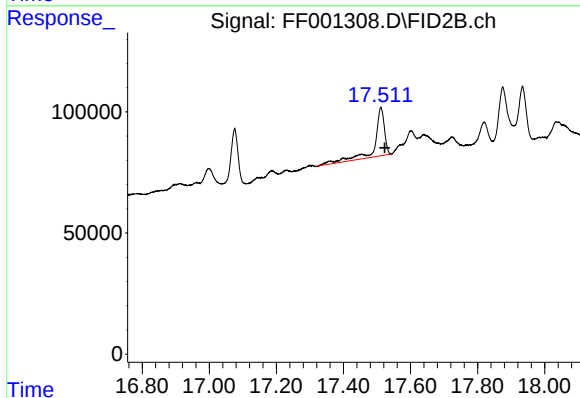


#13 N-TRIACONTANE

R.T.: 17.512 min
Delta R.T.: -0.011 min
Response: 400320
Conc: 3.33 ug/ml

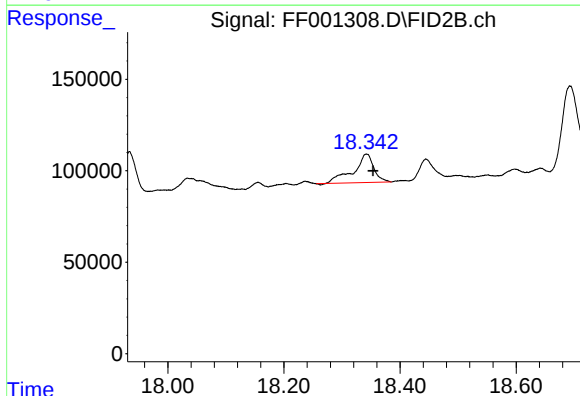

#14 N-DOTRIACONTANE

R.T.: 18.342 min
Delta R.T.: -0.011 min
Response: 377769
Conc: 3.20 ug/ml

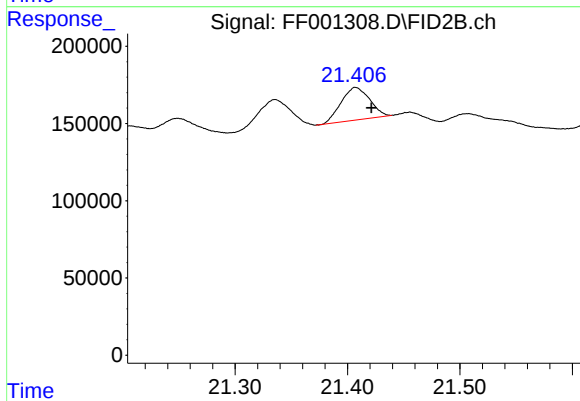

#18 N-TETRACONTANE

R.T.: 21.407 min
Delta R.T.: -0.014 min
Response: 370526
Conc: 3.62 ug/ml