

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001309.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 02:58
 Operator : AJ\SJ
 Sample : J3947-02
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 05:28:40 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	2321968	21.555 ug/ml
Target Compounds			
4) N-TETRADECANE	8.082	1594888	12.681 ug/ml
11) N-HEXACOSANE	15.678	242135	1.998 ug/ml
12) N-OCTACOSANE	16.625	304419	2.527 ug/ml
13) N-TRIACONTANE	17.512	264059	2.197 ug/ml
14) N-DOTRIACONTANE	18.342	336349	2.853 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001309.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 02:58
Operator : AJ\SJ
Sample : J3947-02
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 05:28:40 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

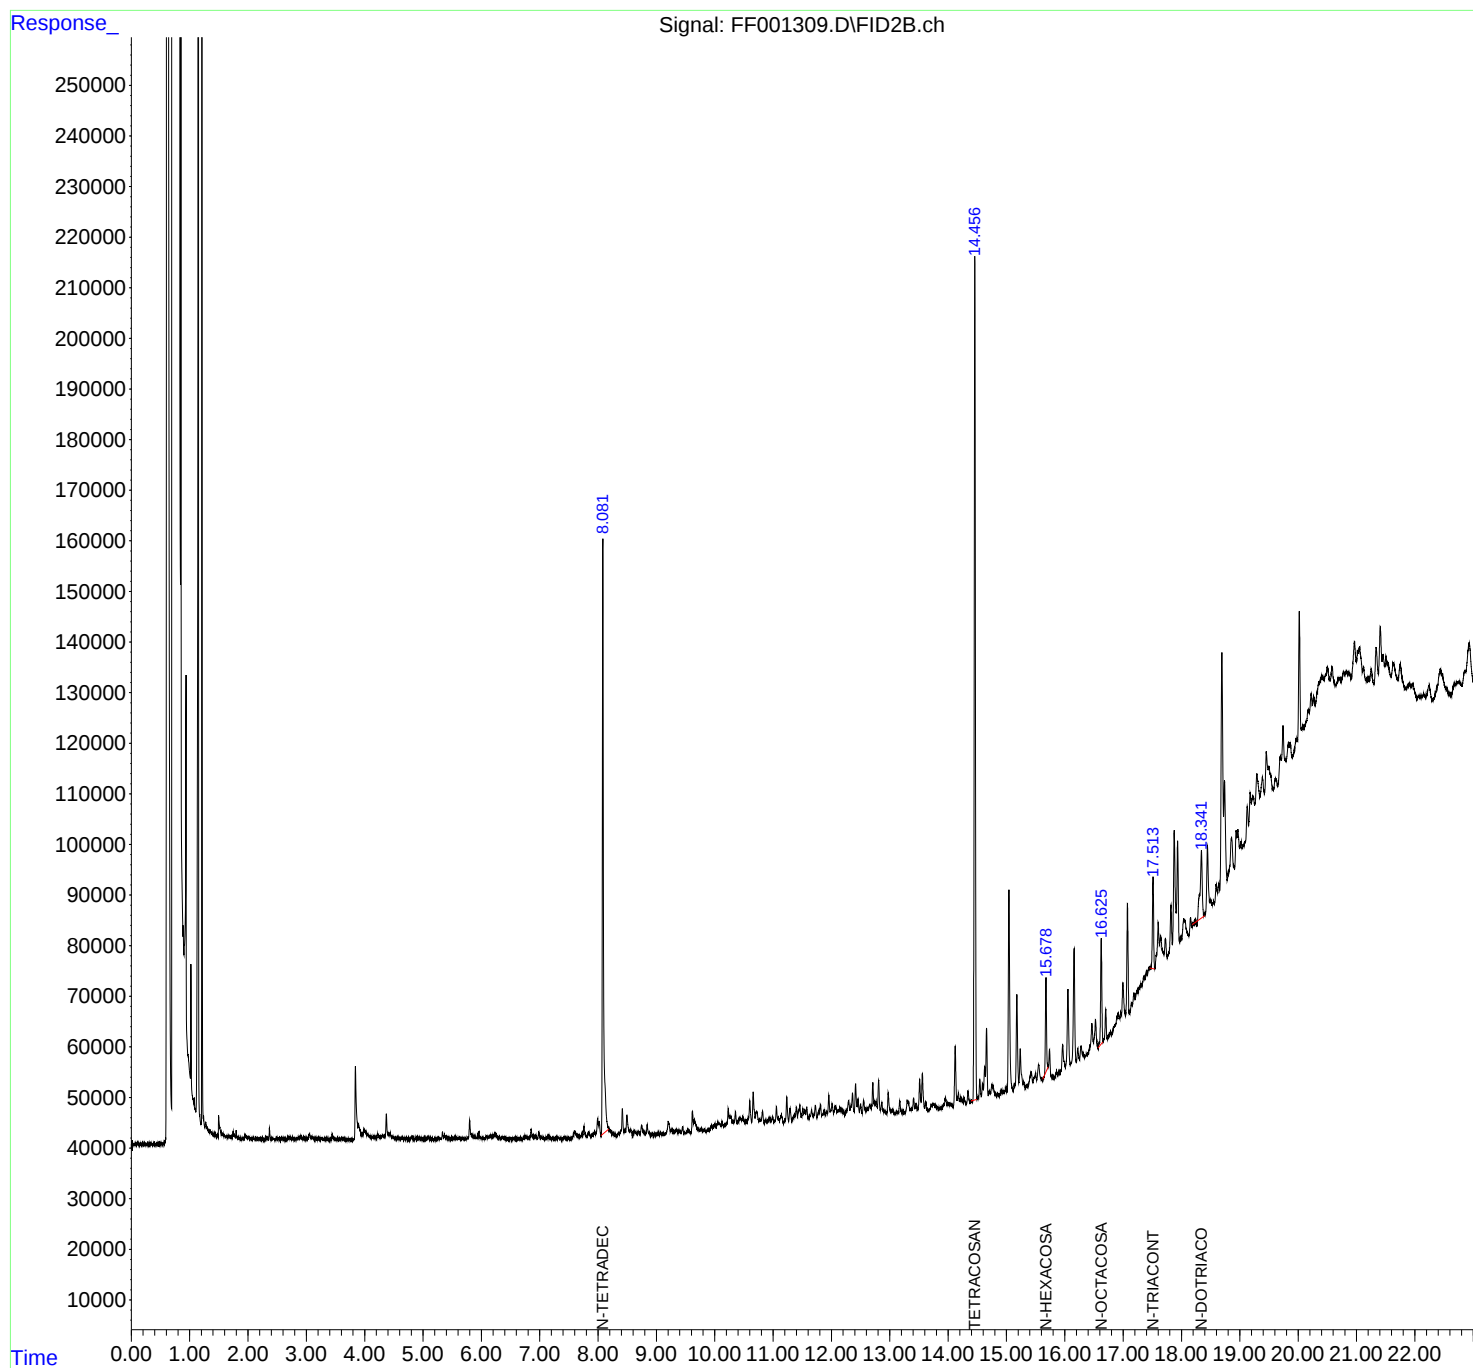


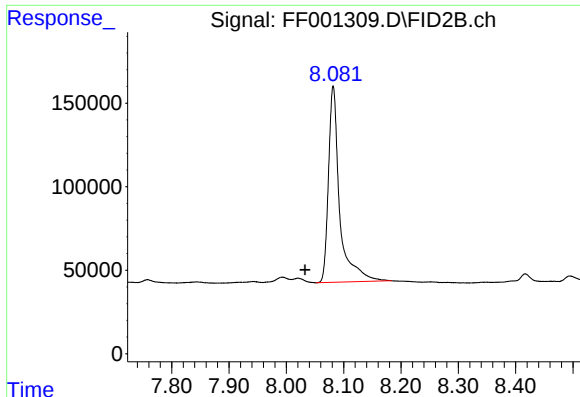

#4 N-TETRADECANE


R.T.: 8.082 min
Delta R.T.: 0.049 min
Response: 1594888
Conc: 12.68 ug/ml

Instrument :
FID_F
ClientSampleId :

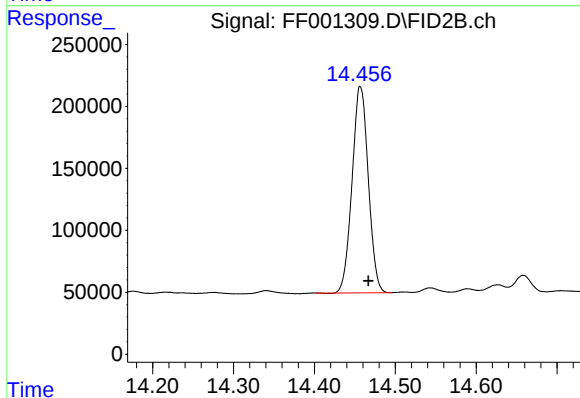


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.457 min
Delta R.T.: -0.010 min
Response: 2321968
Conc: 21.55 ug/ml

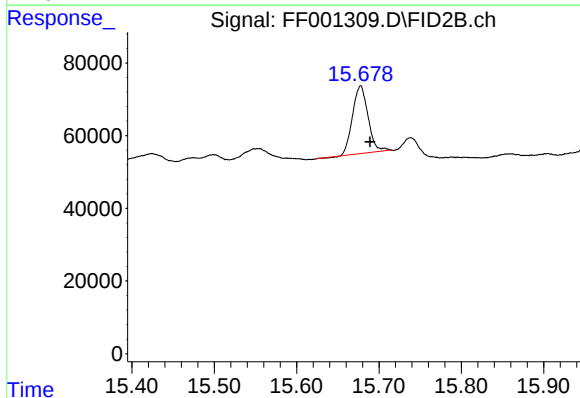


#11 N-HEXACOSANE

R.T.: 15.678 min
Delta R.T.: -0.012 min
Response: 242135
Conc: 2.00 ug/ml

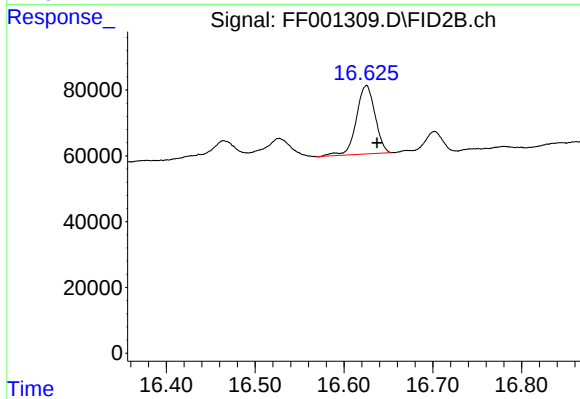

#12 N-OCTACOSANE


R.T.: 16.625 min
Delta R.T.: -0.012 min
Response: 304419
Conc: 2.53 ug/ml

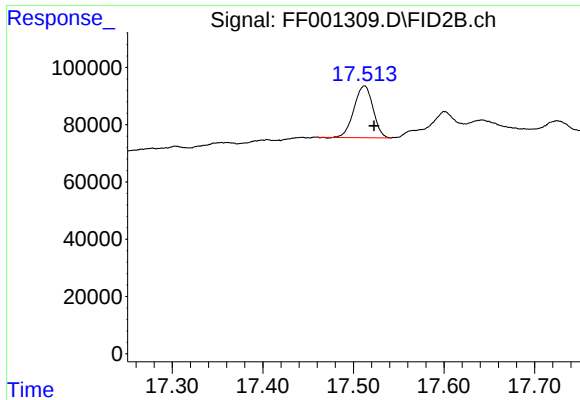

#13 N-TRIACONTANE

R.T.: 17.512 min
Delta R.T.: -0.011 min
Response: 264059
Conc: 2.20 ug/ml

Instrument :
FID_F
ClientSampleId :

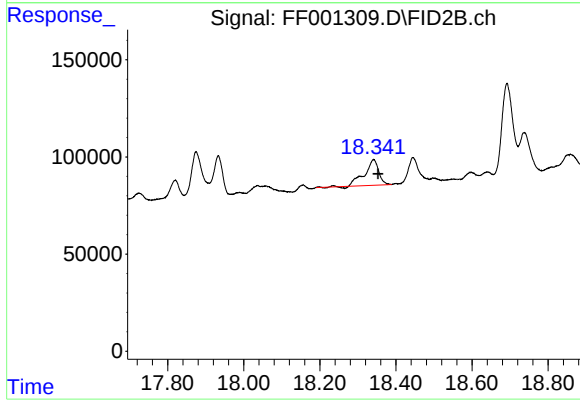

#14 N-DOTRIACONTANE

R.T.: 18.342 min
Delta R.T.: -0.012 min
Response: 336349
Conc: 2.85 ug/ml