

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001310.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 03:28
 Operator : AJ\SJ
 Sample : J3947-03
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 05:28:58 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.459	1730388	16.063 ug/ml
Target Compounds			
4) N-TETRADECANE	8.081	1072959	8.531 ug/ml
7) N-EICOSANE	12.415	636508	5.117 ug/ml
8) N-DOCOSANE	13.574	446385	3.620 ug/ml
10) N-TETRACOSANE	14.630	827678	6.789 ug/ml
12) N-OCTACOSANE	16.632	564484	4.686 ug/ml
13) N-TRIACONTANE	17.516	321482	2.674 ug/ml
14) N-DOTRIACONTANE	18.345	927420	7.866 ug/ml
15) N-TETRATRIACONTANE	19.144	622679	5.298 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001310.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 03:28
Operator : AJ\SJ
Sample : J3947-03
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 05:28:58 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

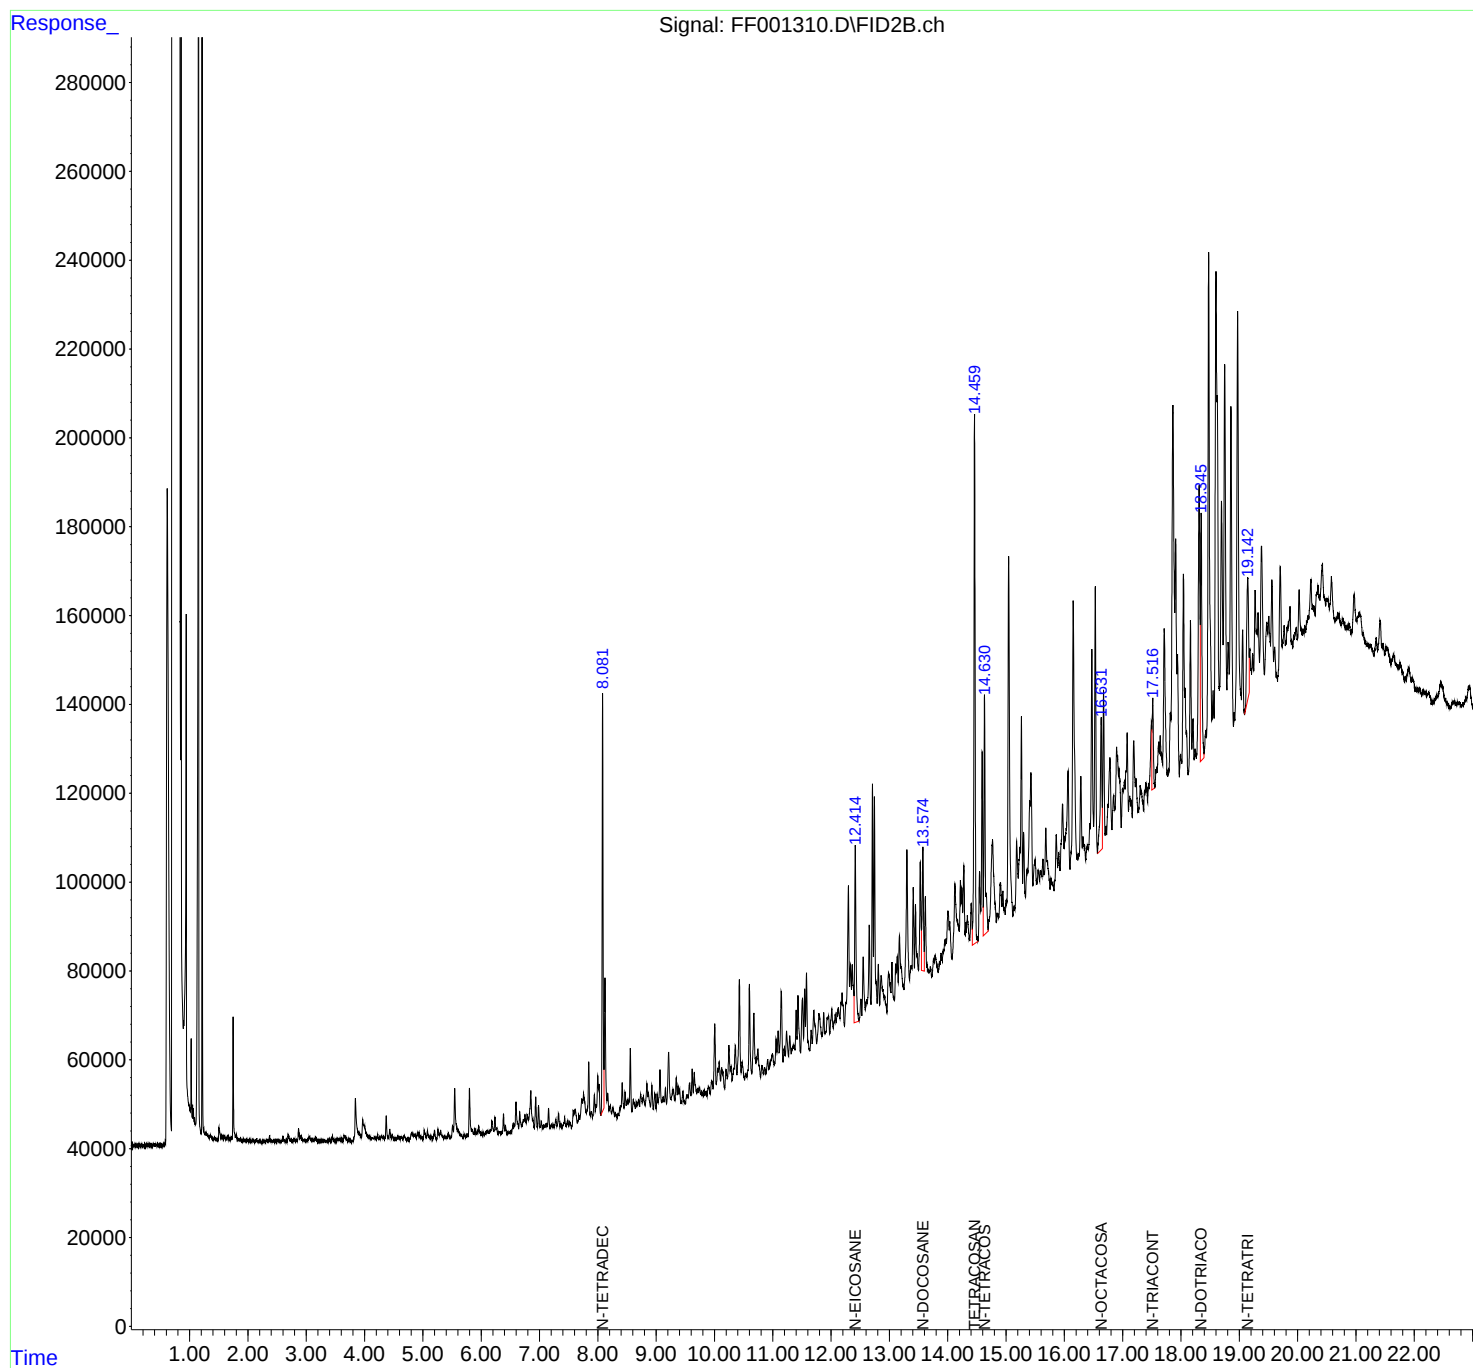


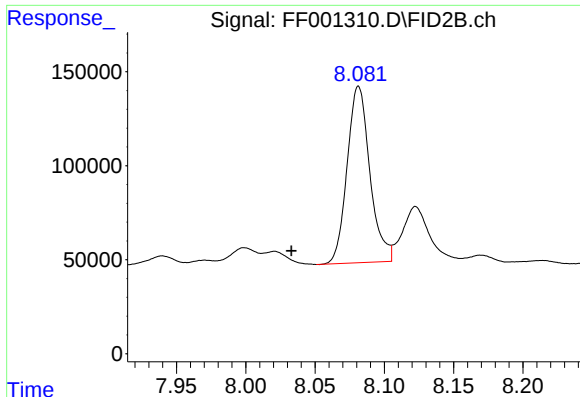

#4 N-TETRADECANE


R.T.: 8.081 min
Delta R.T.: 0.049 min
Response: 1072959
Conc: 8.53 ug/ml

Instrument :
FID_F
ClientSampleId :

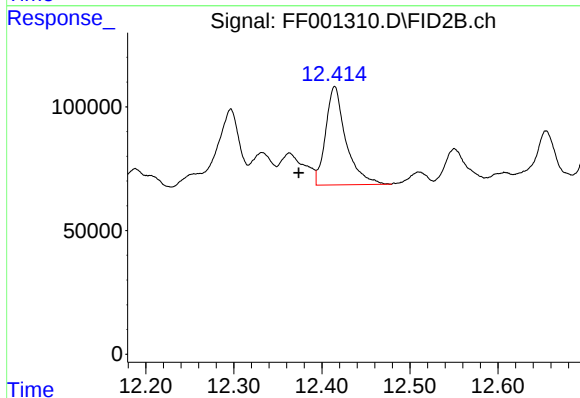


#7 N-EICOSANE

R.T.: 12.415 min
Delta R.T.: 0.041 min
Response: 636508
Conc: 5.12 ug/ml

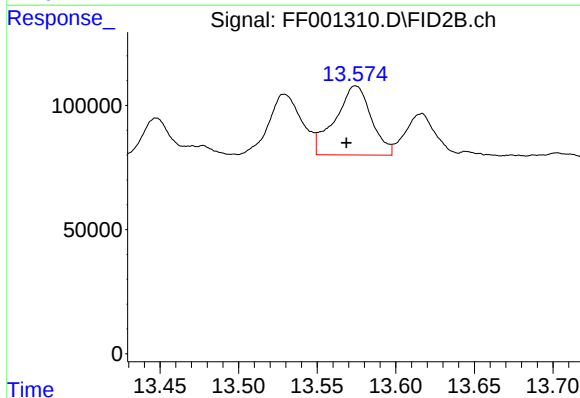


#8 N-DOCOSANE

R.T.: 13.574 min
Delta R.T.: 0.006 min
Response: 446385
Conc: 3.62 ug/ml

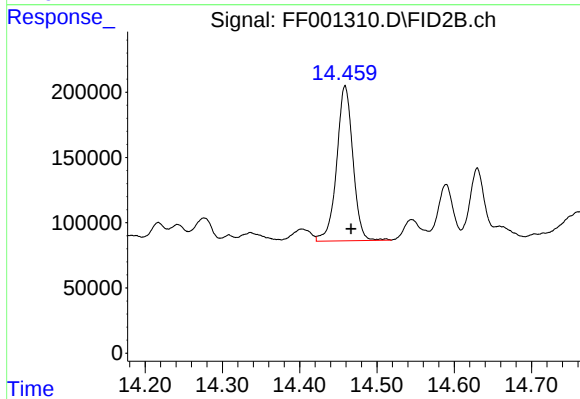

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.459 min
Delta R.T.: -0.008 min
Response: 1730388
Conc: 16.06 ug/ml

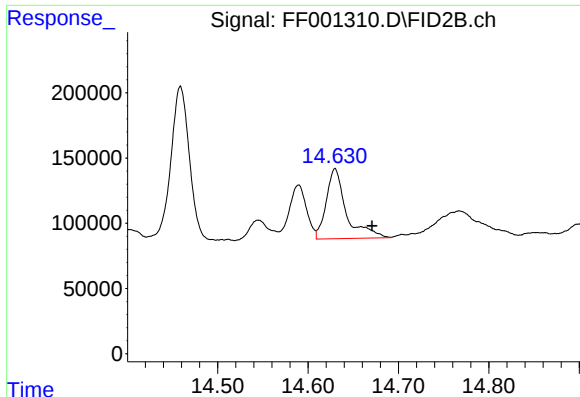

#10 N-TETRACOSANE


R.T.: 14.630 min
Delta R.T.: -0.041 min
Response: 827678
Conc: 6.79 ug/ml

Instrument :
FID_F
ClientSampleId :

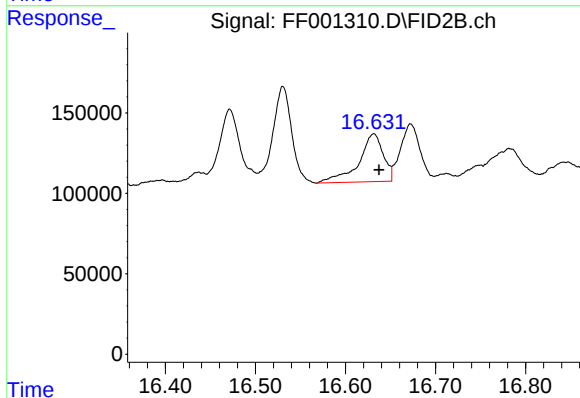


#12 N-OCTACOSANE

R.T.: 16.632 min
Delta R.T.: -0.006 min
Response: 564484
Conc: 4.69 ug/ml

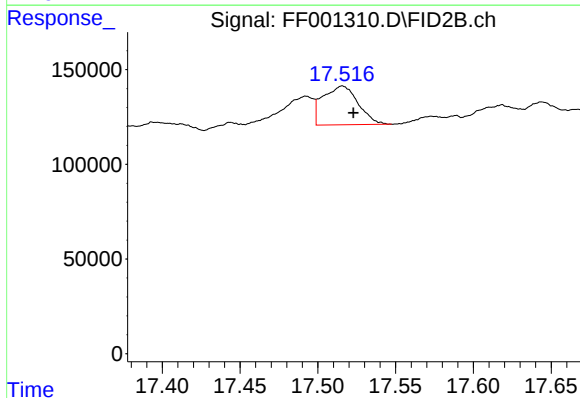


#13 N-TRIACONTANE

R.T.: 17.516 min
Delta R.T.: -0.007 min
Response: 321482
Conc: 2.67 ug/ml

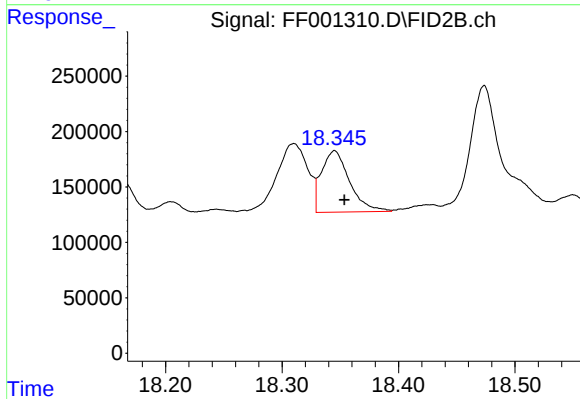

#14 N-DOTRIACONTANE

R.T.: 18.345 min
Delta R.T.: -0.008 min
Response: 927420
Conc: 7.87 ug/ml

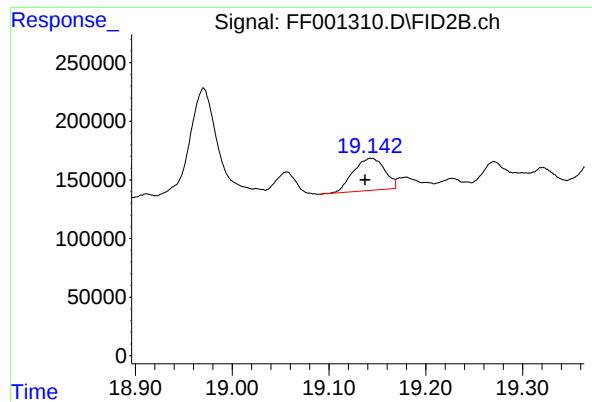

#15 N-TETRATRIACONTANE

R.T.: 19.144 min
Delta R.T.: 0.006 min
Response: 622679
Conc: 5.30 ug/ml

Instrument :
FID_F
ClientSampleId :