

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001312.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 04:28
 Operator : AJ\SJ
 Sample : J3947-05
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 05:29:32 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	1613279	14.976 ug/ml
Target Compounds			
4) N-TETRADECANE	8.081	1053535	8.377 ug/ml
5) N-HEXADECANE	9.622	384452	3.077 ug/ml
7) N-EICOSANE	12.417	5935183	47.714 ug/ml
8) N-DOCOSANE	13.572	331397	2.688 ug/ml
10) N-TETRACOSANE	14.628	1697206	13.922 ug/ml
11) N-HEXACOSANE	15.678	259915	2.144 ug/ml
12) N-OCTACOSANE	16.627	306943	2.548 ug/ml
13) N-TRIACONTANE	17.512	284127	2.364 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001312.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 04:28
Operator : AJ\SJ
Sample : J3947-05
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 05:29:32 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

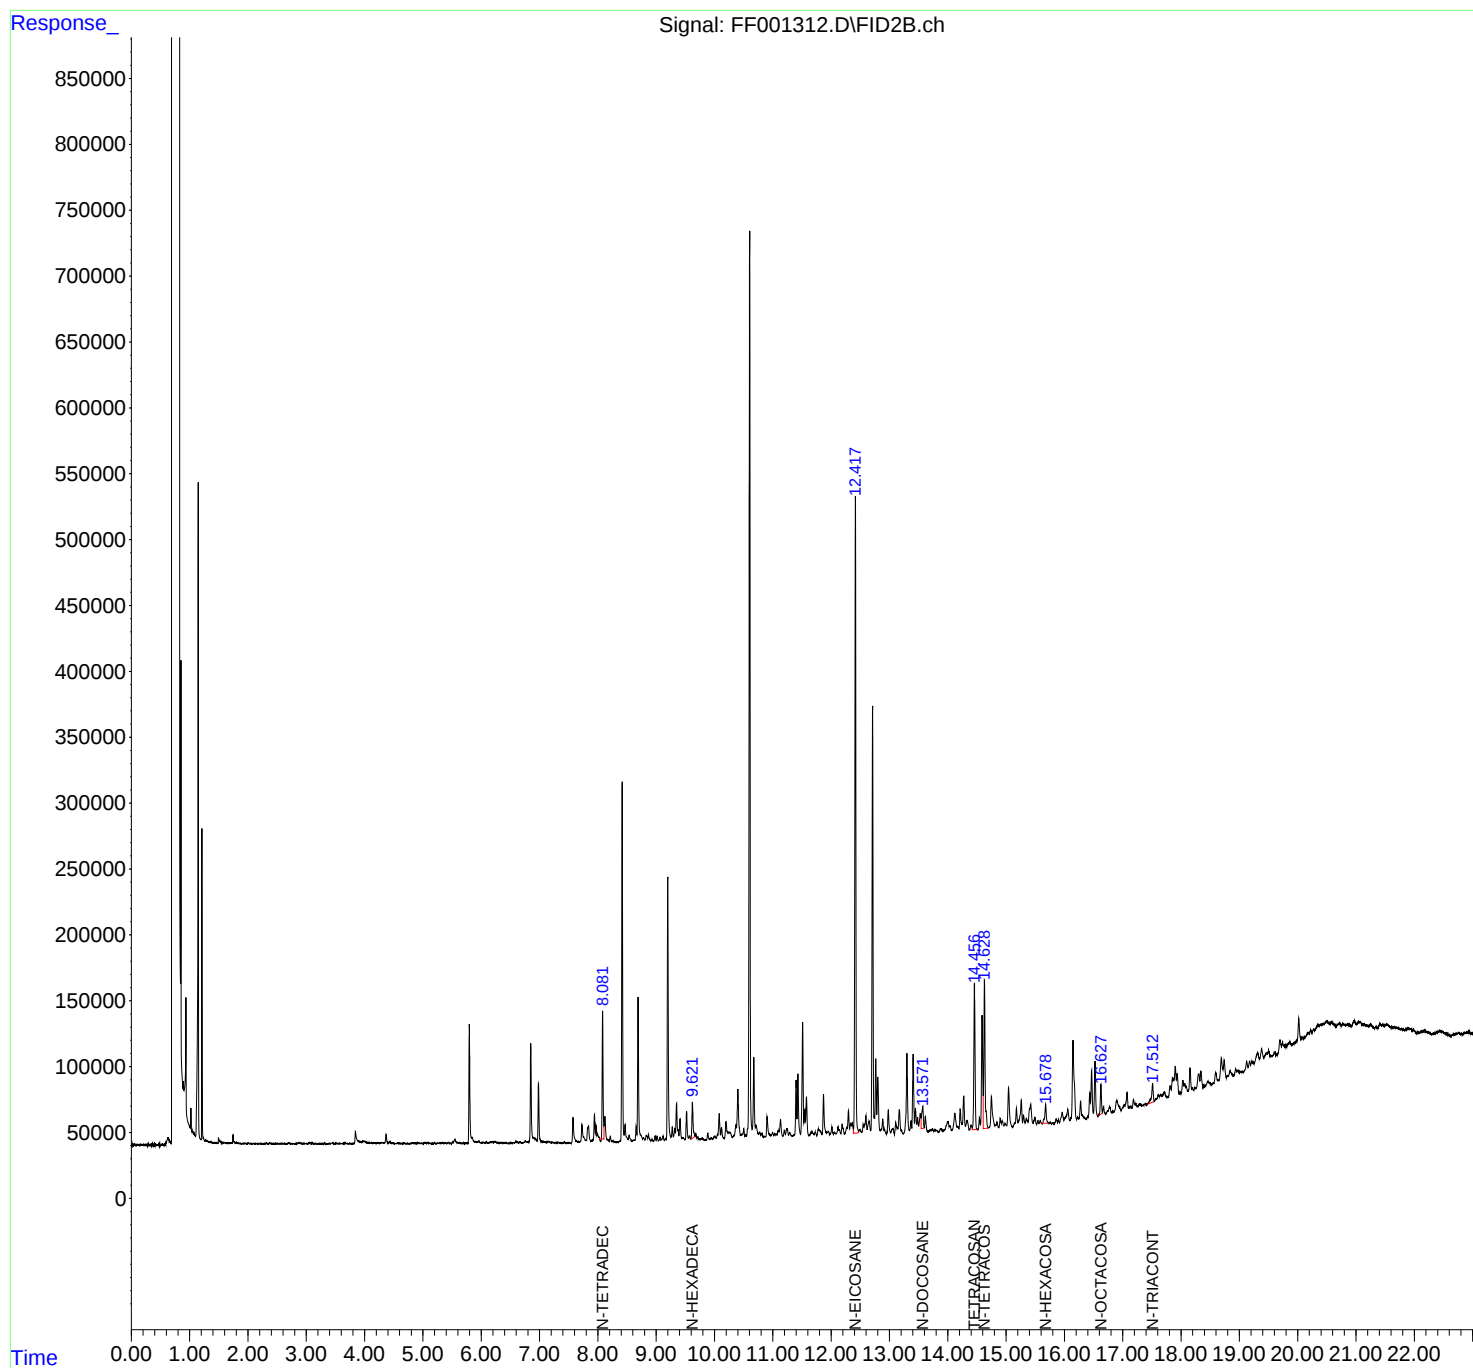


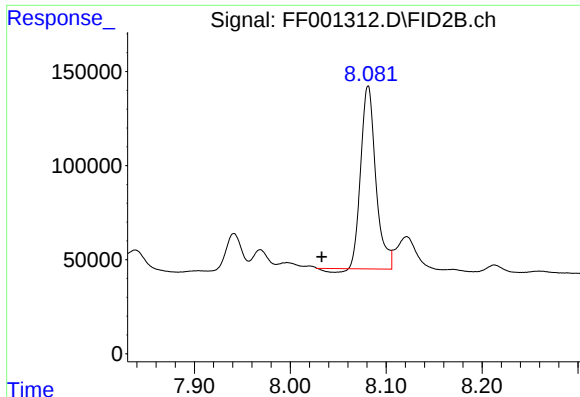

#4 N-TETRADECANE


R.T.: 8.081 min
Delta R.T.: 0.048 min
Response: 1053535
Conc: 8.38 ug/ml

Instrument :
FID_F
ClientSampleId :

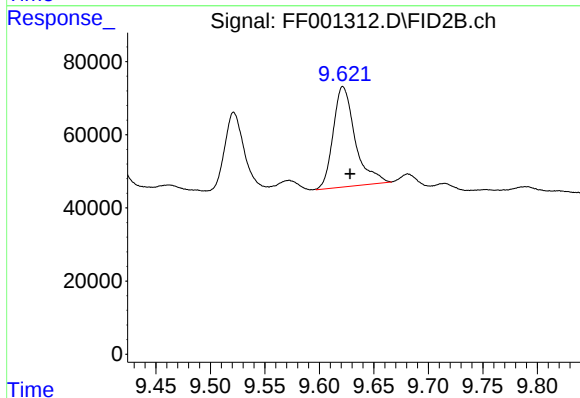


#5 N-HEXADECANE

R.T.: 9.622 min
Delta R.T.: -0.007 min
Response: 384452
Conc: 3.08 ug/ml

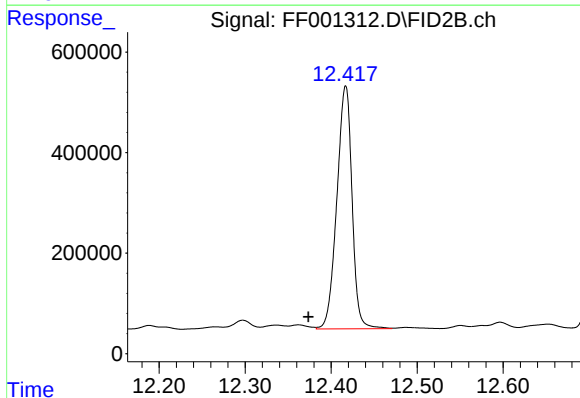


#7 N-EICOSANE

R.T.: 12.417 min
Delta R.T.: 0.043 min
Response: 5935183
Conc: 47.71 ug/ml

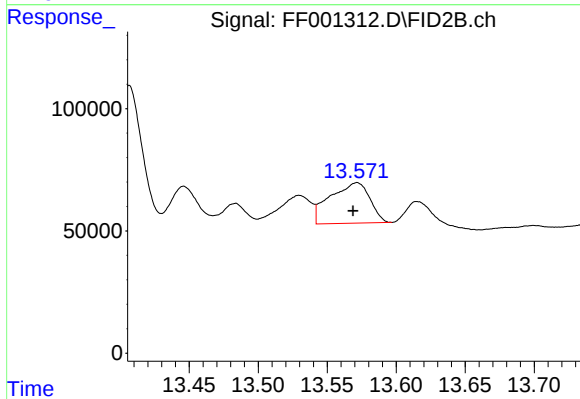

#8 N-DOCOSANE


R.T.: 13.572 min
Delta R.T.: 0.003 min
Response: 331397
Conc: 2.69 ug/ml

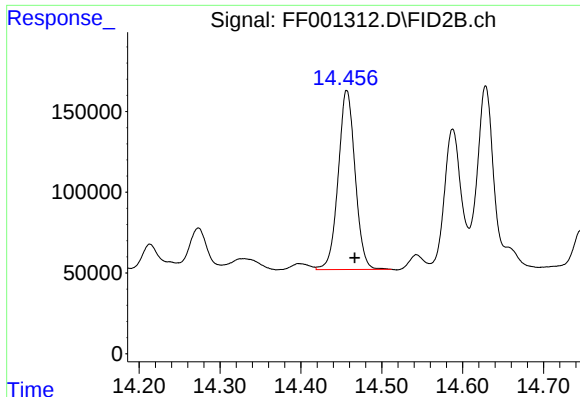

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.457 min
Delta R.T.: -0.010 min
Response: 1613279
Conc: 14.98 ug/ml

Instrument :
FID_F
ClientSampleId :

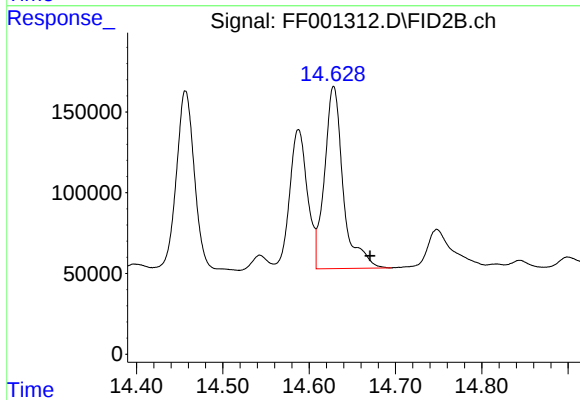


#10 N-TETRACOSANE

R.T.: 14.628 min
Delta R.T.: -0.042 min
Response: 1697206
Conc: 13.92 ug/ml

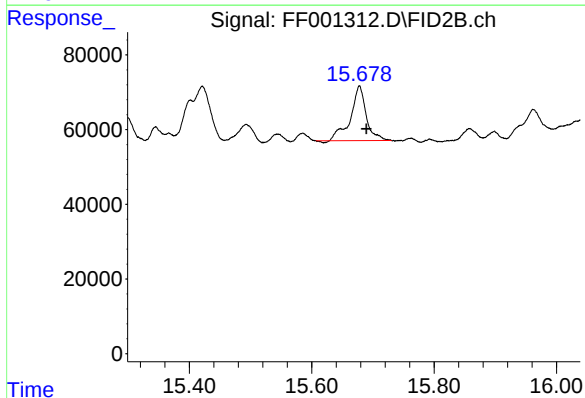


#11 N-HEXACOSANE

R.T.: 15.678 min
Delta R.T.: -0.011 min
Response: 259915
Conc: 2.14 ug/ml

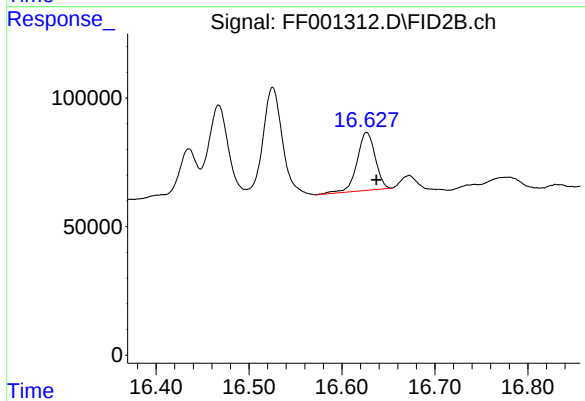

#12 N-OCTACOSANE

R.T.: 16.627 min
Delta R.T.: -0.011 min
Response: 306943
Conc: 2.55 ug/ml

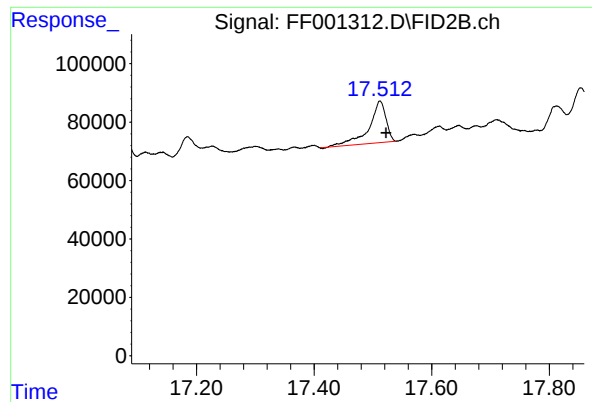

#13 N-TRIACONTANE

R.T.: 17.512 min
Delta R.T.: -0.011 min
Response: 284127
Conc: 2.36 ug/ml

Instrument :
FID_F
ClientSampleId :