

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001314.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 05:27
 Operator : AJ\SJ
 Sample : J3947-07
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 06:47:08 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.462	3345073	31.052 ug/ml
Target Compounds			
4) N-TETRADECANE	8.082	1264938	10.058 ug/ml
5) N-HEXADECANE	9.619	425514	3.406 ug/ml
6) N-OCTADECANE	11.069	247015	1.971 ug/ml
7) N-EICOSANE	12.367	362768	2.916 ug/ml
8) N-DOCOSANE	13.579	2079242	16.862 ug/ml
10) N-TETRACOSANE	14.668	1379104	11.313 ug/ml
11) N-HEXACOSANE	15.688	2640493	21.784 ug/ml
12) N-OCTACOSANE	16.642	6331199	52.553 ug/ml
13) N-TRIACONTANE	17.518	6099399	50.740 ug/ml
14) N-DOTRIACONTANE	18.353	1704016	14.453 ug/ml
15) N-TETRATRIACONTANE	19.147	1004898	8.550 ug/ml
16) N-HEXATRIACONTANE	19.933f	199601	1.757 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001314.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 05:27
Operator : AJ\SJ
Sample : J3947-07
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 06:47:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

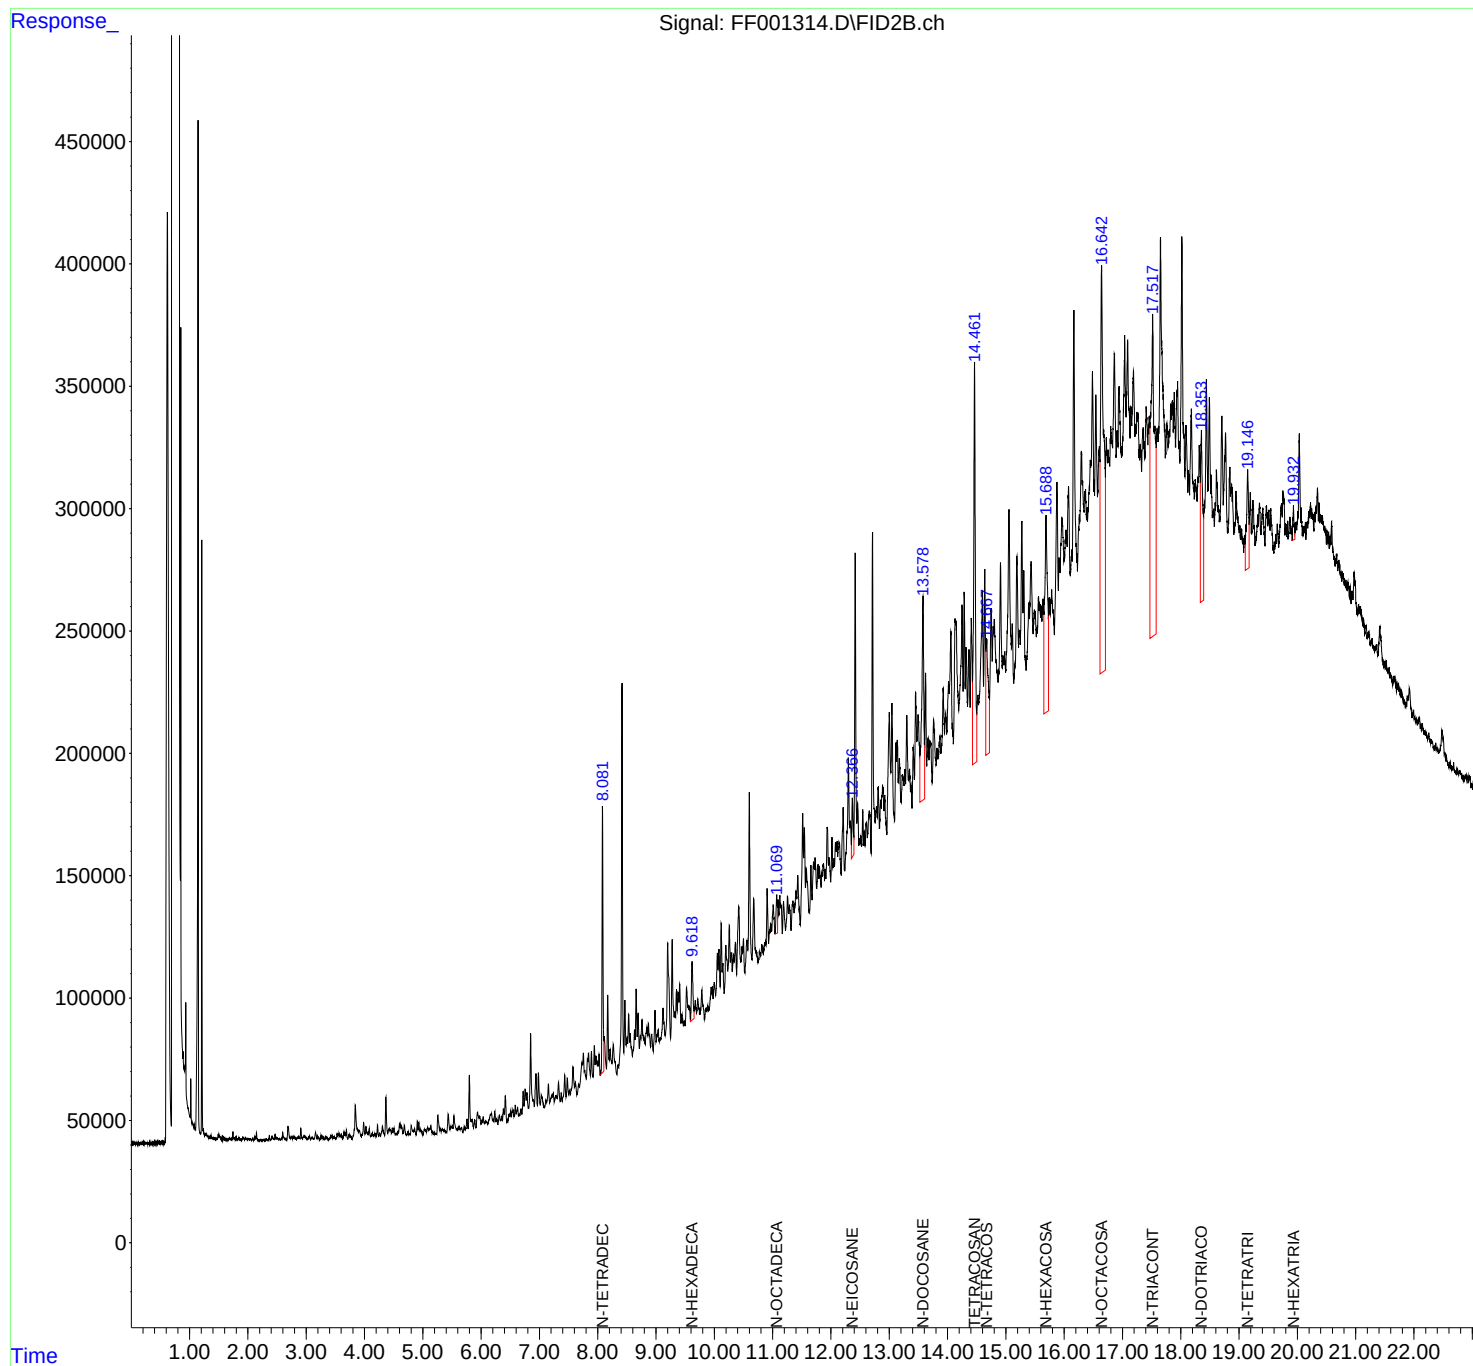


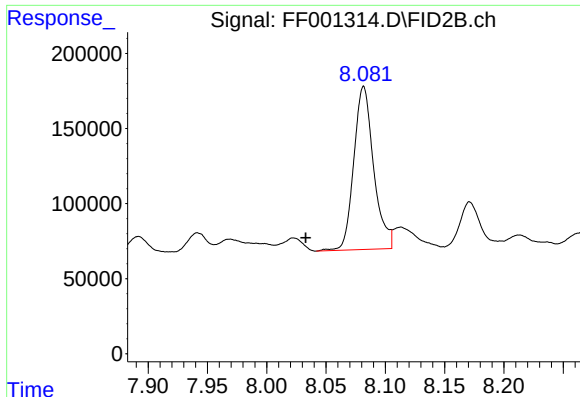

#4 N-TETRADECANE


R.T.: 8.082 min
Delta R.T.: 0.049 min
Response: 1264938
Conc: 10.06 ug/ml

Instrument :
FID_F
ClientSampleId :

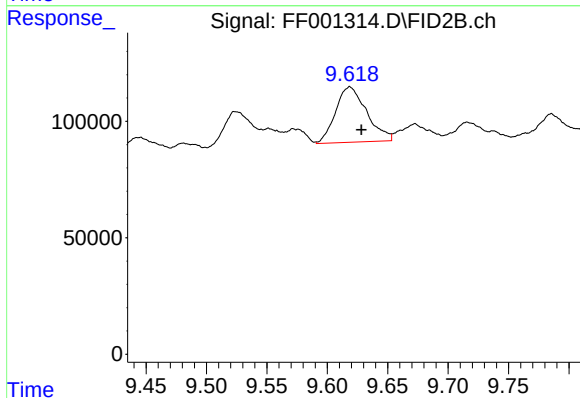


#5 N-HEXADECANE

R.T.: 9.619 min
Delta R.T.: -0.010 min
Response: 425514
Conc: 3.41 ug/ml

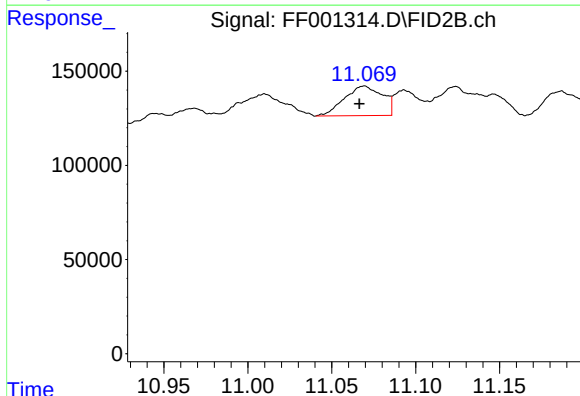


#6 N-OCTADECANE

R.T.: 11.069 min
Delta R.T.: 0.003 min
Response: 247015
Conc: 1.97 ug/ml

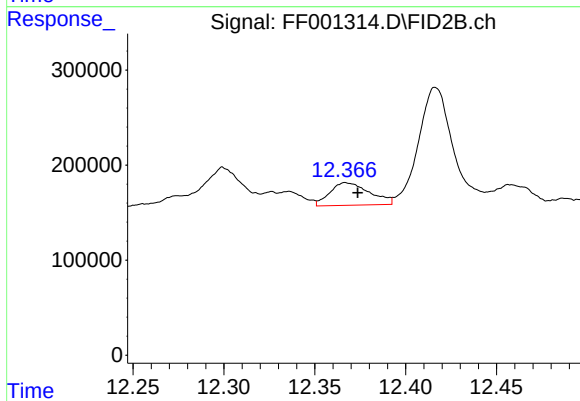

#7 N-EICOSANE


R.T.: 12.367 min
Delta R.T.: -0.006 min
Response: 362768
Conc: 2.92 ug/ml

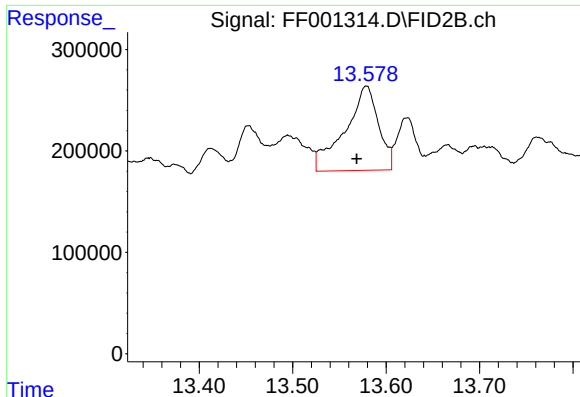

#8 N-DOCOSANE


R.T.: 13.579 min
Delta R.T.: 0.010 min
Response: 2079242
Conc: 16.86 ug/ml

Instrument :
FID_F
ClientSampleId :

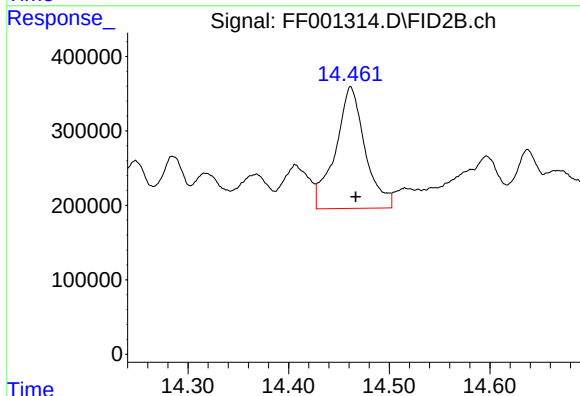


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.462 min
Delta R.T.: -0.005 min
Response: 3345073
Conc: 31.05 ug/ml

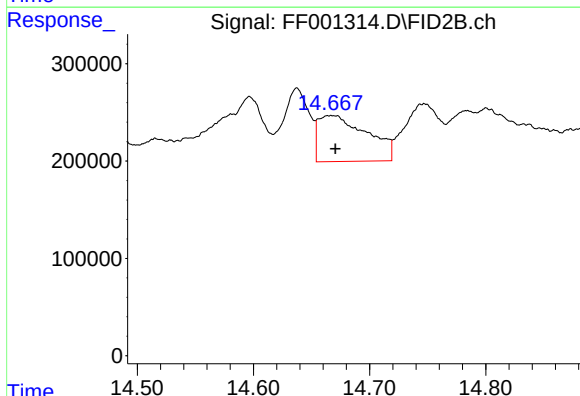


#10 N-TETRACOSANE

R.T.: 14.668 min
Delta R.T.: -0.003 min
Response: 1379104
Conc: 11.31 ug/ml

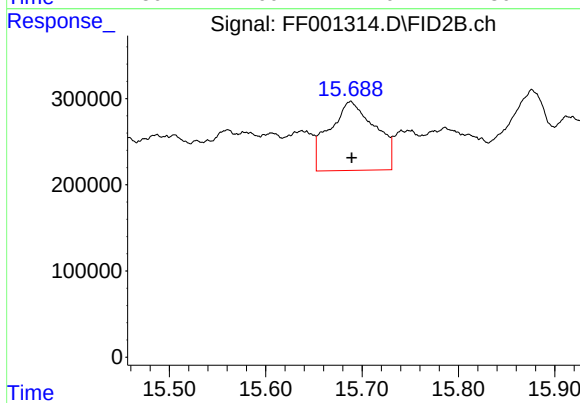

#11 N-HEXACOSANE


R.T.: 15.688 min
Delta R.T.: -0.001 min
Response: 2640493
Conc: 21.78 ug/ml

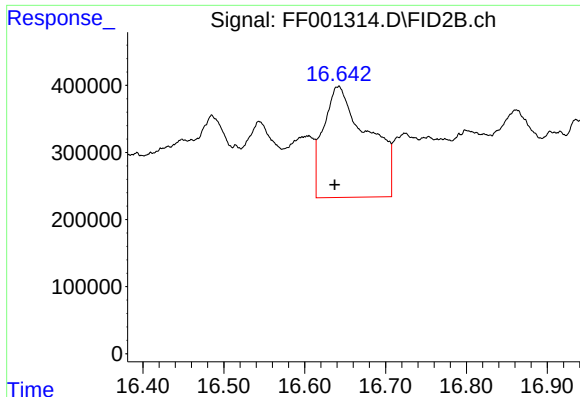

#12 N-OCTACOSANE


R.T.: 16.642 min
Delta R.T.: 0.005 min
Response: 6331199
Conc: 52.55 ug/ml

Instrument :
FID_F
ClientSampleId :

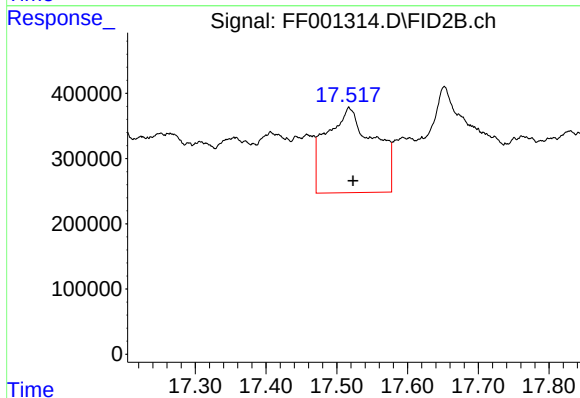


#13 N-TRIACONTANE

R.T.: 17.518 min
Delta R.T.: -0.005 min
Response: 6099399
Conc: 50.74 ug/ml

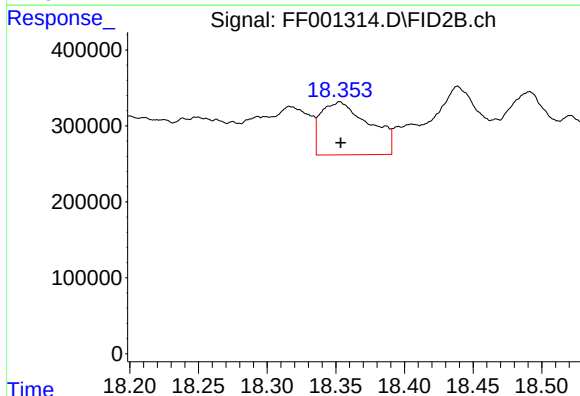


#14 N-DOTRIACONTANE

R.T.: 18.353 min
Delta R.T.: 0.000 min
Response: 1704016
Conc: 14.45 ug/ml

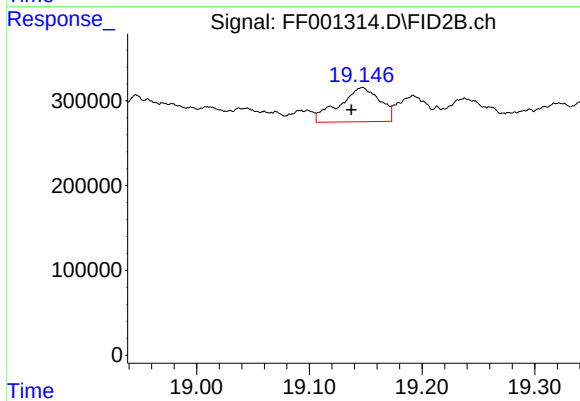

#15 N-TETRATRIACONTANE

R.T.: 19.147 min
Delta R.T.: 0.010 min
Response: 1004898
Conc: 8.55 ug/ml

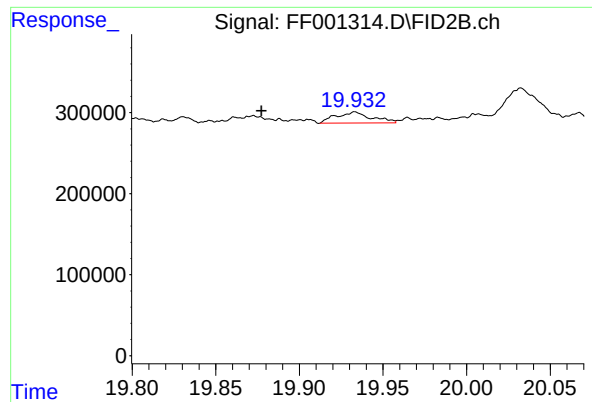

#16 N-HEXATRIACONTANE

R.T.: 19.933 min
Delta R.T.: 0.056 min
Response: 199601
Conc: 1.76 ug/ml

Instrument :
FID_F
ClientSampleId :