

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001315.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 05:57
 Operator : AJ\SJ
 Sample : J3947-08
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 06:47:45 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.463	3146863	29.212 ug/ml
Target Compounds			
4) N-TETRADECANE	8.082	1296785	10.311 ug/ml
5) N-HEXADECANE	9.620	422145	3.379 ug/ml
6) N-OCTADECANE	11.071	356775	2.847 ug/ml
7) N-EICOSANE	12.371	579713	4.660 ug/ml
8) N-DOCOSANE	13.583	2032168	16.480 ug/ml
10) N-TETRACOSANE	14.665	1018610	8.356 ug/ml
11) N-HEXACOSANE	15.690	2083422	17.188 ug/ml
12) N-OCTACOSANE	16.646	6202078	51.481 ug/ml
13) N-TRIACONTANE	17.522	7111214	59.157 ug/ml
14) N-DOTRIACONTANE	18.352	1184357	10.045 ug/ml
15) N-TETRATRIACONTANE	19.150	555891	4.730 ug/ml
16) N-HEXATRIACONTANE	19.928f	345087	3.038 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001315.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 05:57
Operator : AJ\SJ
Sample : J3947-08
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 06:47:45 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

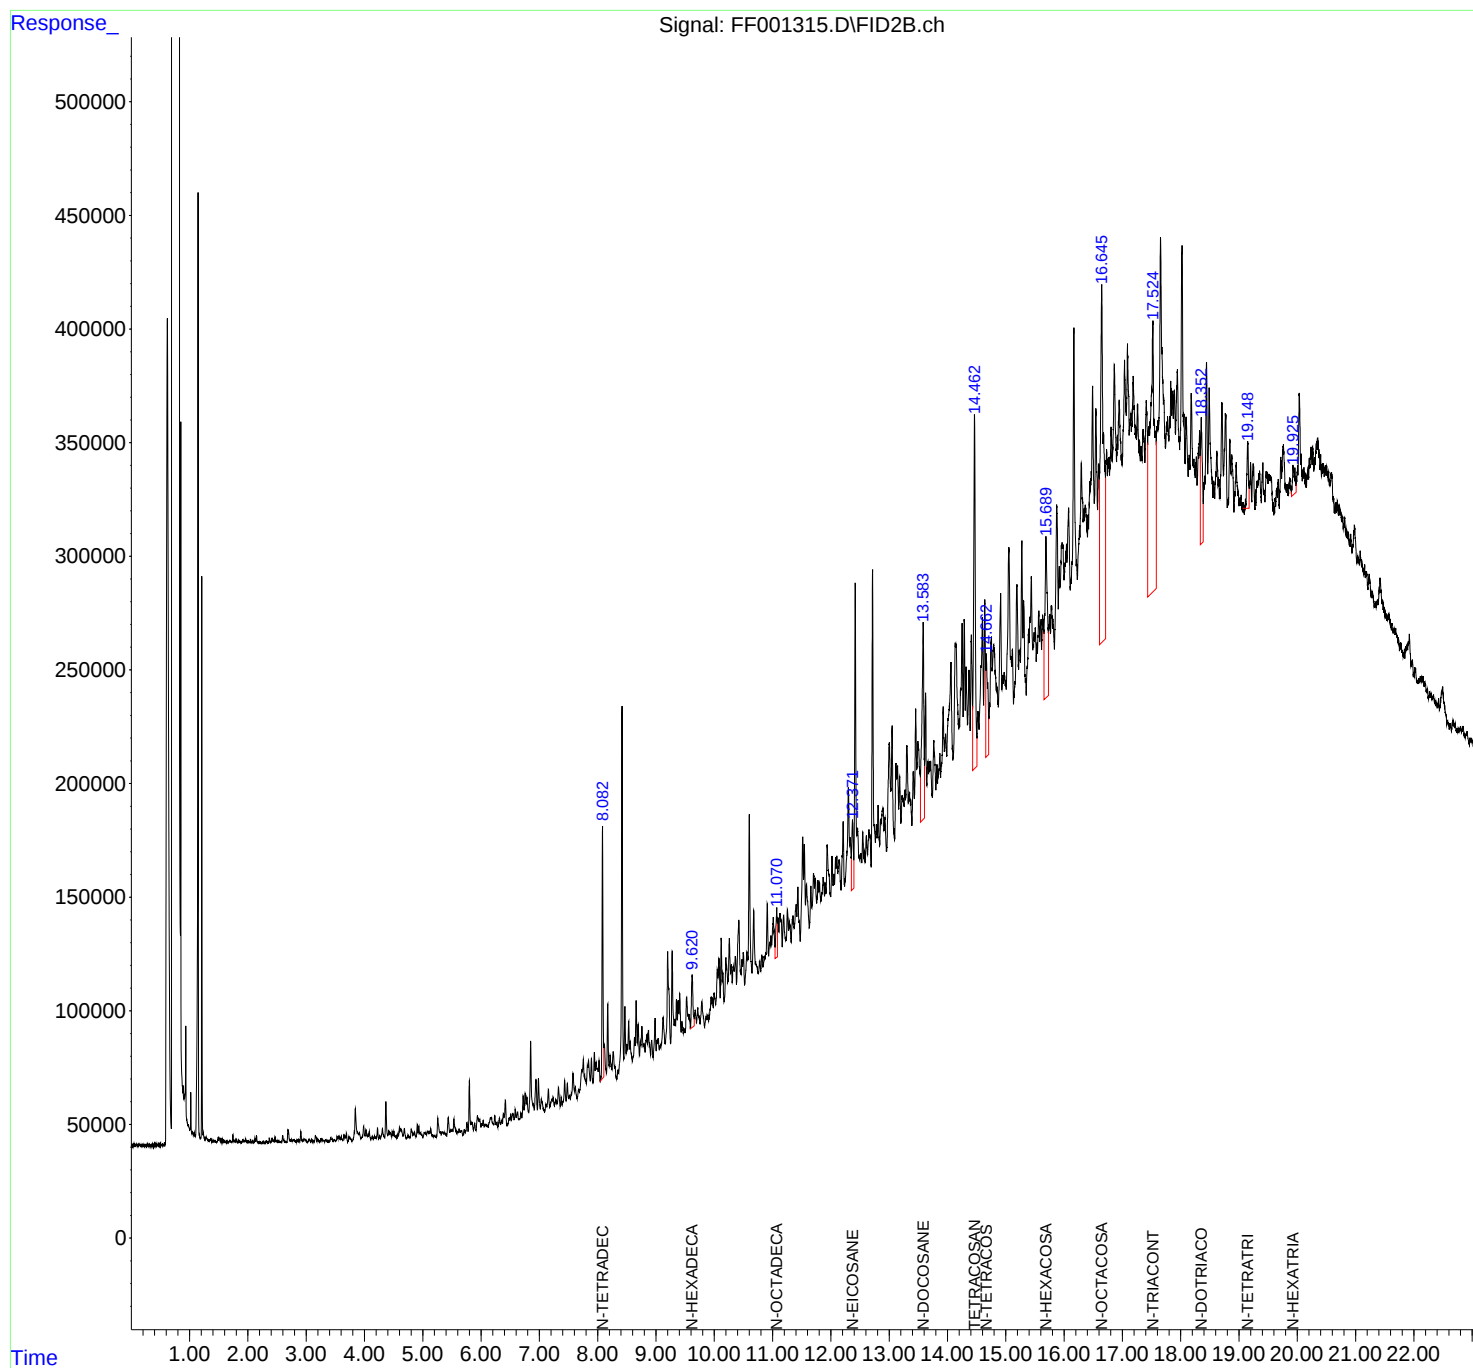


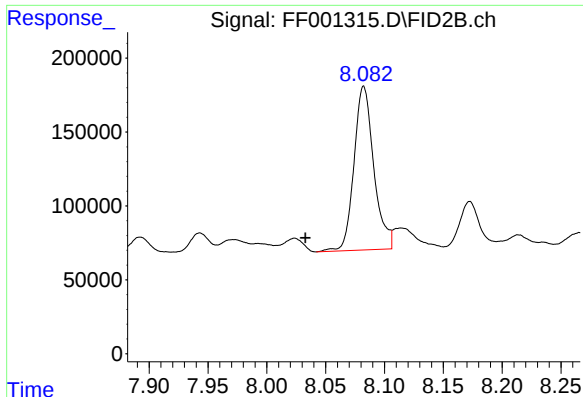

#4 N-TETRADECANE


R.T.: 8.082 min
Delta R.T.: 0.050 min
Response: 1296785
Conc: 10.31 ug/ml

Instrument :
FID_F
ClientSampleId :

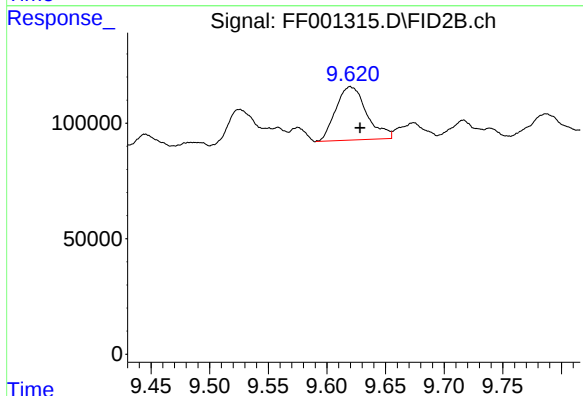


#5 N-HEXADECANE

R.T.: 9.620 min
Delta R.T.: -0.008 min
Response: 422145
Conc: 3.38 ug/ml

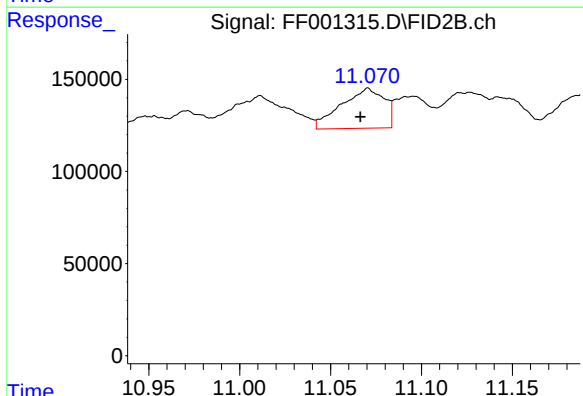


#6 N-OCTADECANE

R.T.: 11.071 min
Delta R.T.: 0.004 min
Response: 356775
Conc: 2.85 ug/ml

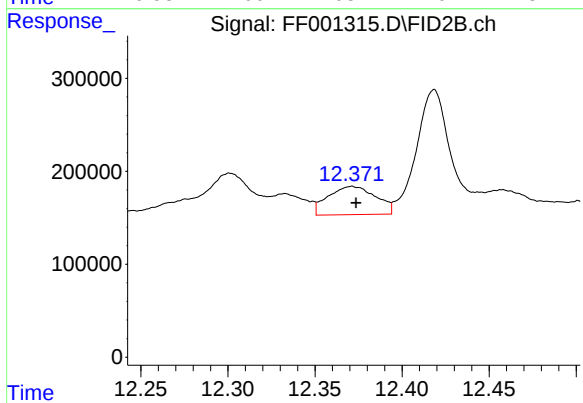

#7 N-EICOSANE


R.T.: 12.371 min
Delta R.T.: -0.003 min
Response: 579713
Conc: 4.66 ug/ml

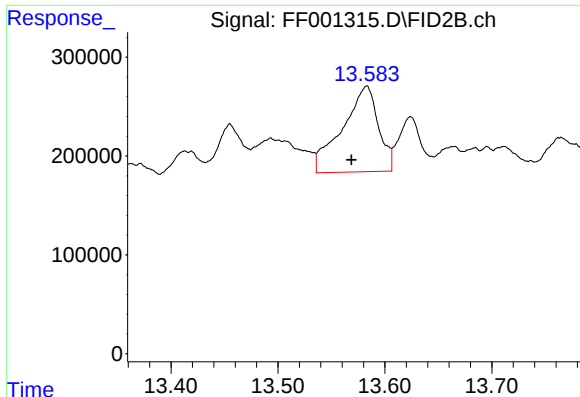

#8 N-DOCOSANE


R.T.: 13.583 min
Delta R.T.: 0.014 min
Response: 2032168
Conc: 16.48 ug/ml

Instrument :
FID_F
ClientSampleId :

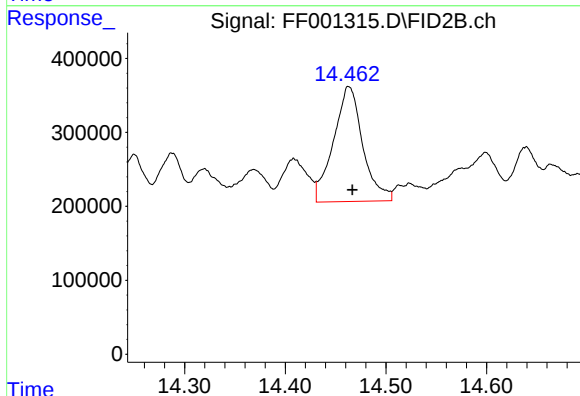


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.463 min
Delta R.T.: -0.003 min
Response: 3146863
Conc: 29.21 ug/ml

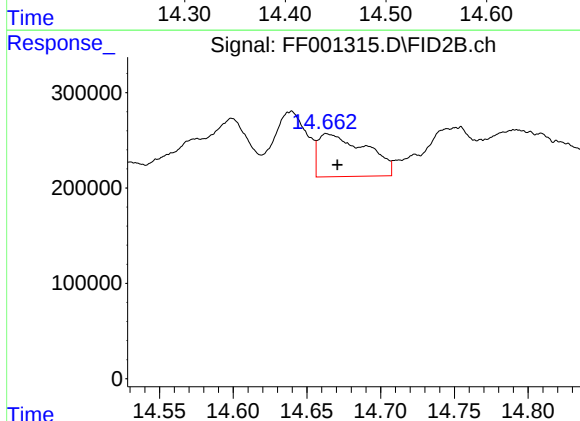


#10 N-TETRACOSANE

R.T.: 14.665 min
Delta R.T.: -0.006 min
Response: 1018610
Conc: 8.36 ug/ml

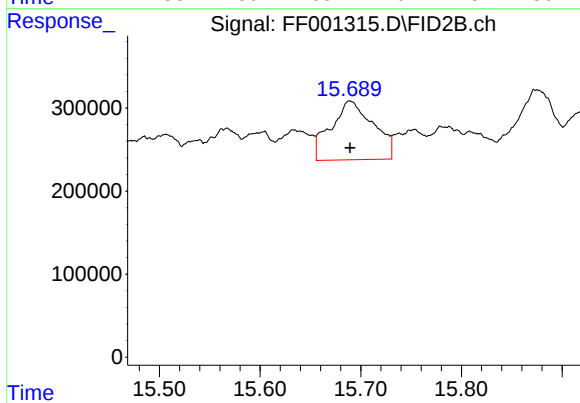

#11 N-HEXACOSANE


R.T.: 15.690 min
Delta R.T.: 0.000 min
Response: 2083422
Conc: 17.19 ug/ml

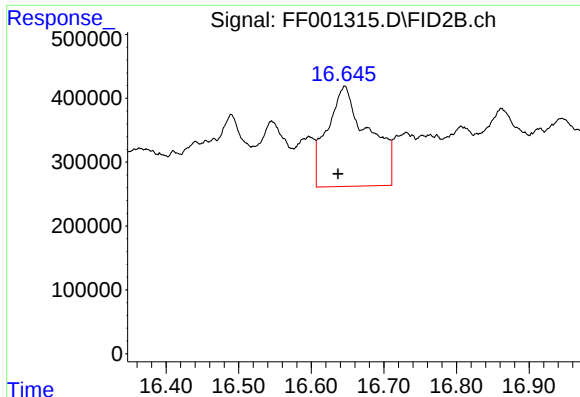

#12 N-OCTACOSANE


R.T.: 16.646 min
Delta R.T.: 0.009 min
Response: 6202078
Conc: 51.48 ug/ml

Instrument :
FID_F
ClientSampleId :

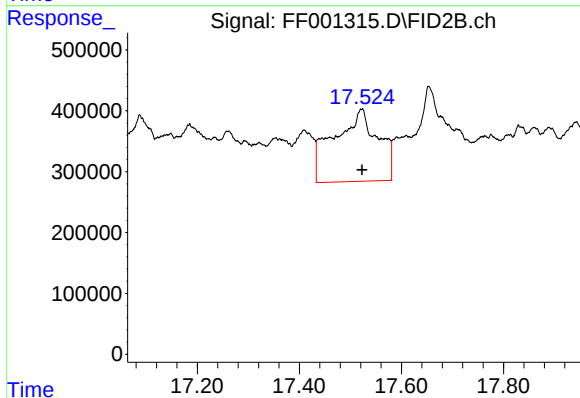


#13 N-TRIACONTANE

R.T.: 17.522 min
Delta R.T.: 0.000 min
Response: 7111214
Conc: 59.16 ug/ml

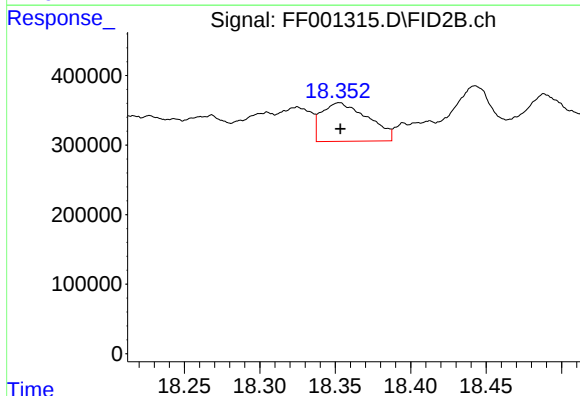


#14 N-DOTRIACONTANE

R.T.: 18.352 min
Delta R.T.: -0.001 min
Response: 1184357
Conc: 10.05 ug/ml

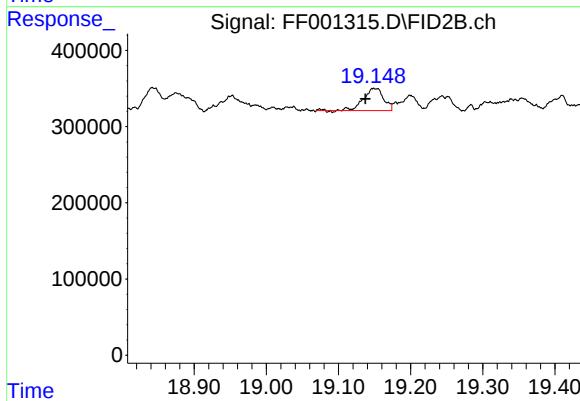

#15 N-TETRATRIACONTANE

R.T.: 19.150 min
Delta R.T.: 0.013 min
Response: 555891
Conc: 4.73 ug/ml

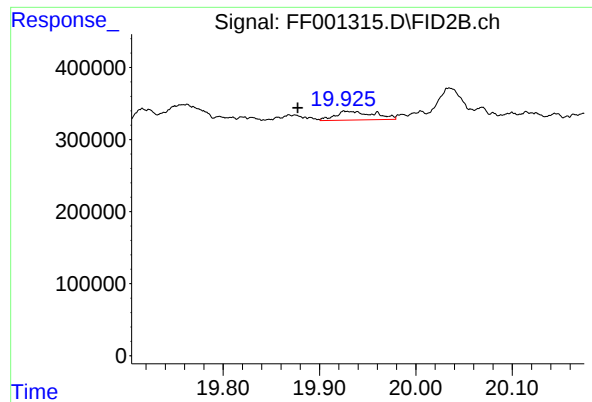

#16 N-HEXATRIACONTANE

R.T.: 19.928 min
Delta R.T.: 0.051 min
Response: 345087
Conc: 3.04 ug/ml

Instrument :
FID_F
ClientSampleId :