

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
 Data File : FF001318.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 06:27
 Operator : AJ\SJ
 Sample : J3948-03
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 08:48:42 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.460	1832327	17.010 ug/ml
Target Compounds			
4) N-TETRADECANE	8.000	292849	2.328 ug/ml
6) N-OCTADECANE	11.134f	503399	4.017 ug/ml
7) N-EICOSANE	12.335	416548	3.349 ug/ml
8) N-DOCOSANE	13.577	647458	5.251 ug/ml
10) N-TETRACOSANE	14.634	3037204	24.914 ug/ml
12) N-OCTACOSANE	16.631	807410	6.702 ug/ml
13) N-TRIACONTANE	17.516	452580	3.765 ug/ml
14) N-DOTRIACONTANE	18.334	620660	5.264 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071218\
Data File : FF001318.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 06:27
Operator : AJ\SJ
Sample : J3948-03
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 08:48:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

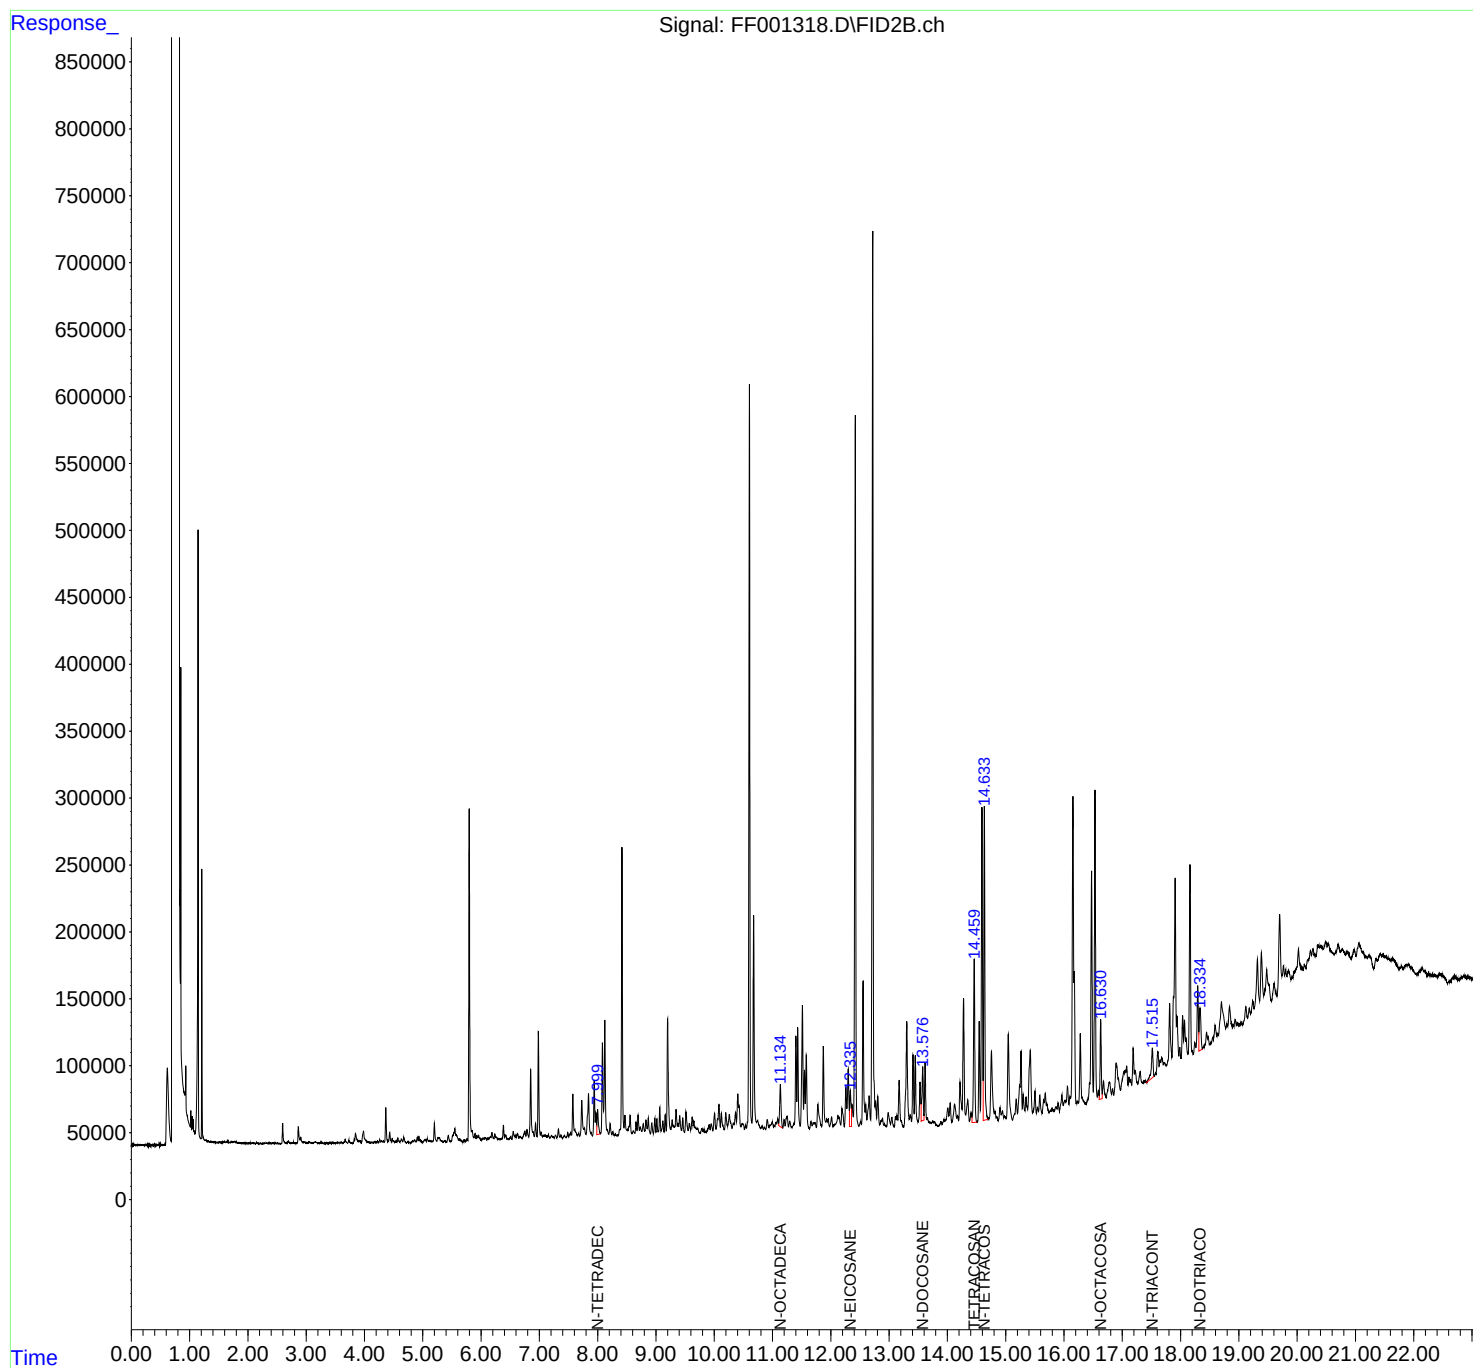


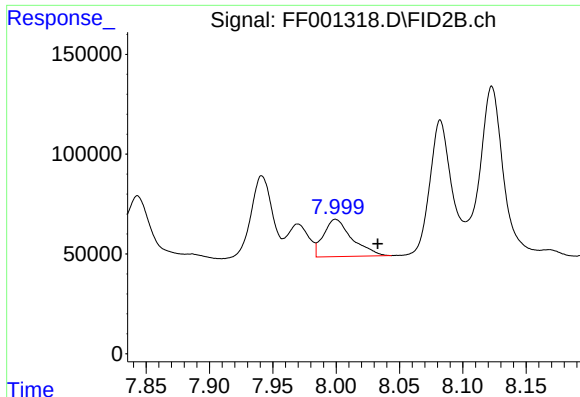

#4 N-TETRADECANE


R.T.: 8.000 min
Delta R.T.: -0.033 min
Response: 292849
Conc: 2.33 ug/ml

Instrument :
FID_F
ClientSampleId :

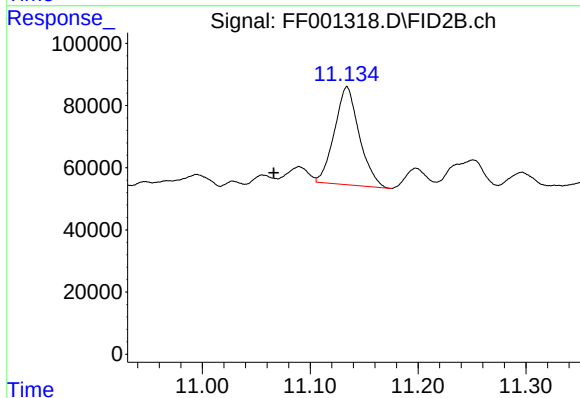


#6 N-OCTADECANE

R.T.: 11.134 min
Delta R.T.: 0.068 min
Response: 503399
Conc: 4.02 ug/ml

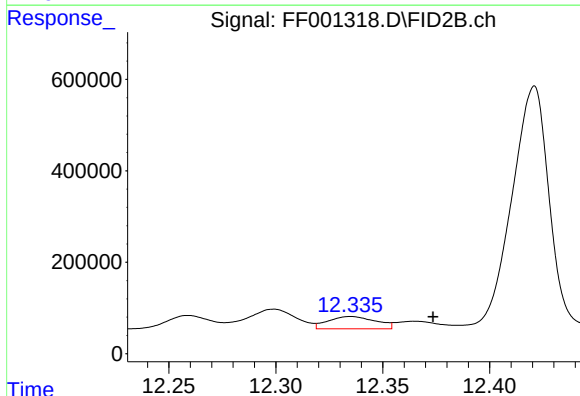


#7 N-EICOSANE

R.T.: 12.335 min
Delta R.T.: -0.038 min
Response: 416548
Conc: 3.35 ug/ml

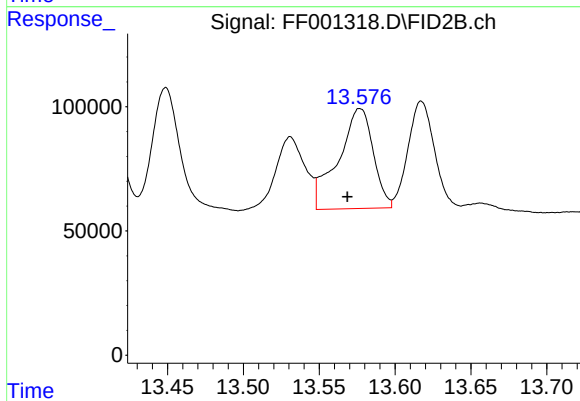

#8 N-DOCOSANE


R.T.: 13.577 min
Delta R.T.: 0.008 min
Response: 647458
Conc: 5.25 ug/ml

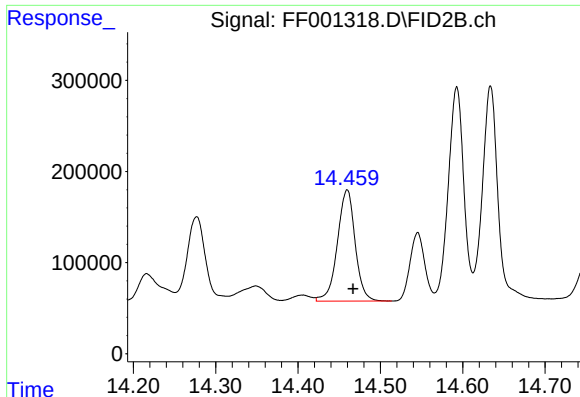

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.460 min
Delta R.T.: -0.007 min
Response: 1832327
Conc: 17.01 ug/ml

Instrument :
FID_F
ClientSampleId :

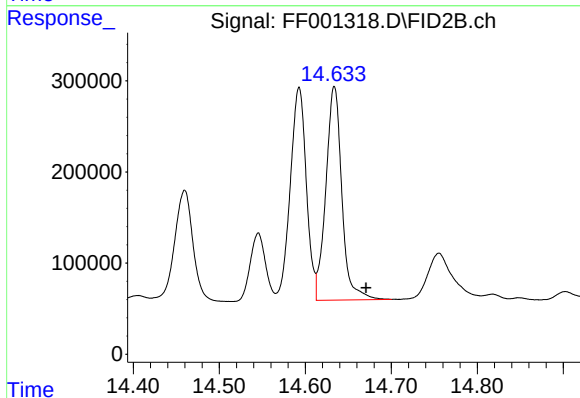


#10 N-TETRACOSANE

R.T.: 14.634 min
Delta R.T.: -0.037 min
Response: 3037204
Conc: 24.91 ug/ml

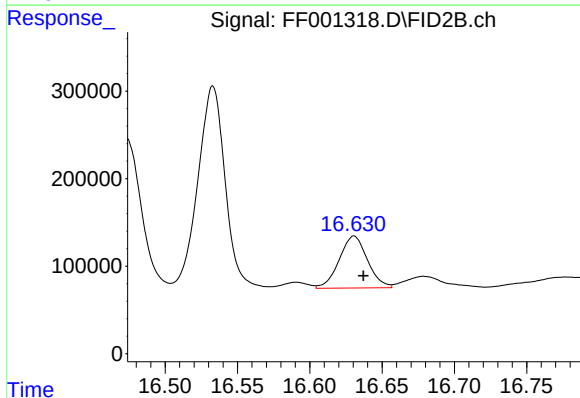


#12 N-OCTACOSANE

R.T.: 16.631 min
Delta R.T.: -0.007 min
Response: 807410
Conc: 6.70 ug/ml

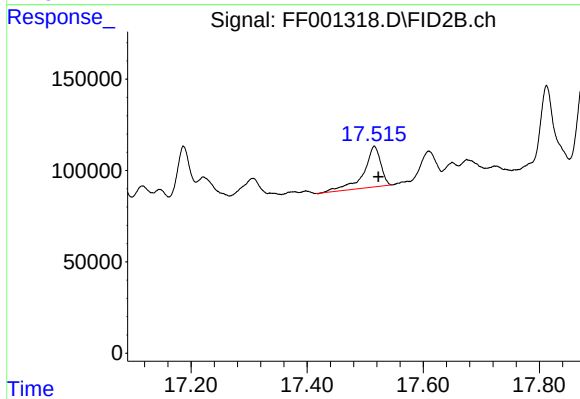

#13 N-TRIACONTANE

R.T.: 17.516 min
Delta R.T.: -0.007 min
Response: 452580
Conc: 3.76 ug/ml

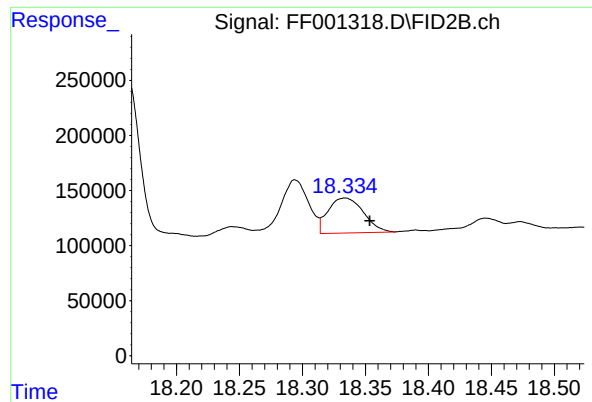

#14 N-DOTRIACONTANE

R.T.: 18.334 min
Delta R.T.: -0.020 min
Response: 620660
Conc: 5.26 ug/ml

Instrument :
FID_F
ClientSampleId :