

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071218\
Data File : FG001636.D
Signal(s) : FID1A.ch
Acq On : 12 Jul 2018 13:59
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 04:13:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.274	3977449	30.238 ug/ml
12)	N-OCTACOSANE	16.690	3896429	29.805 ug/ml
13)	N-TRIACONTANE	17.576	308118	2.365 ug/ml
14)	N-DOTRIACONTANE	18.410	441449	3.468 ug/ml
15)	N-TETRATRIACONTANE	19.195	326359	2.593 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071218\
Data File : FG001636.D
Signal(s) : FID1A.ch
Acq On : 12 Jul 2018 13:59
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 04:13:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

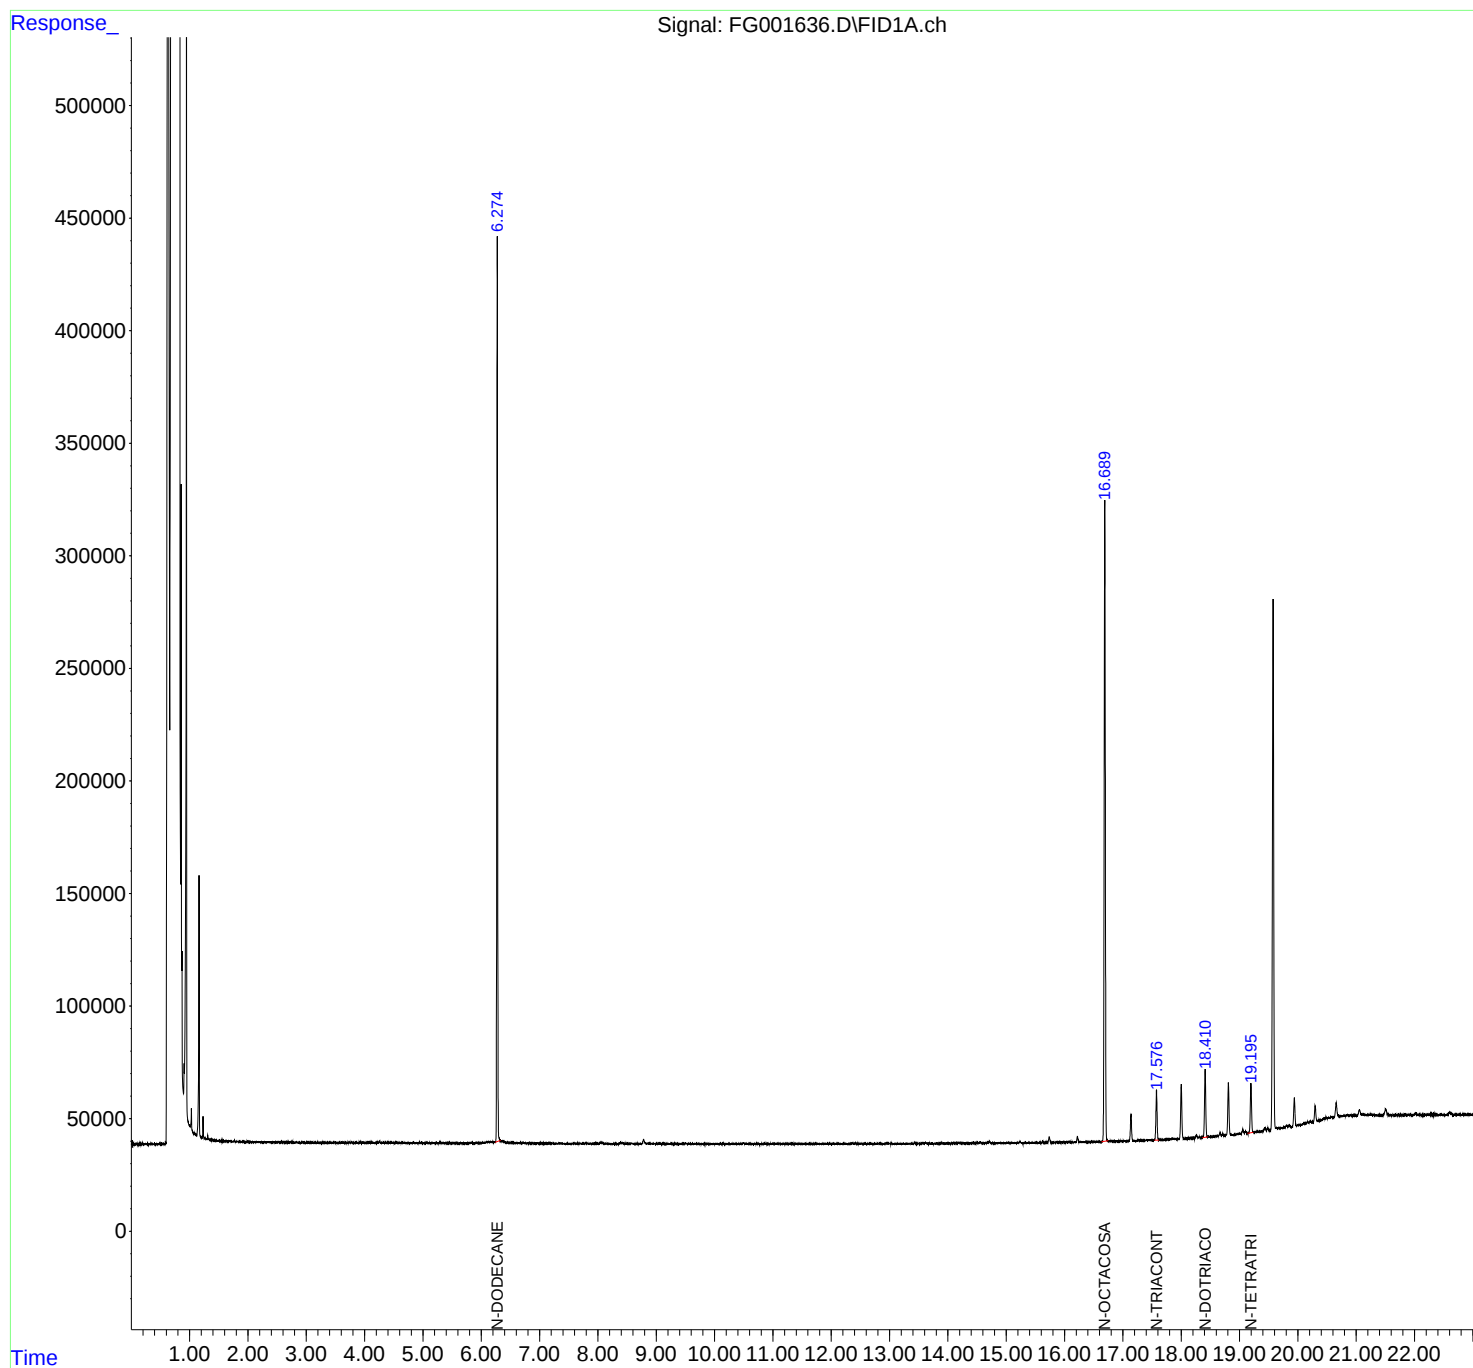


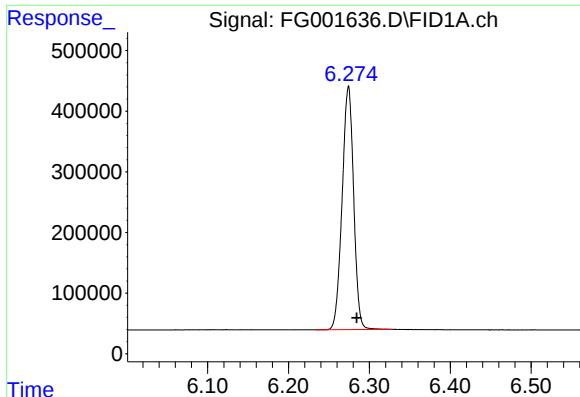

#3 N-DODECANE


R.T.: 6.274 min
Delta R.T.: -0.010 min
Response: 3977449
Conc: 30.24 ug/ml

Instrument :
FID_F
ClientSampleId :

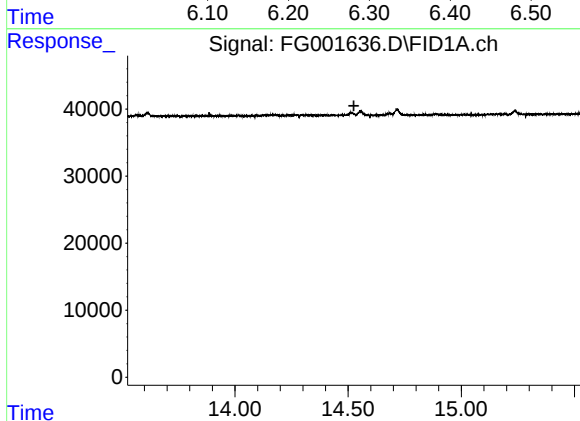


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.525 min
Response: 0
Conc: N.D.

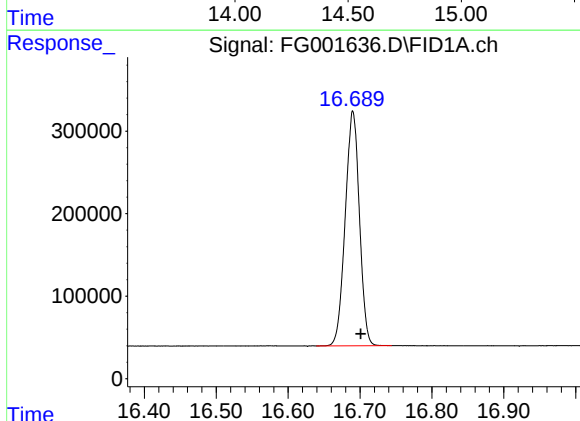


#12 N-OCTACOSANE

R.T.: 16.690 min
Delta R.T.: -0.011 min
Response: 3896429
Conc: 29.80 ug/ml

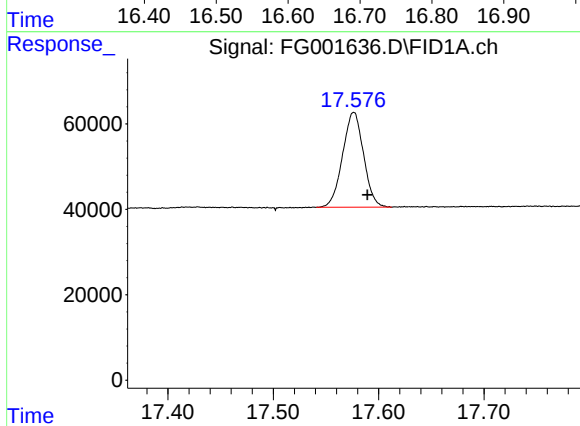

#13 N-TRIACONTANE


R.T.: 17.576 min
Delta R.T.: -0.013 min
Response: 308118
Conc: 2.36 ug/ml

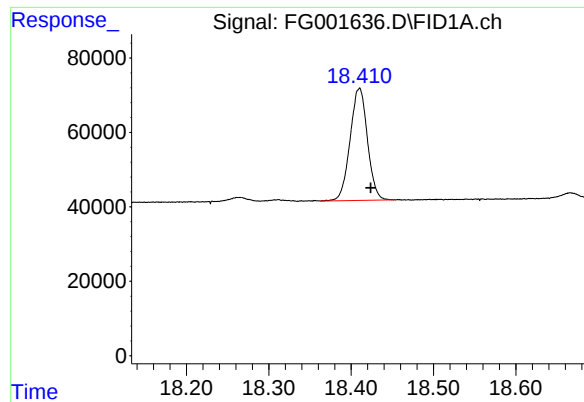

#14 N-DOTRIACONTANE

R.T.: 18.410 min
Delta R.T.: -0.014 min
Response: 441449
Conc: 3.47 ug/ml

Instrument :
FID_F
ClientSampleId :

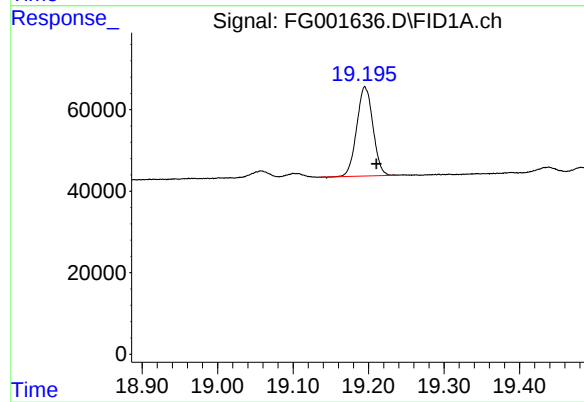

#15 N-TETRATRIACONTANE

R.T.: 19.195 min
Delta R.T.: -0.015 min
Response: 326359
Conc: 2.59 ug/ml