

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071218\
 Data File : FG001646.D
 Signal(s) : FID1A.ch
 Acq On : 12 Jul 2018 20:59
 Operator : AJ\SJ
 Sample : J3857-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 04:16:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.514	2300162	19.770 ug/ml
Target Compounds			
2) N-DECANE	4.203f	321068	2.489 ug/ml
3) N-DODECANE	6.264	200252	1.522 ug/ml
4) N-TETRADECANE	8.055	256990	1.943 ug/ml
5) N-HEXADECANE	9.680	1376118	10.405 ug/ml
6) N-OCTADECANE	11.101	403129	3.014 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071218\
Data File : FG001646.D
Signal(s) : FID1A.ch
Acq On : 12 Jul 2018 20:59
Operator : AJ\SJ
Sample : J3857-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 04:16:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

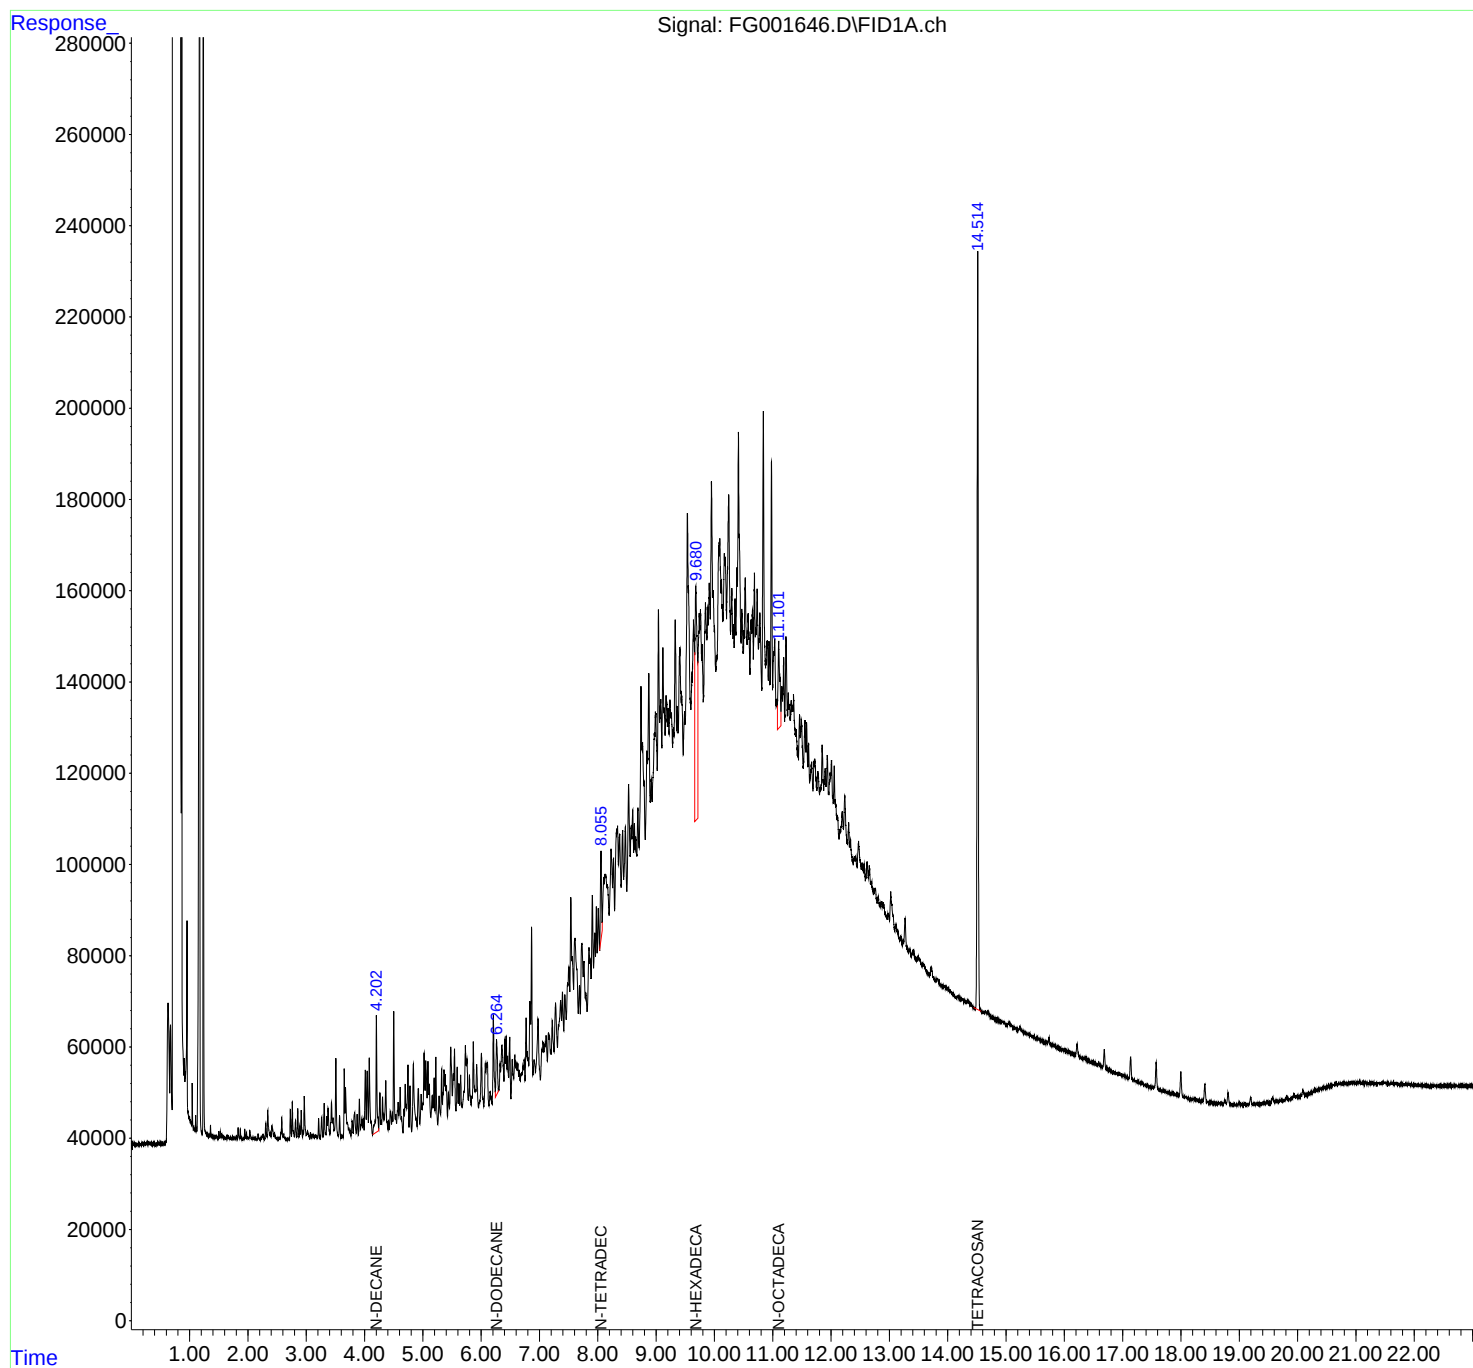


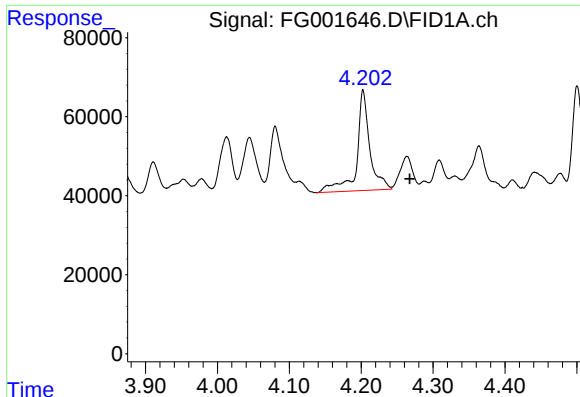

#2 N-DECANE


R.T.: 4.203 min
Delta R.T.: -0.065 min
Response: 321068
Conc: 2.49 ug/ml

Instrument :
FID_F
ClientSampleId :

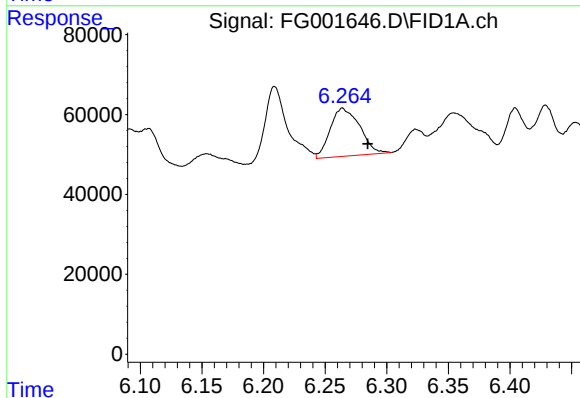


#3 N-DODECANE

R.T.: 6.264 min
Delta R.T.: -0.020 min
Response: 200252
Conc: 1.52 ug/ml

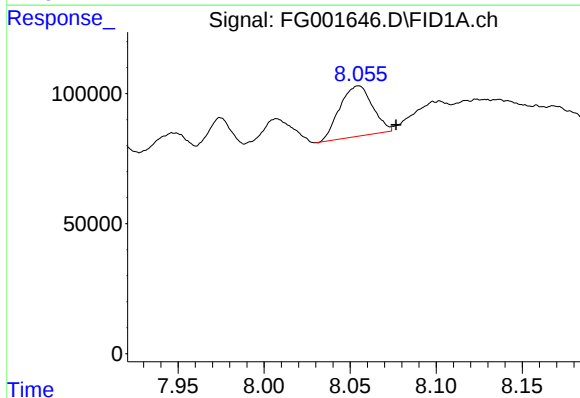


#4 N-TETRADECANE

R.T.: 8.055 min
Delta R.T.: -0.022 min
Response: 256990
Conc: 1.94 ug/ml

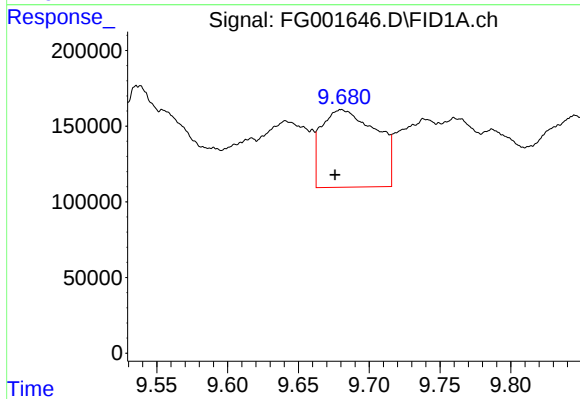

#5 N-HEXADECANE


R.T.: 9.680 min
Delta R.T.: 0.004 min
Response: 1376118
Conc: 10.41 ug/ml

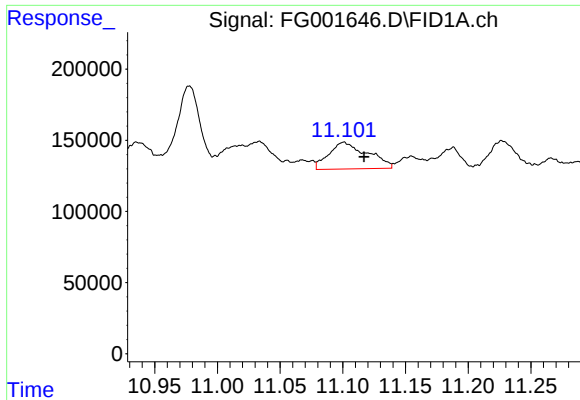

#6 N-OCTADECANE

R.T.: 11.101 min
Delta R.T.: -0.016 min
Response: 403129
Conc: 3.01 ug/ml

Instrument :
FID_F
ClientSampleId :

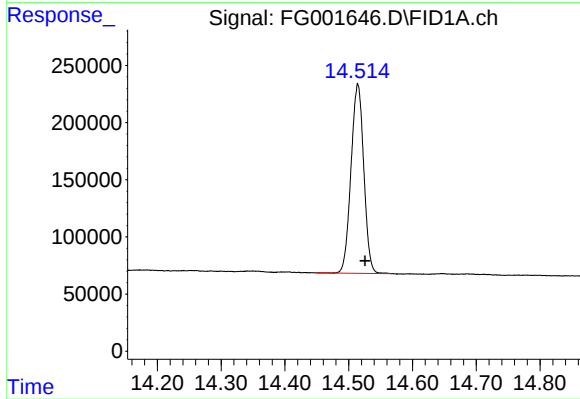

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.514 min
Delta R.T.: -0.011 min
Response: 2300162
Conc: 19.77 ug/ml