

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
 Data File : PS001006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 04:34
 Operator : UA
 Sample : PB111041BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 06:57:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.634	11.050	88037769	75924605	426.705	348.603
Target Compounds							
1) T	Dalapon	0.000	2.416	0	902512	N.D.	3.350 #
2) T	3,5-DICHL...	0.000	9.288	0	45423179	N.D.	154.420 #
3) T	4-Nitroph...	11.205	0.000	37722333	0	275.025	N.D. #
5) T	DICAMBA	0.000	11.397	0	4629039	N.D.	5.897 #
6) T	MCPD	12.329	0.000	9036808	0	16.452	N.D. #
7) T	MCPA	12.604	0.000	13521588	0	14.816	N.D. #
8) T	DICHLORPROP	0.000	12.417	0	1990242	N.D.	9.854 #
13) T	2,4-DB	15.915	0.000	6843357	0	42.273	N.D. #
14) T	DINOSEB	0.000	15.747	0	6631936	N.D.	7.919 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
Data File : PS001006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 04:34
Operator : UA
Sample : PB111041BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 06:57:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

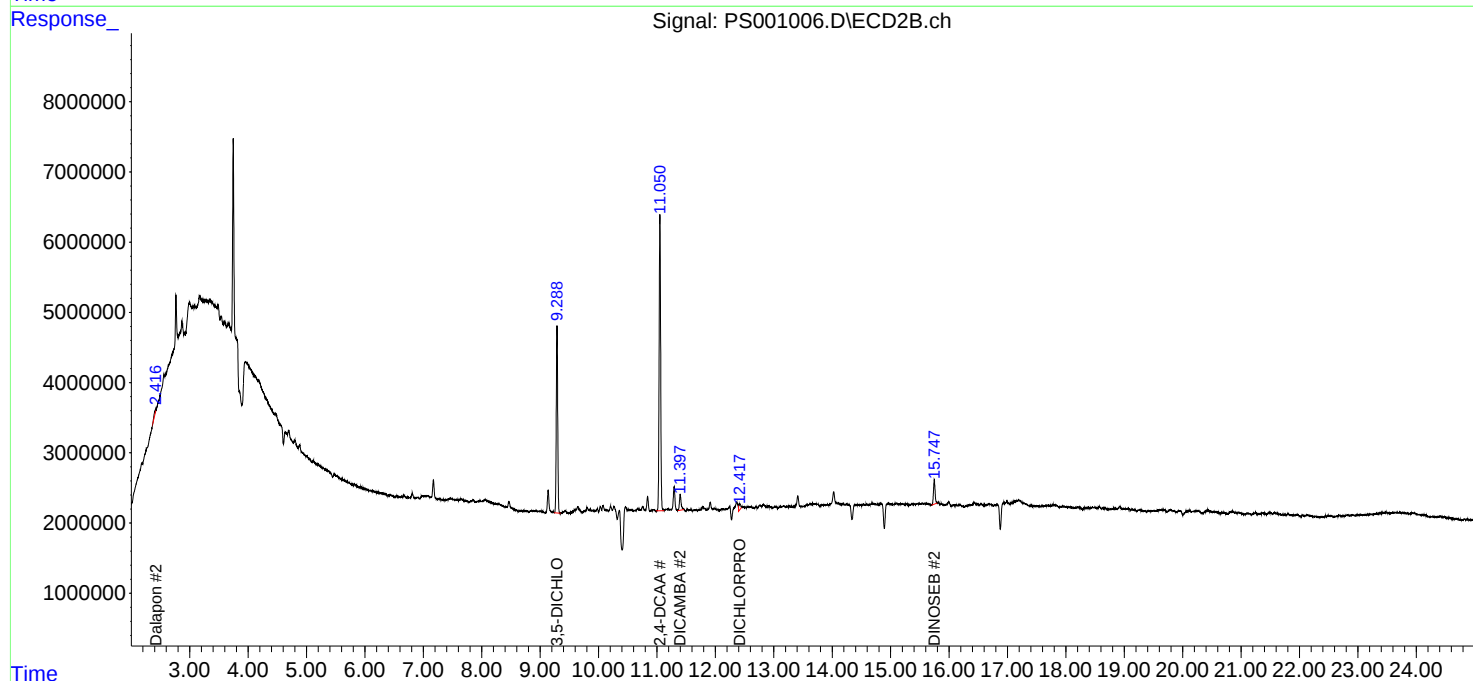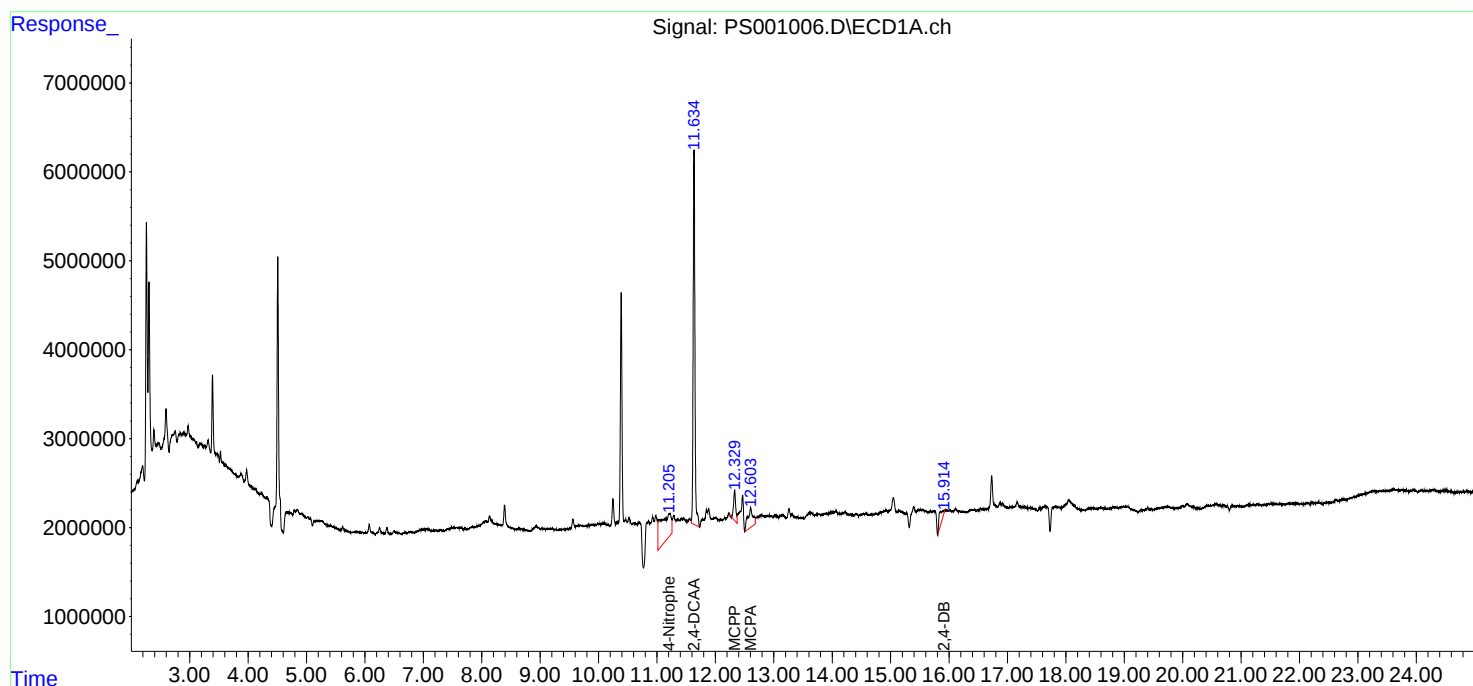


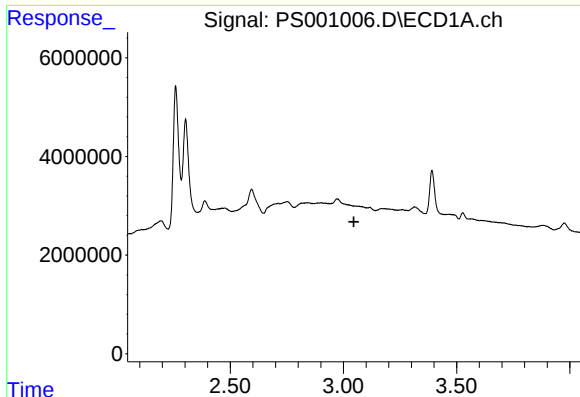

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.046 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

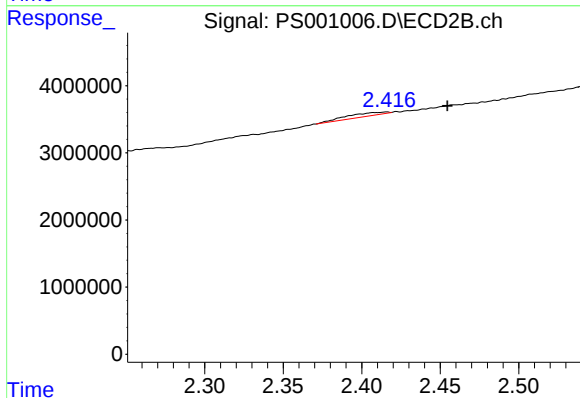


#1 Dalapon

R.T.: 2.416 min
Delta R.T.: -0.038 min
Response: 902512
Conc: 3.35 ng/ml

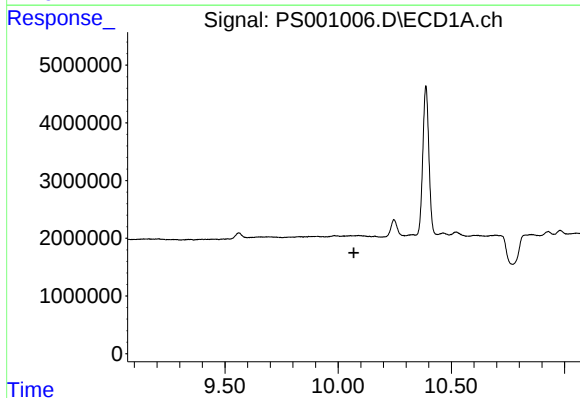


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

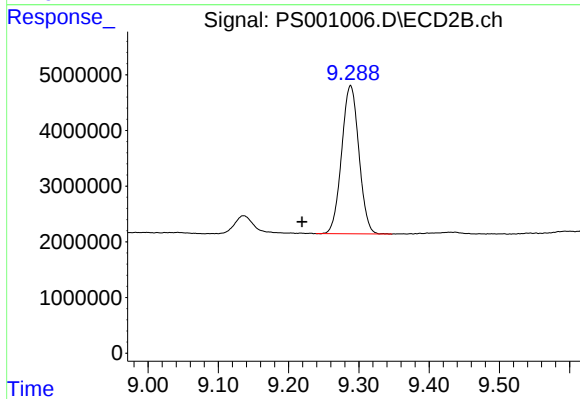

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.288 min
Delta R.T.: 0.069 min
Response: 45423179
Conc: 154.42 ng/ml

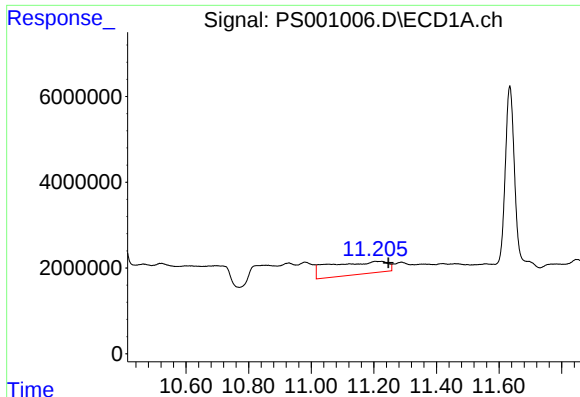

#3 4-Nitrophenol


R.T.: 11.205 min
Delta R.T.: -0.041 min
Response: 37722333
Conc: 275.02 ng/ml

Instrument :
FID_F
ClientSampleId :

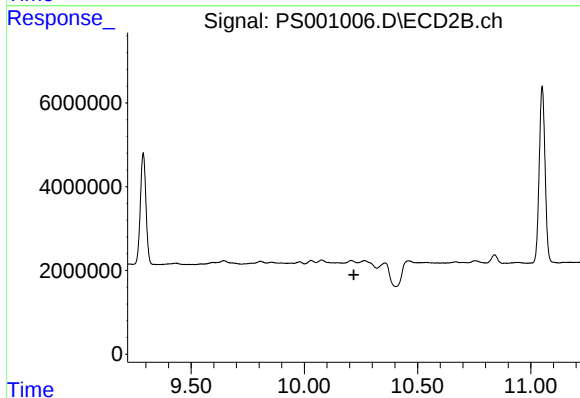


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.219 min
Response: 0
Conc: N.D.

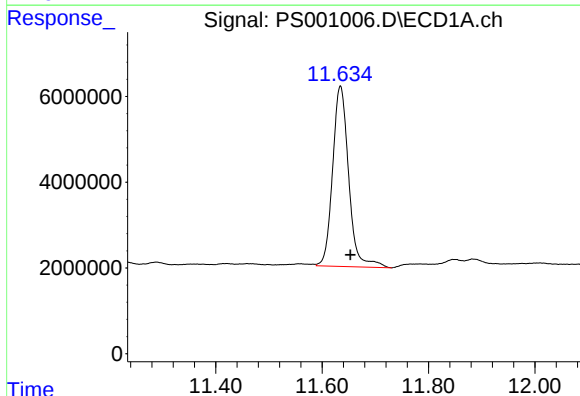


#4 2,4-DCAA

R.T.: 11.634 min
Delta R.T.: -0.019 min
Response: 88037769
Conc: 426.70 ng/ml

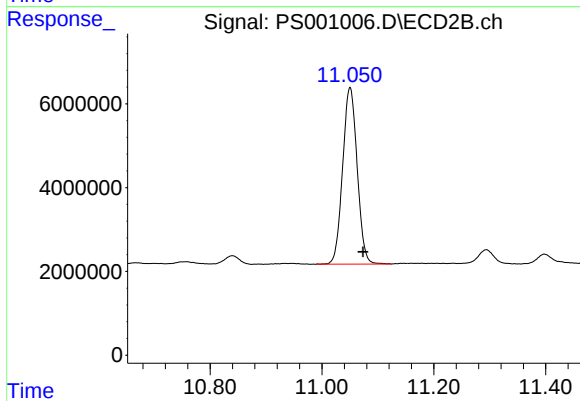

#4 2,4-DCAA


R.T.: 11.050 min
Delta R.T.: -0.023 min
Response: 75924605
Conc: 348.60 ng/ml

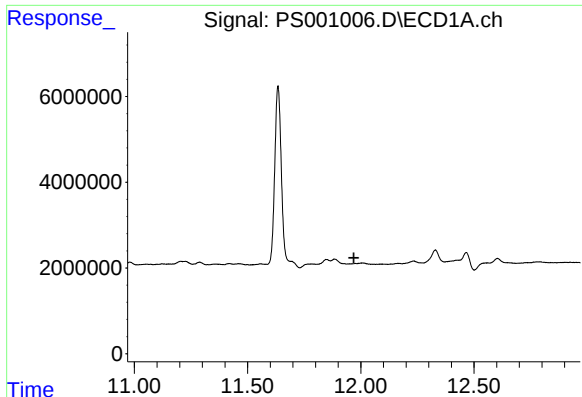

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

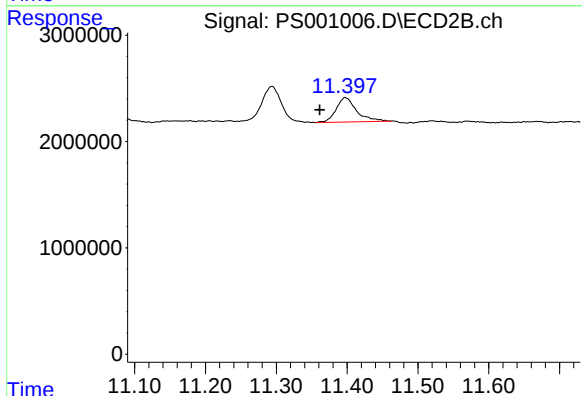


#5 DICAMBA

R.T.: 11.397 min
Delta R.T.: 0.036 min
Response: 4629039
Conc: 5.90 ng/ml

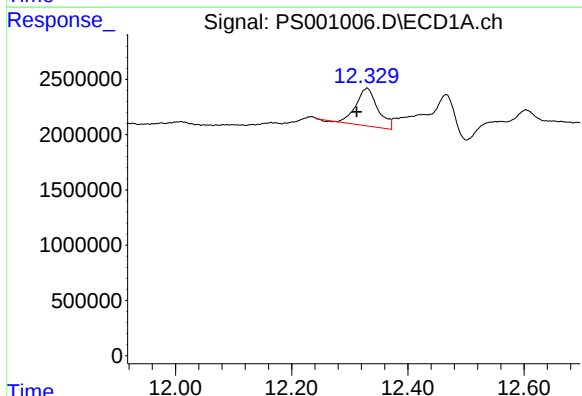


#6 MCP

R.T.: 12.329 min
Delta R.T.: 0.017 min
Response: 9036808
Conc: 16.45 ug/ml

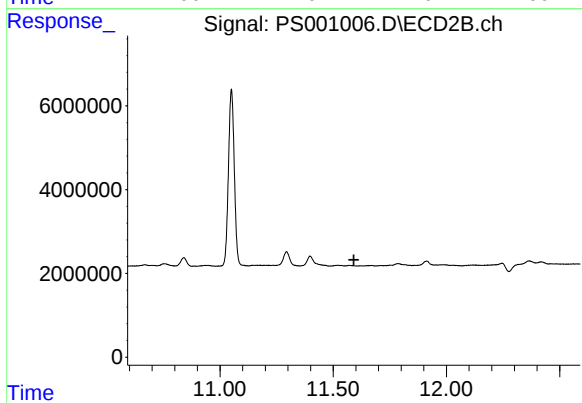

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

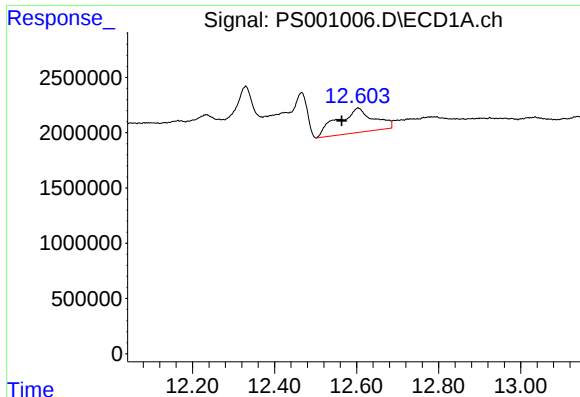

#7 MCPA


R.T.: 12.604 min
Delta R.T.: 0.040 min
Response: 13521588
Conc: 14.82 ug/ml

Instrument :
FID_F
ClientSampleId :

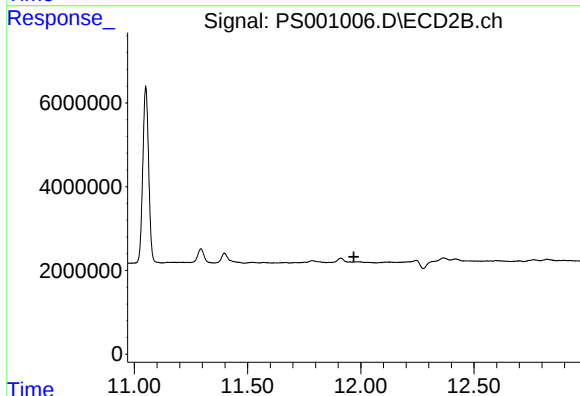


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

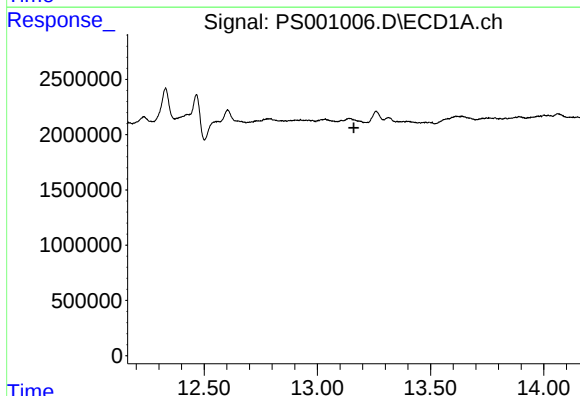


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

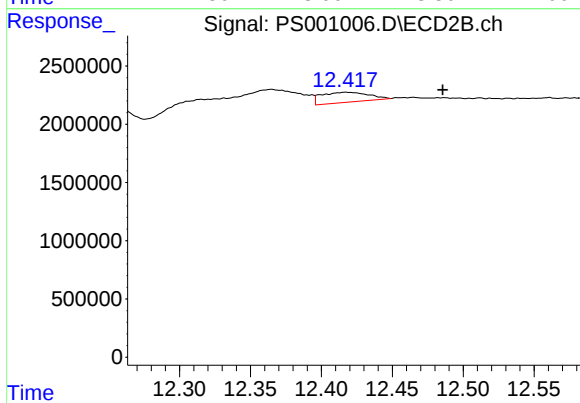

#8 DICHLORPROP


R.T.: 12.417 min
Delta R.T.: -0.068 min
Response: 1990242
Conc: 9.85 ng/ml

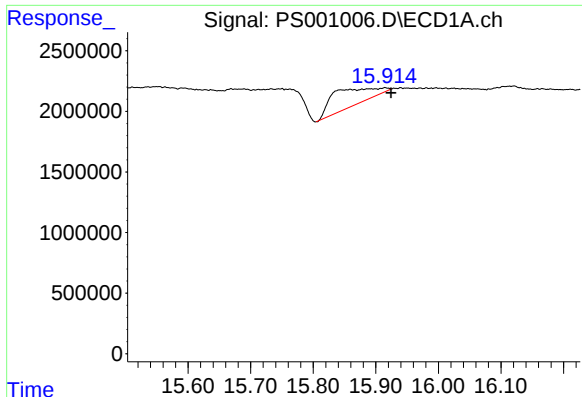

#13 2,4-DB


R.T.: 15.915 min
Delta R.T.: -0.009 min
Response: 6843357
Conc: 42.27 ng/ml

Instrument :
FID_F
ClientSampleId :

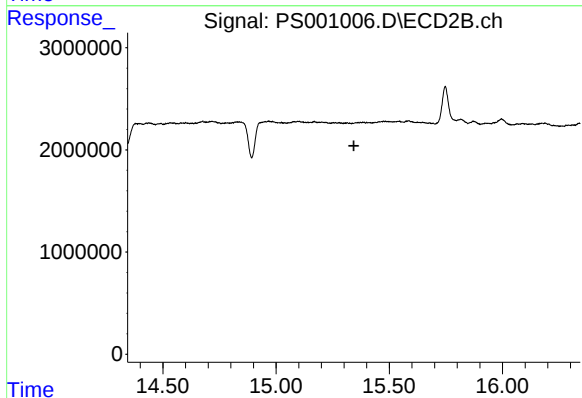


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.344 min
Response: 0
Conc: N.D.

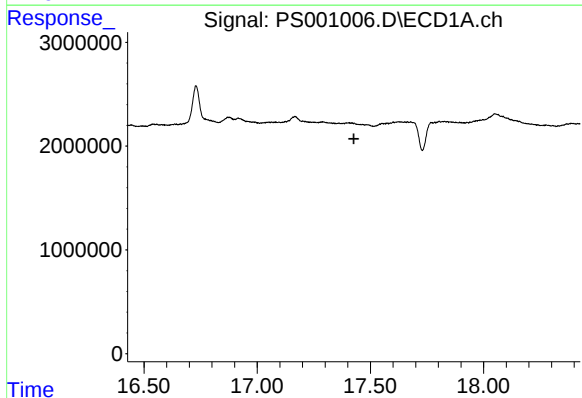

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.427 min
Response: 0
Conc: N.D.

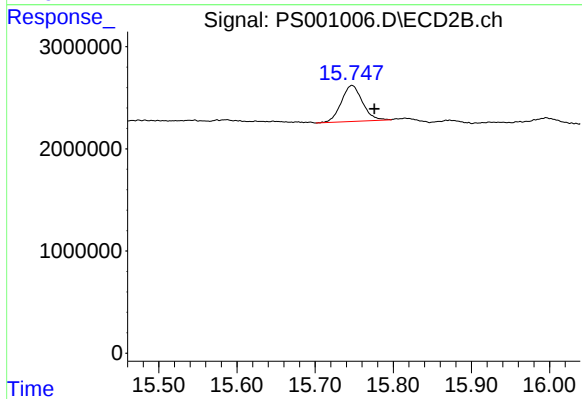

#14 DINOSEB

R.T.: 15.747 min
Delta R.T.: -0.029 min
Response: 6631936
Conc: 7.92 ng/ml