

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
 Data File : PS001007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 05:05
 Operator : UA
 Sample : PB111041BS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 06:57:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.631	11.046	94816111	86684120	459.558	398.004
Target Compounds							
1) T	Dalapon	3.017	2.428	87344690	83044921	325.296	308.228
2) T	3,5-DICHL...	10.046	9.192	117.4E6	106.9E6	392.050	363.365
3) T	4-Nitroph...	11.223	10.191	48859770	49558893	356.225	410.715
5) T	DICAMBA	11.947	11.333	317.2E6	304.7E6	402.818	388.132
6) T	MCPD	12.330	11.606	6291796	10265850	11.454	19.633 #
7) T	MCPA	12.534	11.932	30416080	24713806	33.328	31.795
8) T	DICHLORPROP	13.138	12.458	85778703	87150412	425.562	431.486
9) T	2,4-D	13.496	12.930	109.1E6	110.5E6	400.801	398.816
10) T	Pentachlo...	13.886	13.485	1265.7E6	1219.8E6	416.759	388.643
11) T	2,4,5-TP ...	14.755	14.099	492.1E6	491.2E6	402.798	391.421
12) T	2,4,5-T	15.152	14.669	483.2E6	397.6E6	396.792	384.259
13) T	2,4-DB	15.903	15.315	77445489	59357738	478.400	387.503
14) T	DINOSEB	17.404	15.746	308.8E6	289.2E6	357.023	345.296
15) T	Picloram	17.162	16.985	591.0E6	551.2E6	326.337	361.961
16) T	DCPA	17.745	16.985	402.1E6	551.2E6	276.192	320.595



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
Data File : PS001007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 05:05
Operator : UA
Sample : PB111041BS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 06:57:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

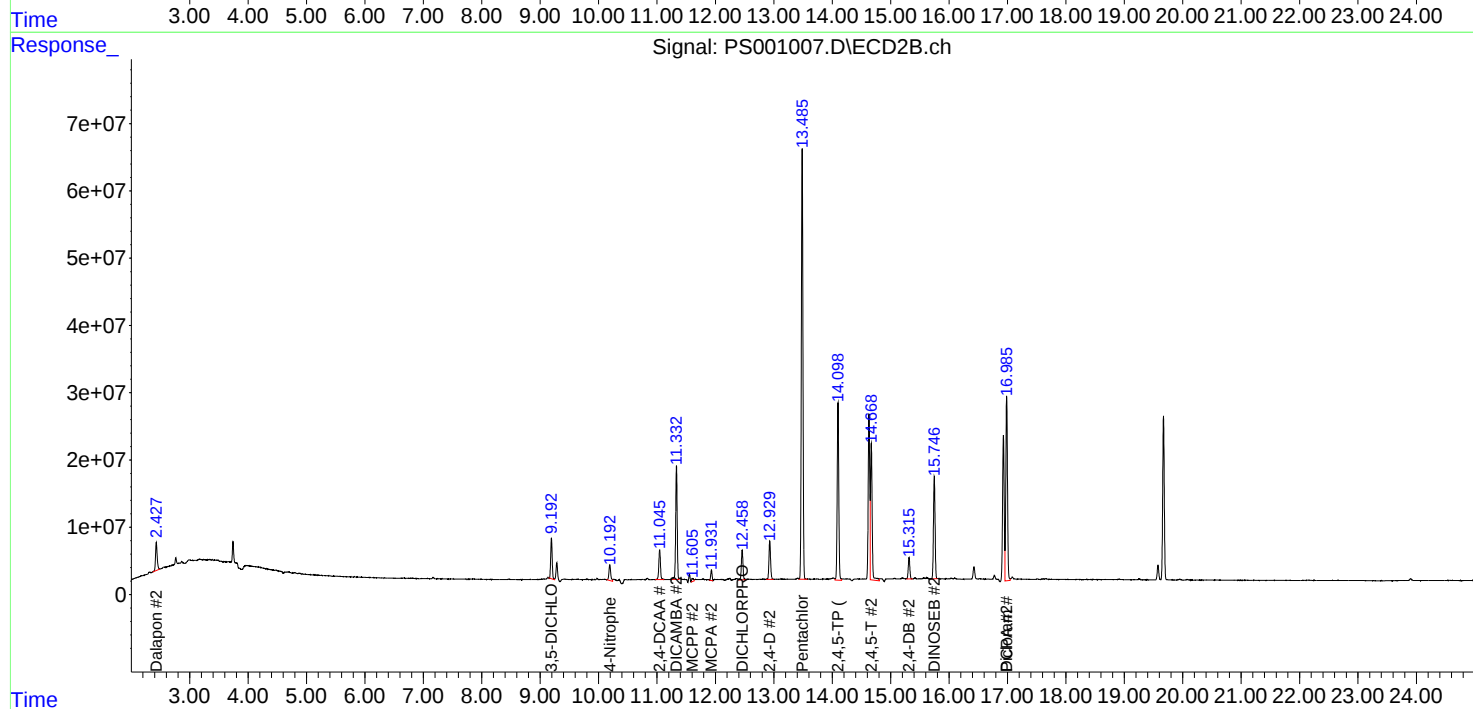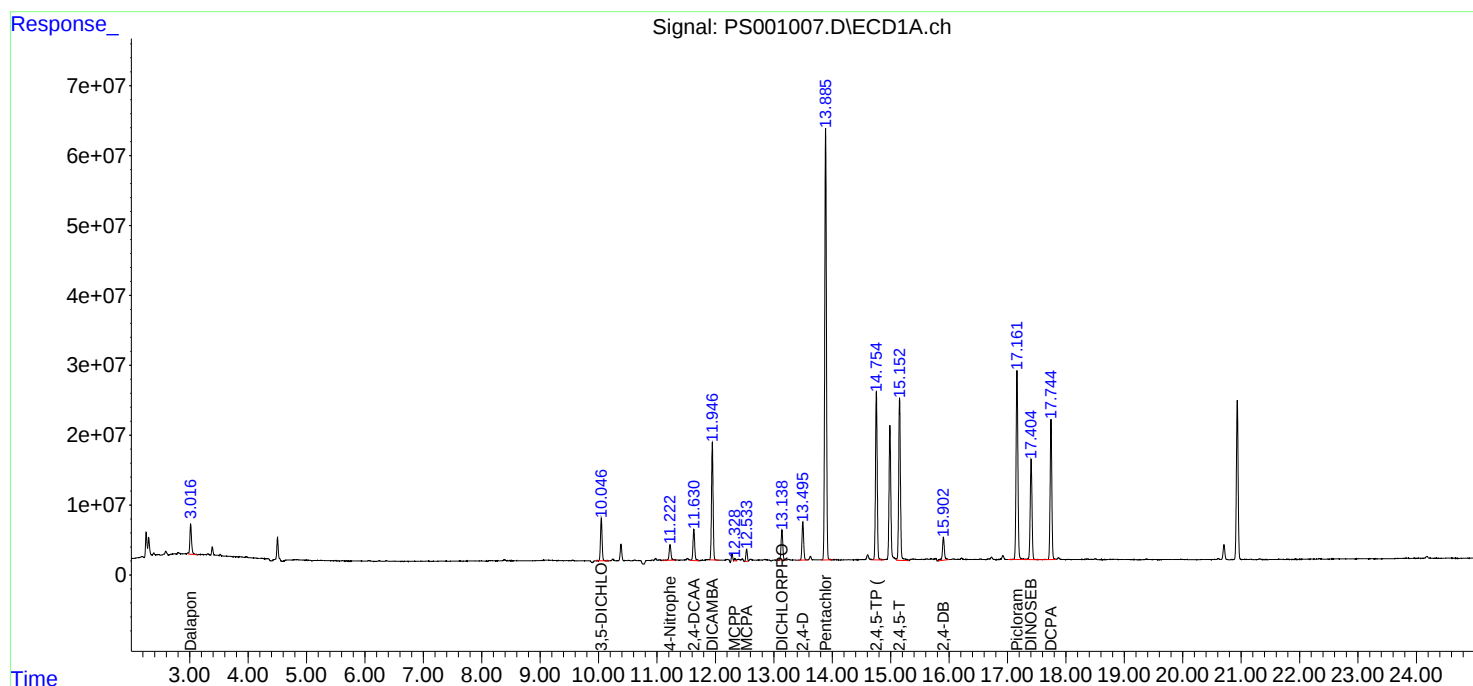


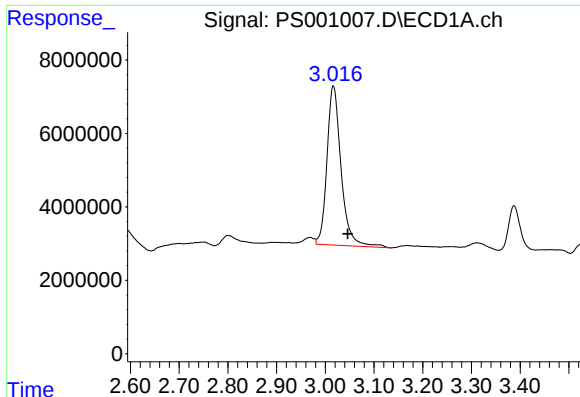

#1 Dalapon


R.T.: 3.017 min
Delta R.T.: -0.029 min
Response: 87344690
Conc: 325.30 ng/ml

Instrument :
FID_F
ClientSampleId :

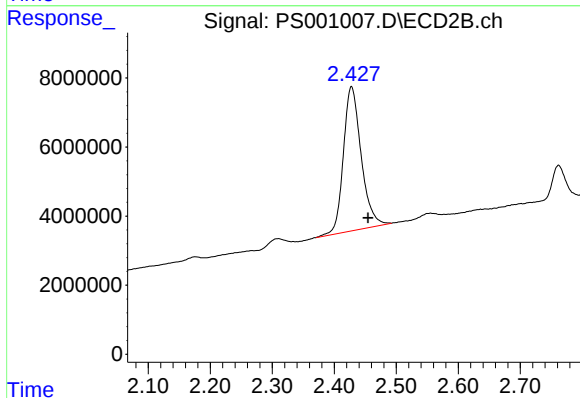


#1 Dalapon

R.T.: 2.428 min
Delta R.T.: -0.027 min
Response: 83044921
Conc: 308.23 ng/ml

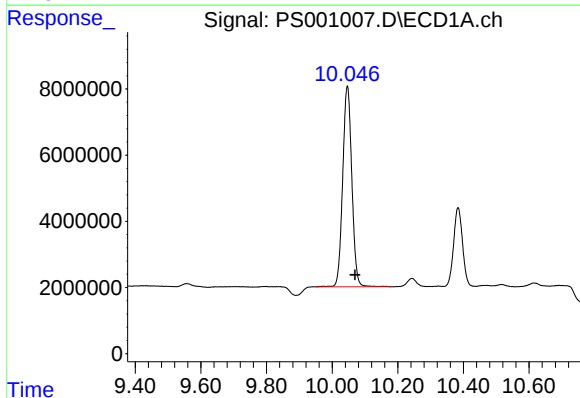


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.046 min
Delta R.T.: -0.023 min
Response: 117426315
Conc: 392.05 ng/ml

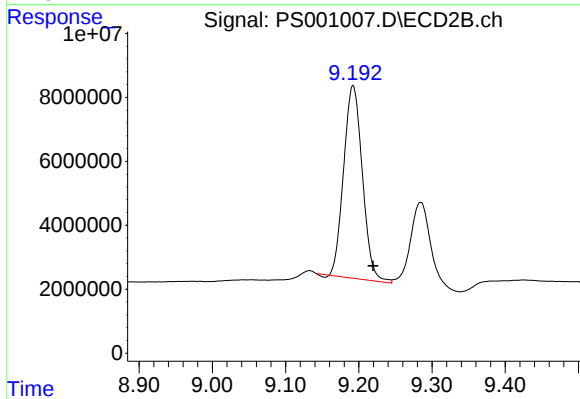

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.192 min
Delta R.T.: -0.027 min
Response: 106885190
Conc: 363.37 ng/ml

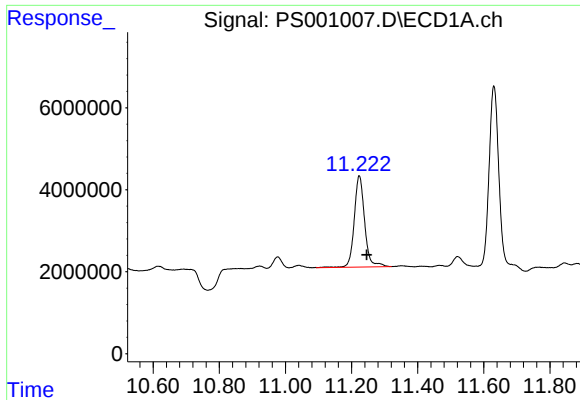

#3 4-Nitrophenol


R.T.: 11.223 min
Delta R.T.: -0.023 min
Response: 48859770
Conc: 356.23 ng/ml

Instrument :
FID_F
ClientSampleId :

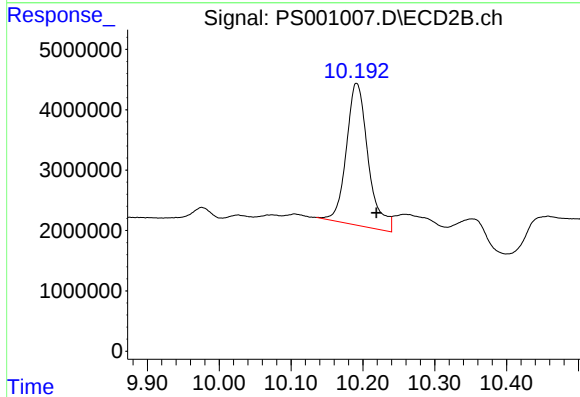


#3 4-Nitrophenol

R.T.: 10.191 min
Delta R.T.: -0.028 min
Response: 49558893
Conc: 410.71 ng/ml

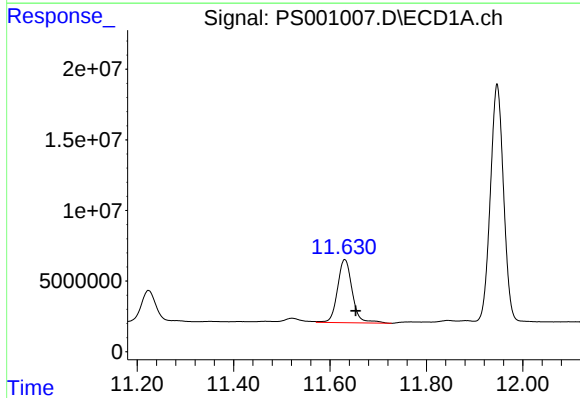


#4 2,4-DCAA

R.T.: 11.631 min
Delta R.T.: -0.023 min
Response: 94816111
Conc: 459.56 ng/ml

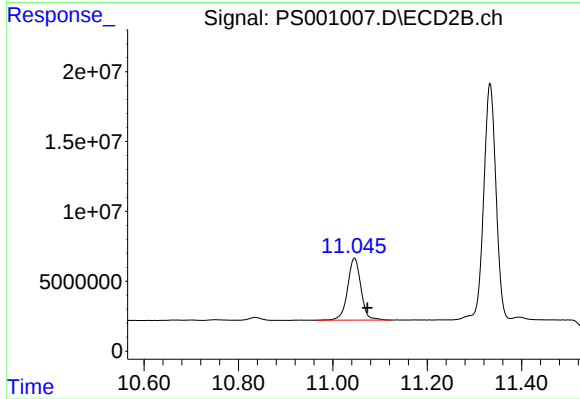

#4 2,4-DCAA


R.T.: 11.046 min
Delta R.T.: -0.028 min
Response: 86684120
Conc: 398.00 ng/ml

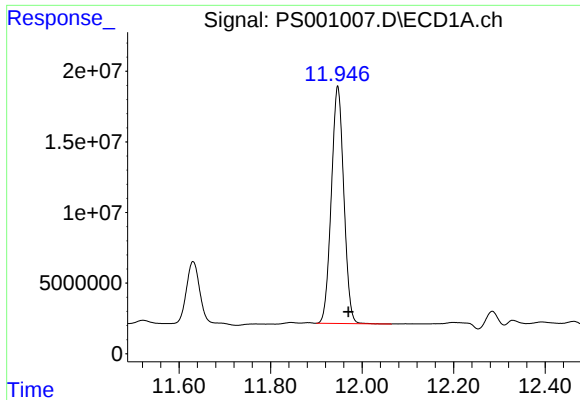

#5 DICAMBA


R.T.: 11.947 min
Delta R.T.: -0.023 min
Response: 317168564
Conc: 402.82 ng/ml

Instrument :
FID_F
ClientSampleId :

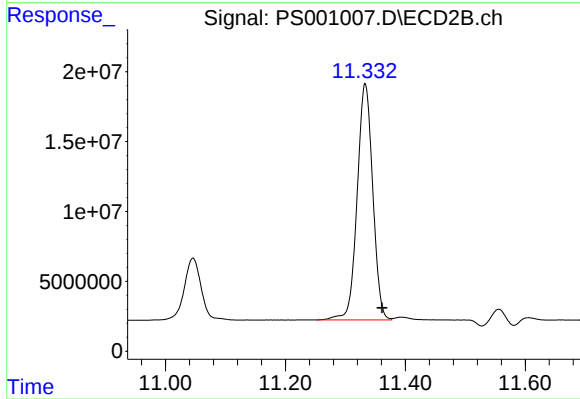


#5 DICAMBA

R.T.: 11.333 min
Delta R.T.: -0.028 min
Response: 304660843
Conc: 388.13 ng/ml

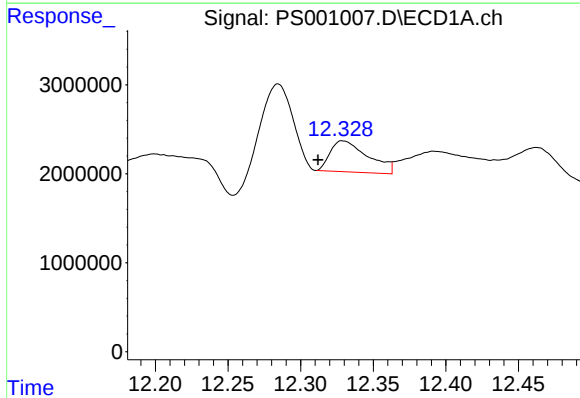


#6 MCP

R.T.: 12.330 min
Delta R.T.: 0.017 min
Response: 6291796
Conc: 11.45 ug/ml

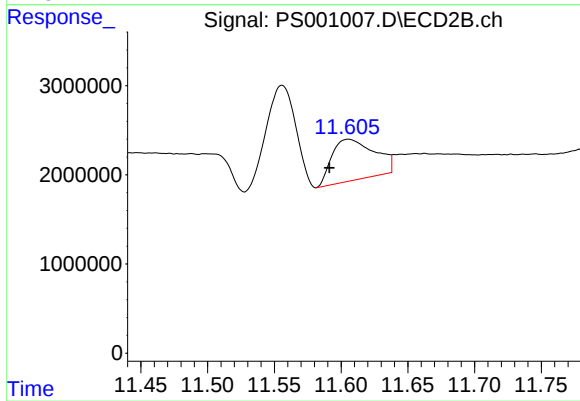

#6 MCP


R.T.: 11.606 min
Delta R.T.: 0.014 min
Response: 10265850
Conc: 19.63 ug/ml

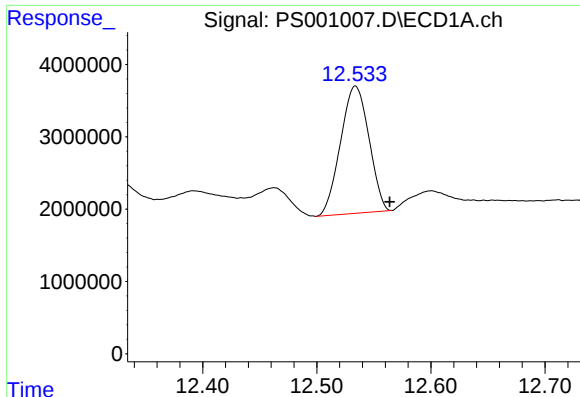

#7 MCPA


R.T.: 12.534 min
Delta R.T.: -0.030 min
Response: 30416080
Conc: 33.33 ug/ml

Instrument :
FID_F
ClientSampleId :

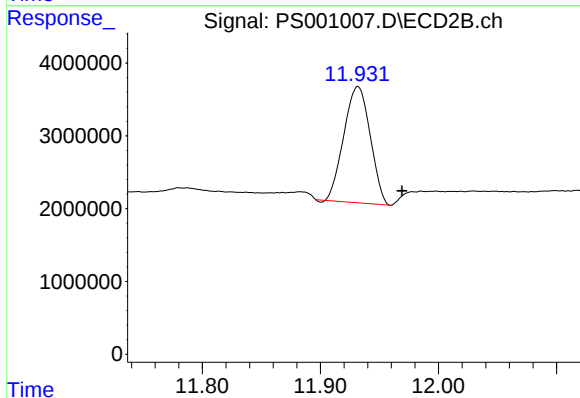


#7 MCPA

R.T.: 11.932 min
Delta R.T.: -0.038 min
Response: 24713806
Conc: 31.79 ug/ml

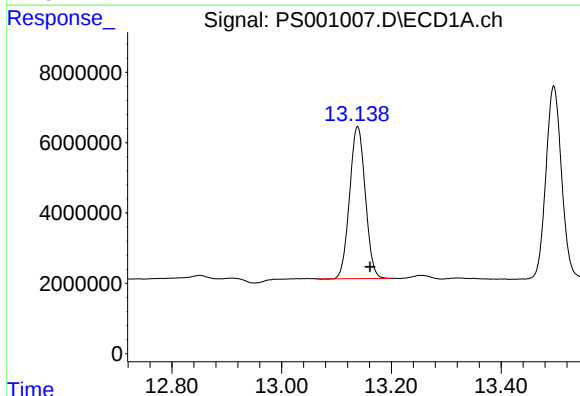


#8 DICHLORPROP

R.T.: 13.138 min
Delta R.T.: -0.023 min
Response: 85778703
Conc: 425.56 ng/ml

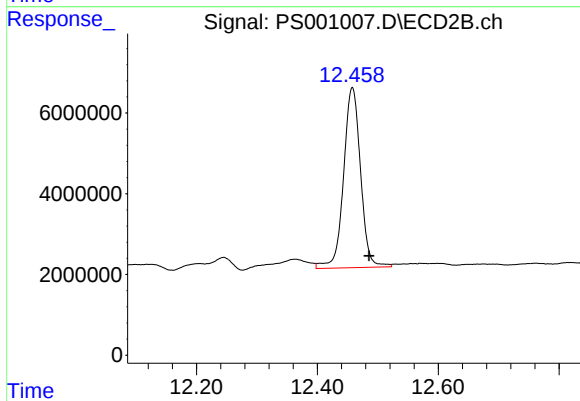

#8 DICHLORPROP


R.T.: 12.458 min
Delta R.T.: -0.028 min
Response: 87150412
Conc: 431.49 ng/ml

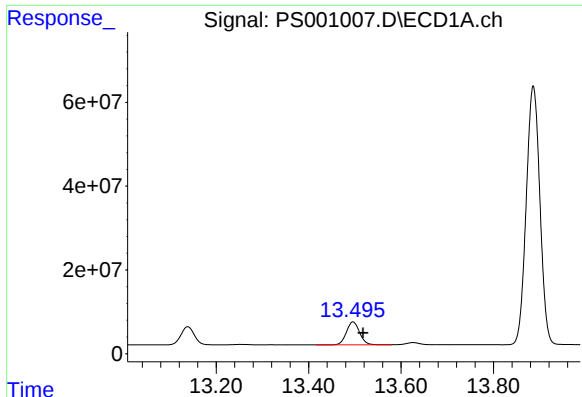

#9 2,4-D


R.T.: 13.496 min
Delta R.T.: -0.022 min
Response: 109093495
Conc: 400.80 ng/ml

Instrument :
FID_F
ClientSampleId :

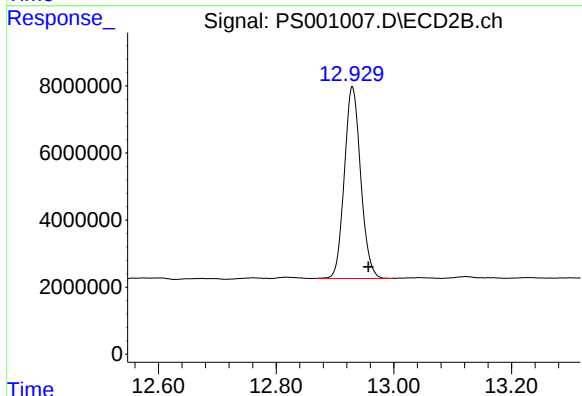


#9 2,4-D

R.T.: 12.930 min
Delta R.T.: -0.027 min
Response: 110456022
Conc: 398.82 ng/ml

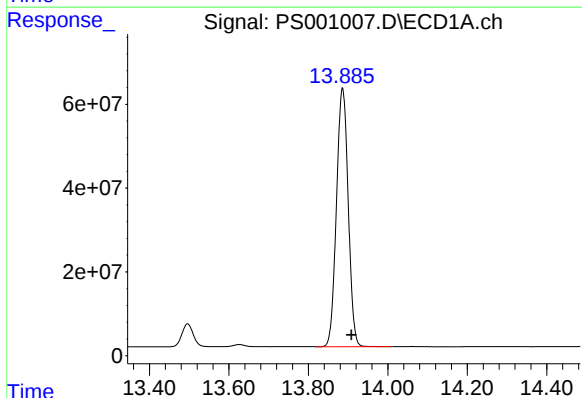


#10 Pentachlorophenol

R.T.: 13.886 min
Delta R.T.: -0.022 min
Response: 1265745016
Conc: 416.76 ng/ml

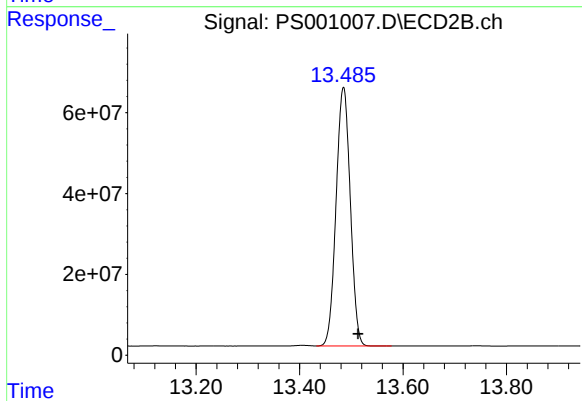

#10 Pentachlorophenol


R.T.: 13.485 min
Delta R.T.: -0.028 min
Response: 1219762732
Conc: 388.64 ng/ml

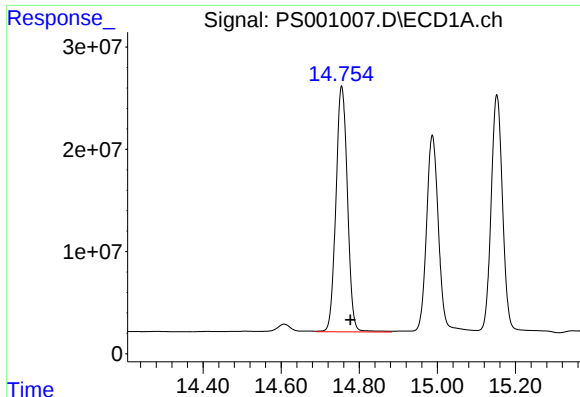

#11 2,4,5-TP (SILVEX)


R.T.: 14.755 min
Delta R.T.: -0.022 min
Response: 492108556
Conc: 402.80 ng/ml

Instrument :
FID_F
ClientSampleId :

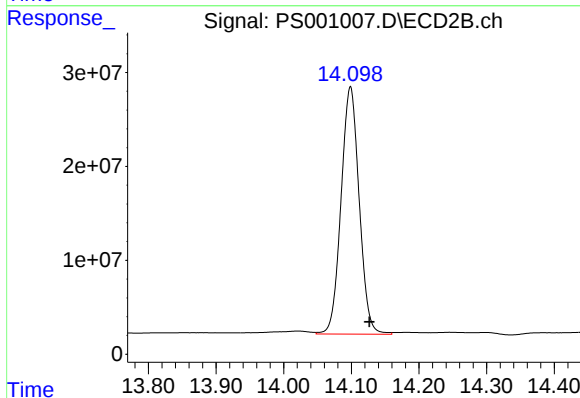


#11 2,4,5-TP (SILVEX)

R.T.: 14.099 min
Delta R.T.: -0.028 min
Response: 491204789
Conc: 391.42 ng/ml

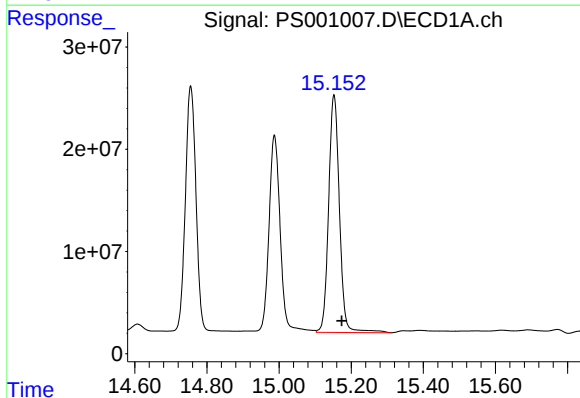


#12 2,4,5-T

R.T.: 15.152 min
Delta R.T.: -0.022 min
Response: 483182166
Conc: 396.79 ng/ml

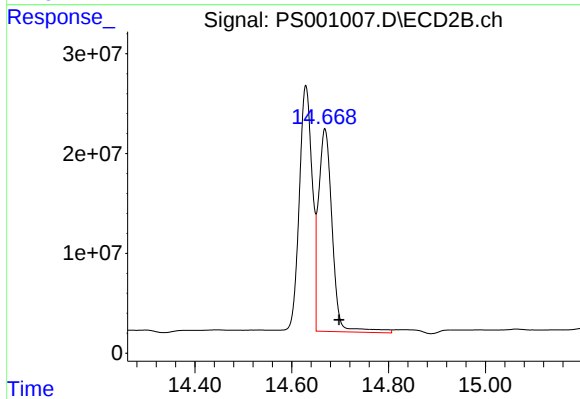

#12 2,4,5-T


R.T.: 14.669 min
Delta R.T.: -0.029 min
Response: 397591312
Conc: 384.26 ng/ml

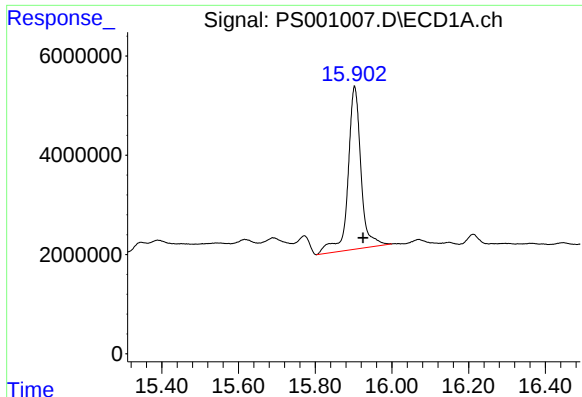

#13 2,4-DB


R.T.: 15.903 min
Delta R.T.: -0.022 min
Response: 77445489
Conc: 478.40 ng/ml

Instrument :
FID_F
ClientSampleId :

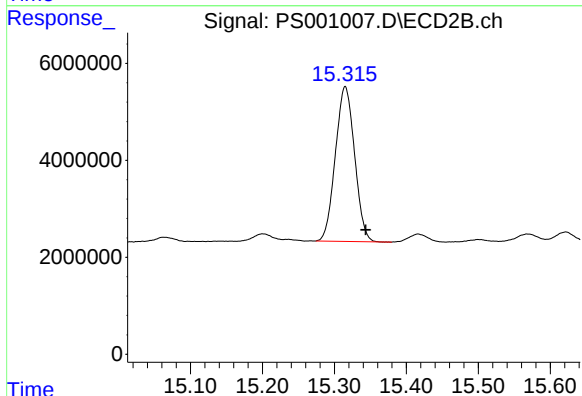


#13 2,4-DB

R.T.: 15.315 min
Delta R.T.: -0.028 min
Response: 59357738
Conc: 387.50 ng/ml

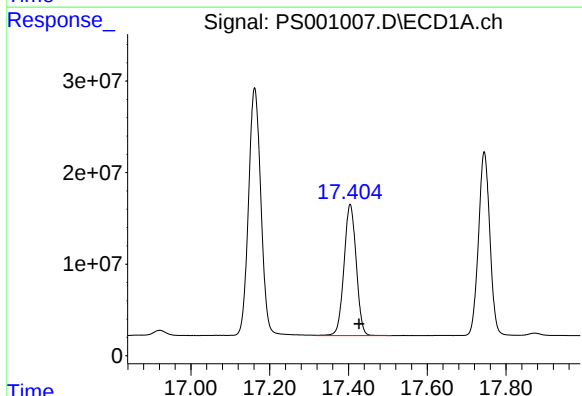


#14 DINOSEB

R.T.: 17.404 min
Delta R.T.: -0.022 min
Response: 308768825
Conc: 357.02 ng/ml

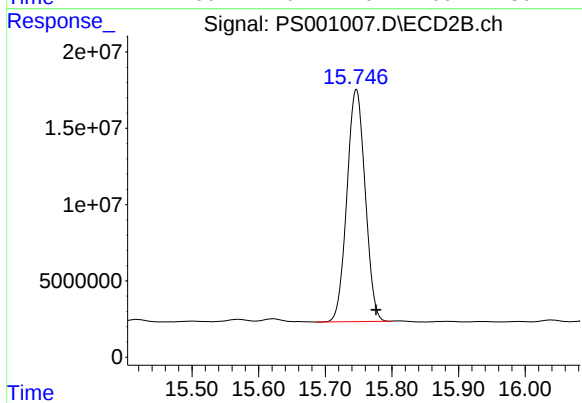

#14 DINOSEB


R.T.: 15.746 min
Delta R.T.: -0.029 min
Response: 289181407
Conc: 345.30 ng/ml

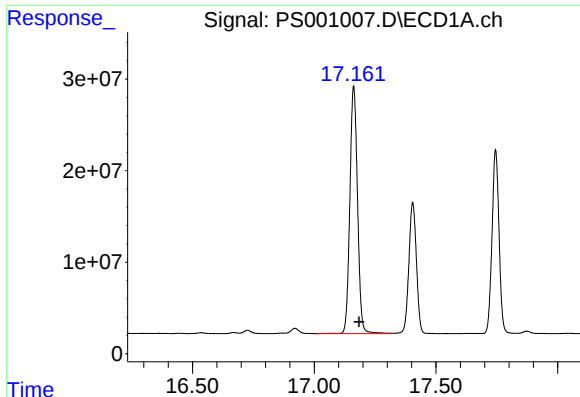

#15 Picloram


R.T.: 17.162 min
Delta R.T.: -0.022 min
Response: 591013594
Conc: 326.34 ng/ml

Instrument :
FID_F
ClientSampleId :

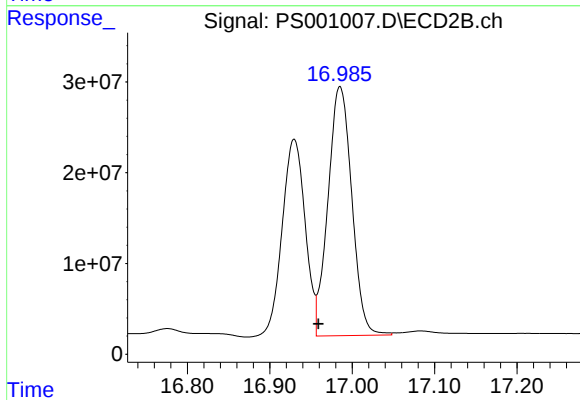


#15 Picloram

R.T.: 16.985 min
Delta R.T.: 0.026 min
Response: 551150626
Conc: 361.96 ng/ml

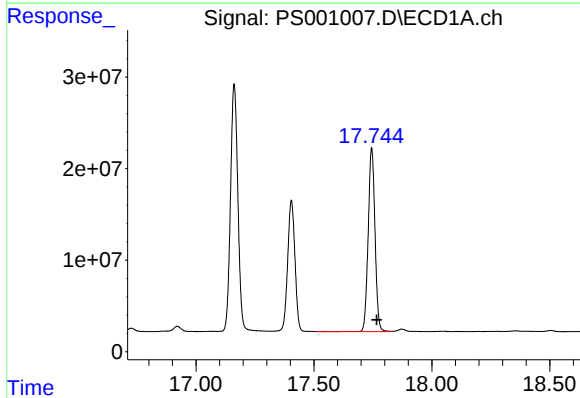

#16 DCPA

R.T.: 17.745 min
Delta R.T.: -0.021 min
Response: 402085046
Conc: 276.19 ng/ml

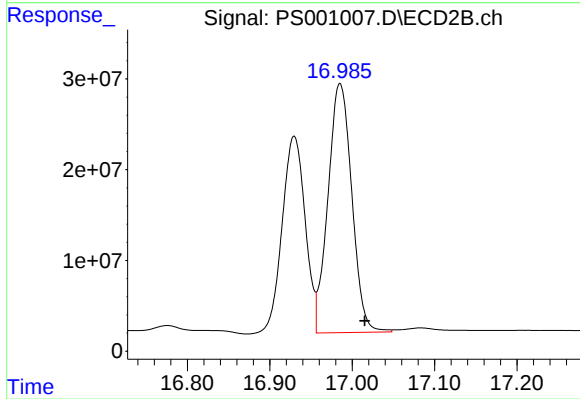

#16 DCPA

R.T.: 16.985 min
Delta R.T.: -0.030 min
Response: 551150626
Conc: 320.60 ng/ml