

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
 Data File : PS001008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 05:36
 Operator : UA
 Sample : PB111041TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 06:58:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.649	11.064	56148005	47301815	272.140	217.183
Target Compounds							
1) T	Dalapon	2.987	0.000	3617903	0	13.474	N.D. #
5) T	DICAMBA	0.000	11.307	0	7026748	N.D.	8.952 #
6) T	MCPD	12.344	0.000	7920549	0	14.419	N.D. #
8) T	DICHLORPROP	0.000	12.435	0	1576883	N.D.	7.807 #
14) T	DINOSEB	0.000	15.823	0	2488056	N.D.	2.971 #
15) T	Picloram	17.180	17.001	2652031	7402902	1.464	4.862 #
16) T	DCPA	0.000	17.001	0	7402902	N.D.	4.306 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
Data File : PS001008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 05:36
Operator : UA
Sample : PB111041TB
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 06:58:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

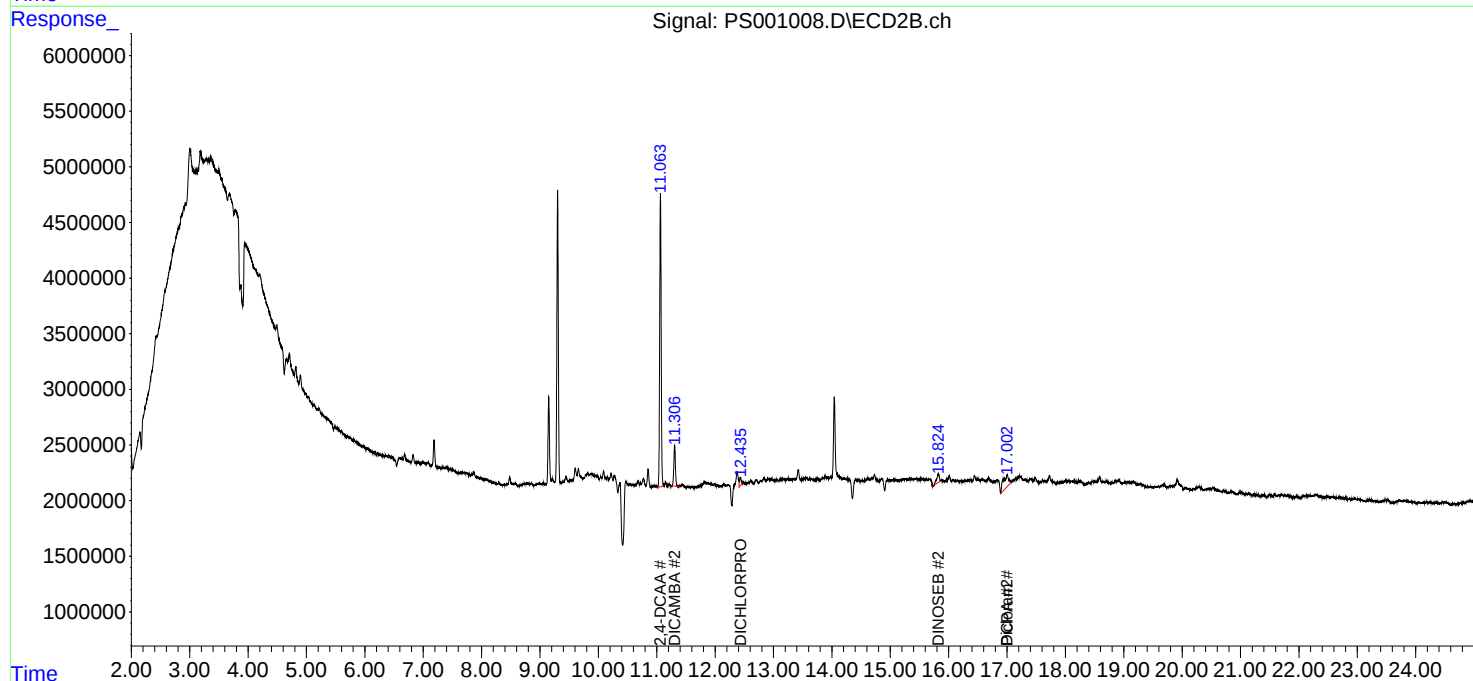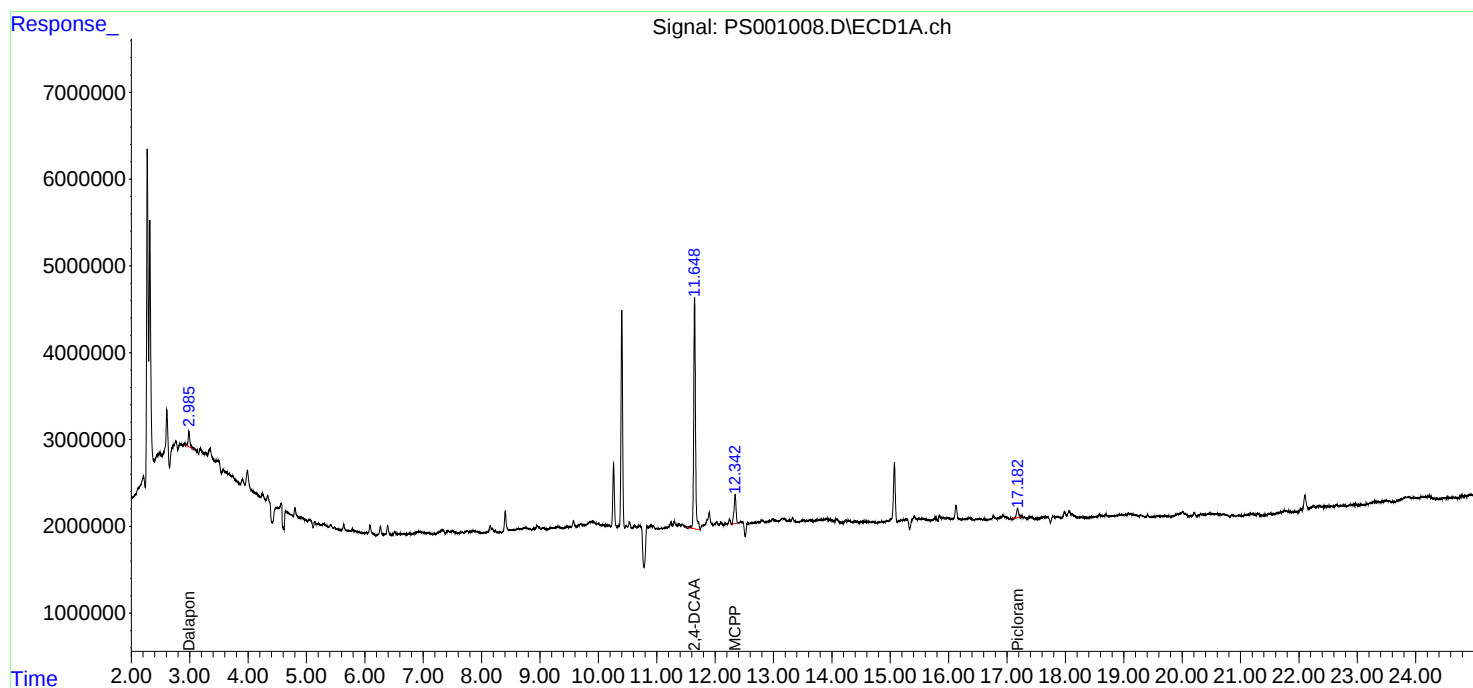


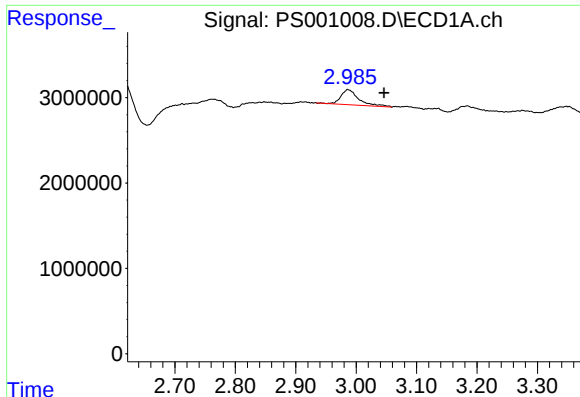

#1 Dalapon


R.T.: 2.987 min
Delta R.T.: -0.059 min
Response: 3617903
Conc: 13.47 ng/ml

Instrument :
FID_F
ClientSampleId :

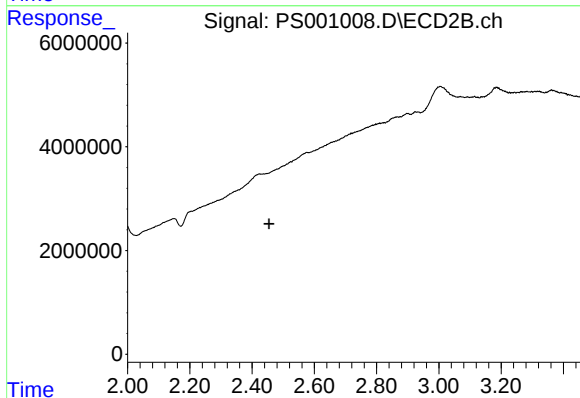


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.455 min
Response: 0
Conc: N.D.

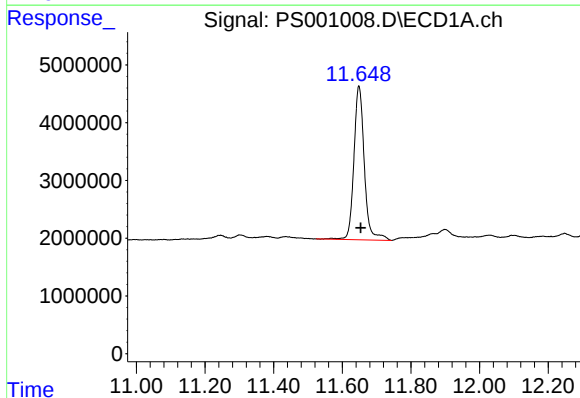


#4 2,4-DCAA

R.T.: 11.649 min
Delta R.T.: -0.005 min
Response: 56148005
Conc: 272.14 ng/ml

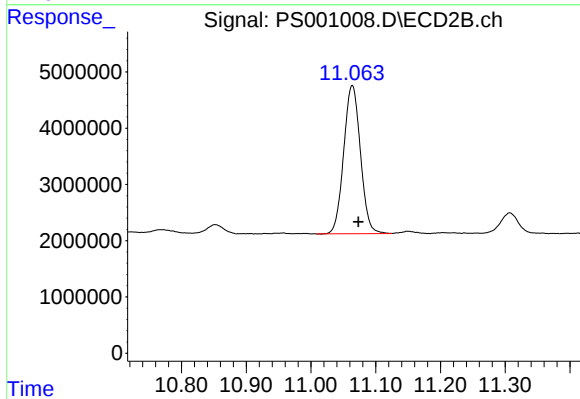

#4 2,4-DCAA


R.T.: 11.064 min
Delta R.T.: -0.010 min
Response: 47301815
Conc: 217.18 ng/ml

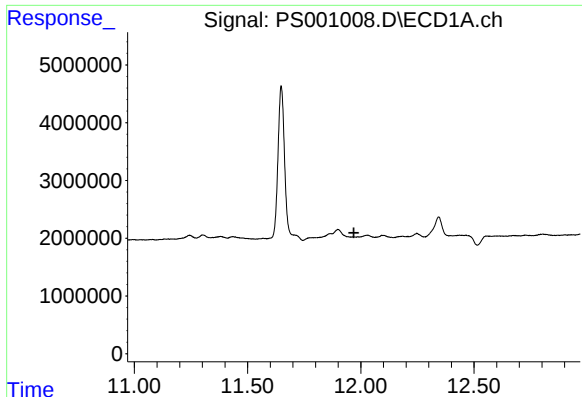

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

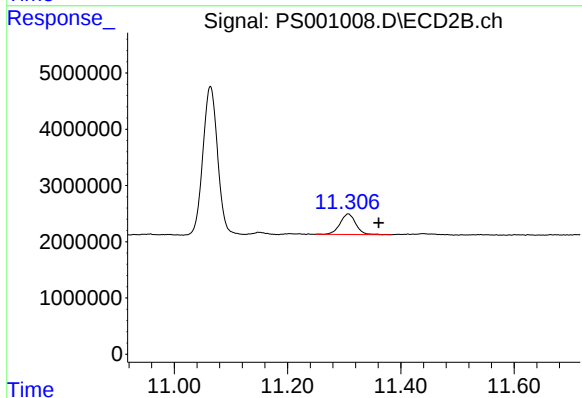


#5 DICAMBA

R.T.: 11.307 min
Delta R.T.: -0.054 min
Response: 7026748
Conc: 8.95 ng/ml

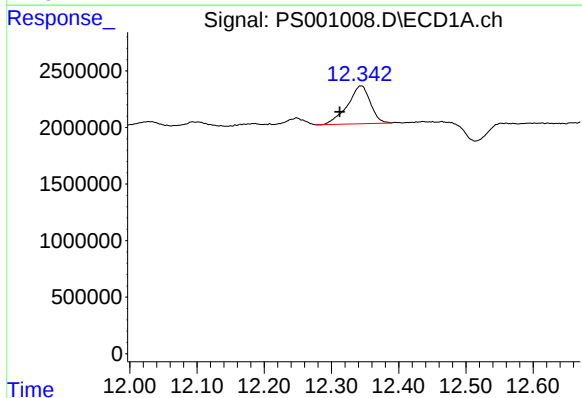


#6 MCPP

R.T.: 12.344 min
Delta R.T.: 0.032 min
Response: 7920549
Conc: 14.42 ug/ml

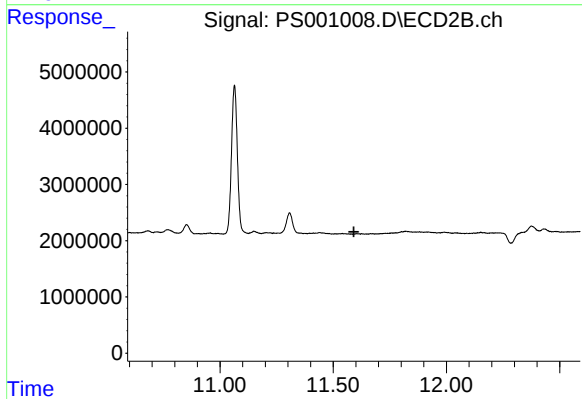

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

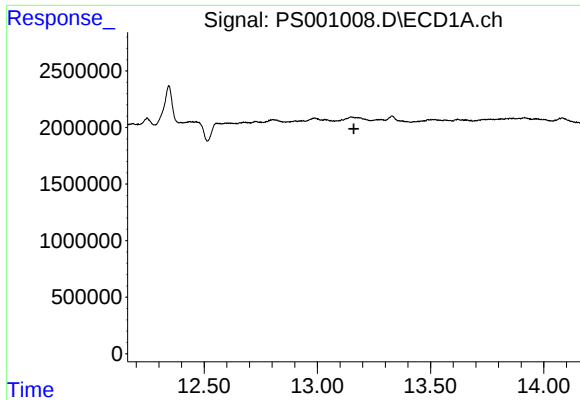

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

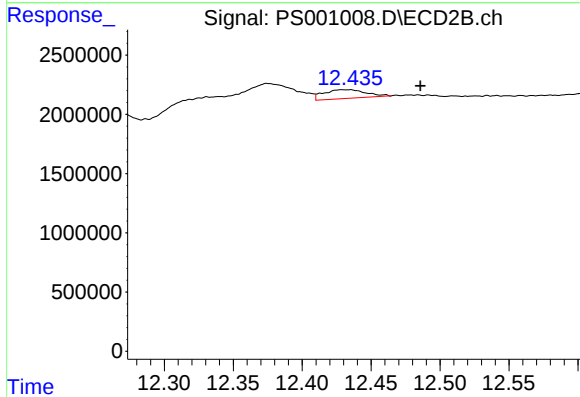


#8 DICHLORPROP

R.T.: 12.435 min
Delta R.T.: -0.051 min
Response: 1576883
Conc: 7.81 ng/ml

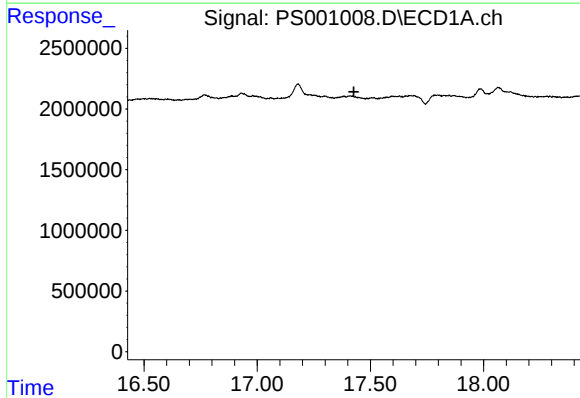


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.427 min
Response: 0
Conc: N.D.

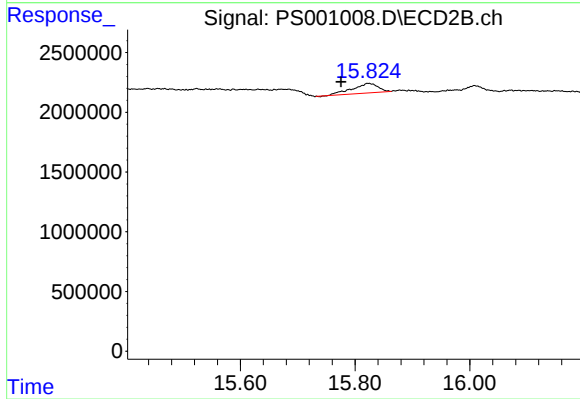

#14 DINOSEB


R.T.: 15.823 min
Delta R.T.: 0.047 min
Response: 2488056
Conc: 2.97 ng/ml

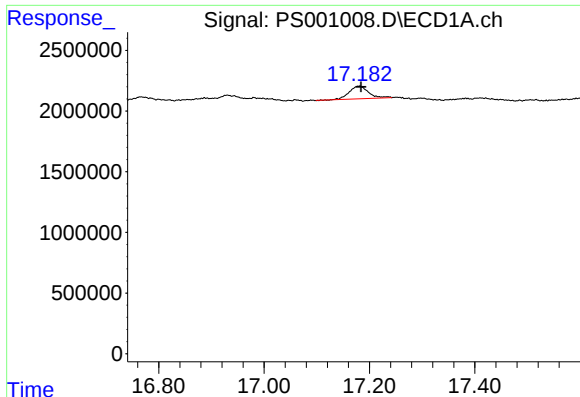

#15 Picloram


R.T.: 17.180 min
Delta R.T.: -0.004 min
Response: 2652031
Conc: 1.46 ng/ml

Instrument :
FID_F
ClientSampleId :

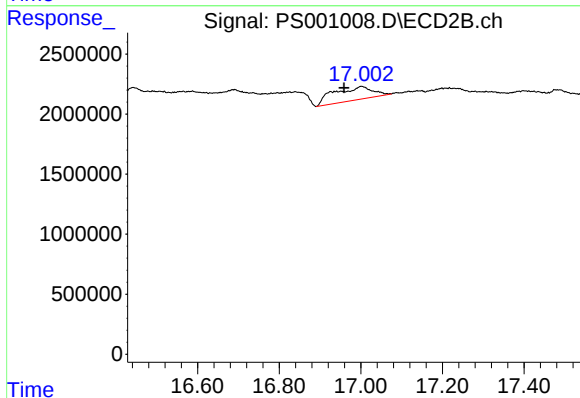


#15 Picloram

R.T.: 17.001 min
Delta R.T.: 0.042 min
Response: 7402902
Conc: 4.86 ng/ml

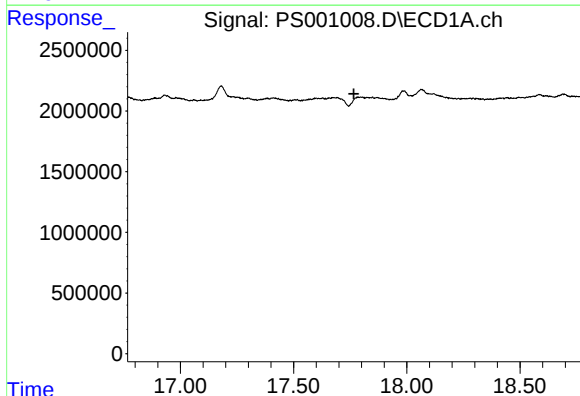

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

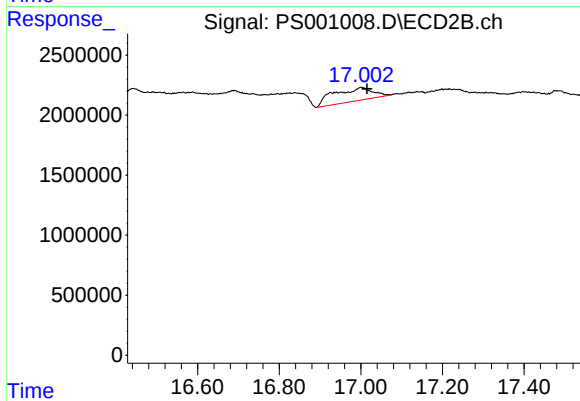

#16 DCPA

R.T.: 17.001 min
Delta R.T.: -0.014 min
Response: 7402902
Conc: 4.31 ng/ml