

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071221\
 Data File : FF008770.D
 Signal(s) : FID2B.ch
 Acq On : 12 Jul 2021 13:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 01:25:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.745	2419823	21.232 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.633	329804	2.815 ug/ml
15)	N-TETRATRIACONTANE	19.410	91398	0.874 ug/ml
16)	N-HEXATRIACONTANE	20.182	277100	2.950 ug/ml
18)	N-TETRACONTANE	21.854	360258	3.893 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071221\
Data File : FF008770.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2021 13:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 01:25:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

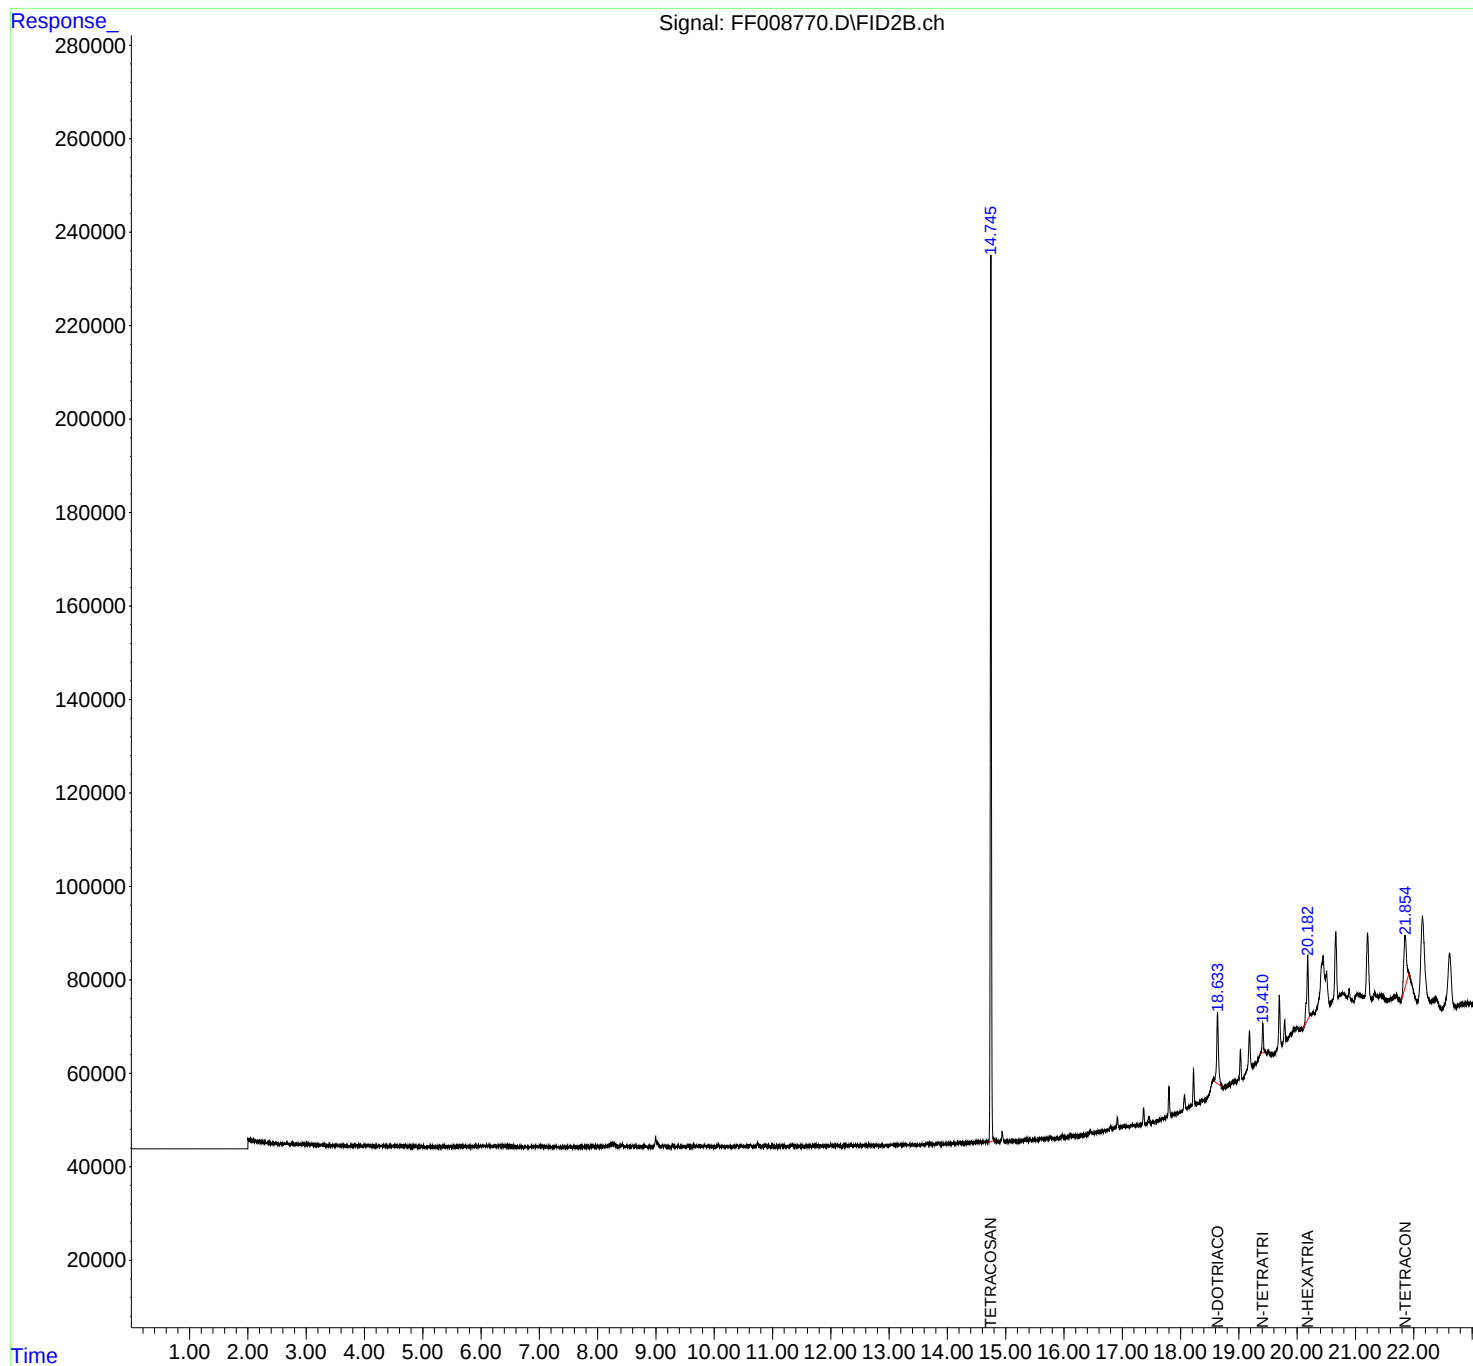


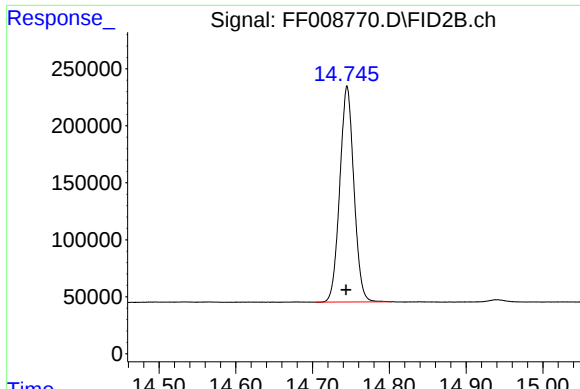

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.745 min
Delta R.T.: 0.001 min
Response: 2419823
Conc: 21.23 ug/ml

Instrument :
FID_F
ClientSampleId :

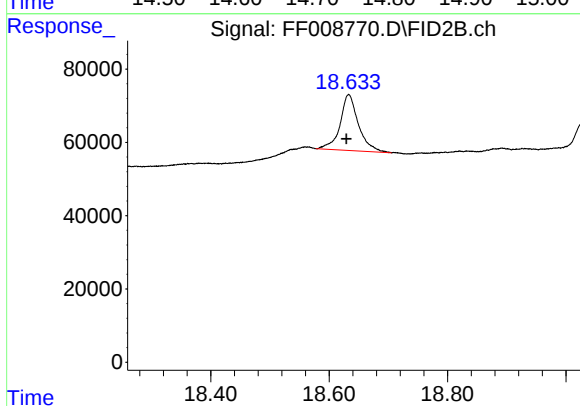


#14 N-DOTRIACONTANE

R.T.: 18.633 min
Delta R.T.: 0.004 min
Response: 329804
Conc: 2.82 ug/ml

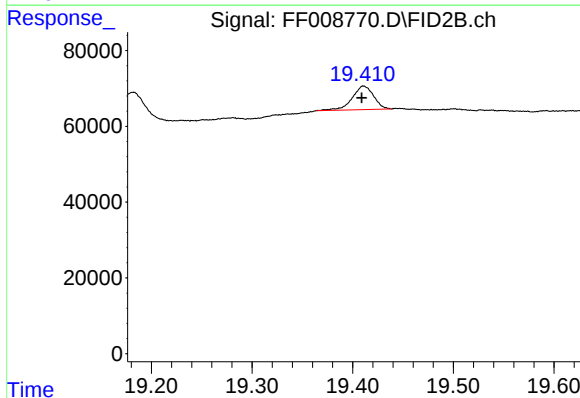


#15 N-TETRATRIACONTANE

R.T.: 19.410 min
Delta R.T.: 0.001 min
Response: 91398
Conc: 0.87 ug/ml

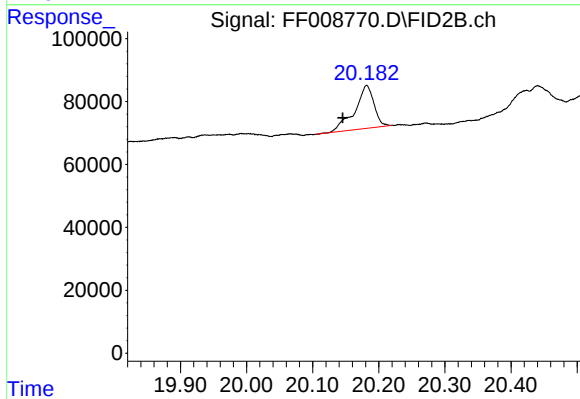

#16 N-HEXATRIACONTANE

R.T.: 20.182 min
Delta R.T.: 0.036 min
Response: 277100
Conc: 2.95 ug/ml

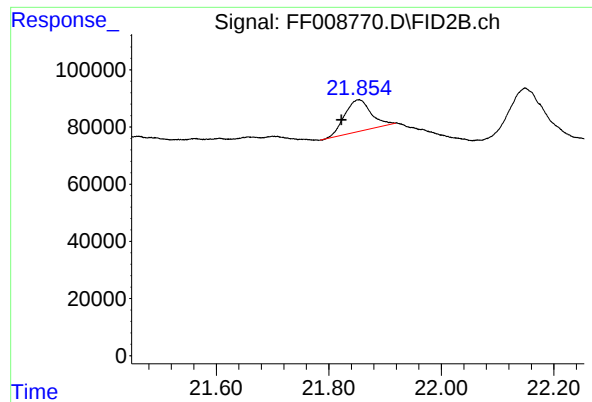

#18 N-TETRACONTANE

R.T.: 21.854 min
Delta R.T.: 0.032 min
Response: 360258
Conc: 3.89 ug/ml

Instrument :
FID_F
ClientSampleId :