

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071221\
 Data File : FF008772.D
 Signal(s) : FID2B.ch
 Acq On : 12 Jul 2021 14:23
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 01:26:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.515	2682083	19.721	ug/ml
12) N-OCTACOSANE	16.917	2255196	18.233	ug/ml
13) N-TRIACONTANE	17.800	95051	0.793	ug/ml
14) N-DOTRIACONTANE	18.632	166941	1.425	ug/ml
15) N-TETRATRIACONTANE	19.411	112864	1.079	ug/ml
16) N-HEXATRIACONTANE	20.150	45017	0.479	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071221\
Data File : FF008772.D
Signal(s) : FID2B.ch
Acq On : 12 Jul 2021 14:23
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 01:26:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

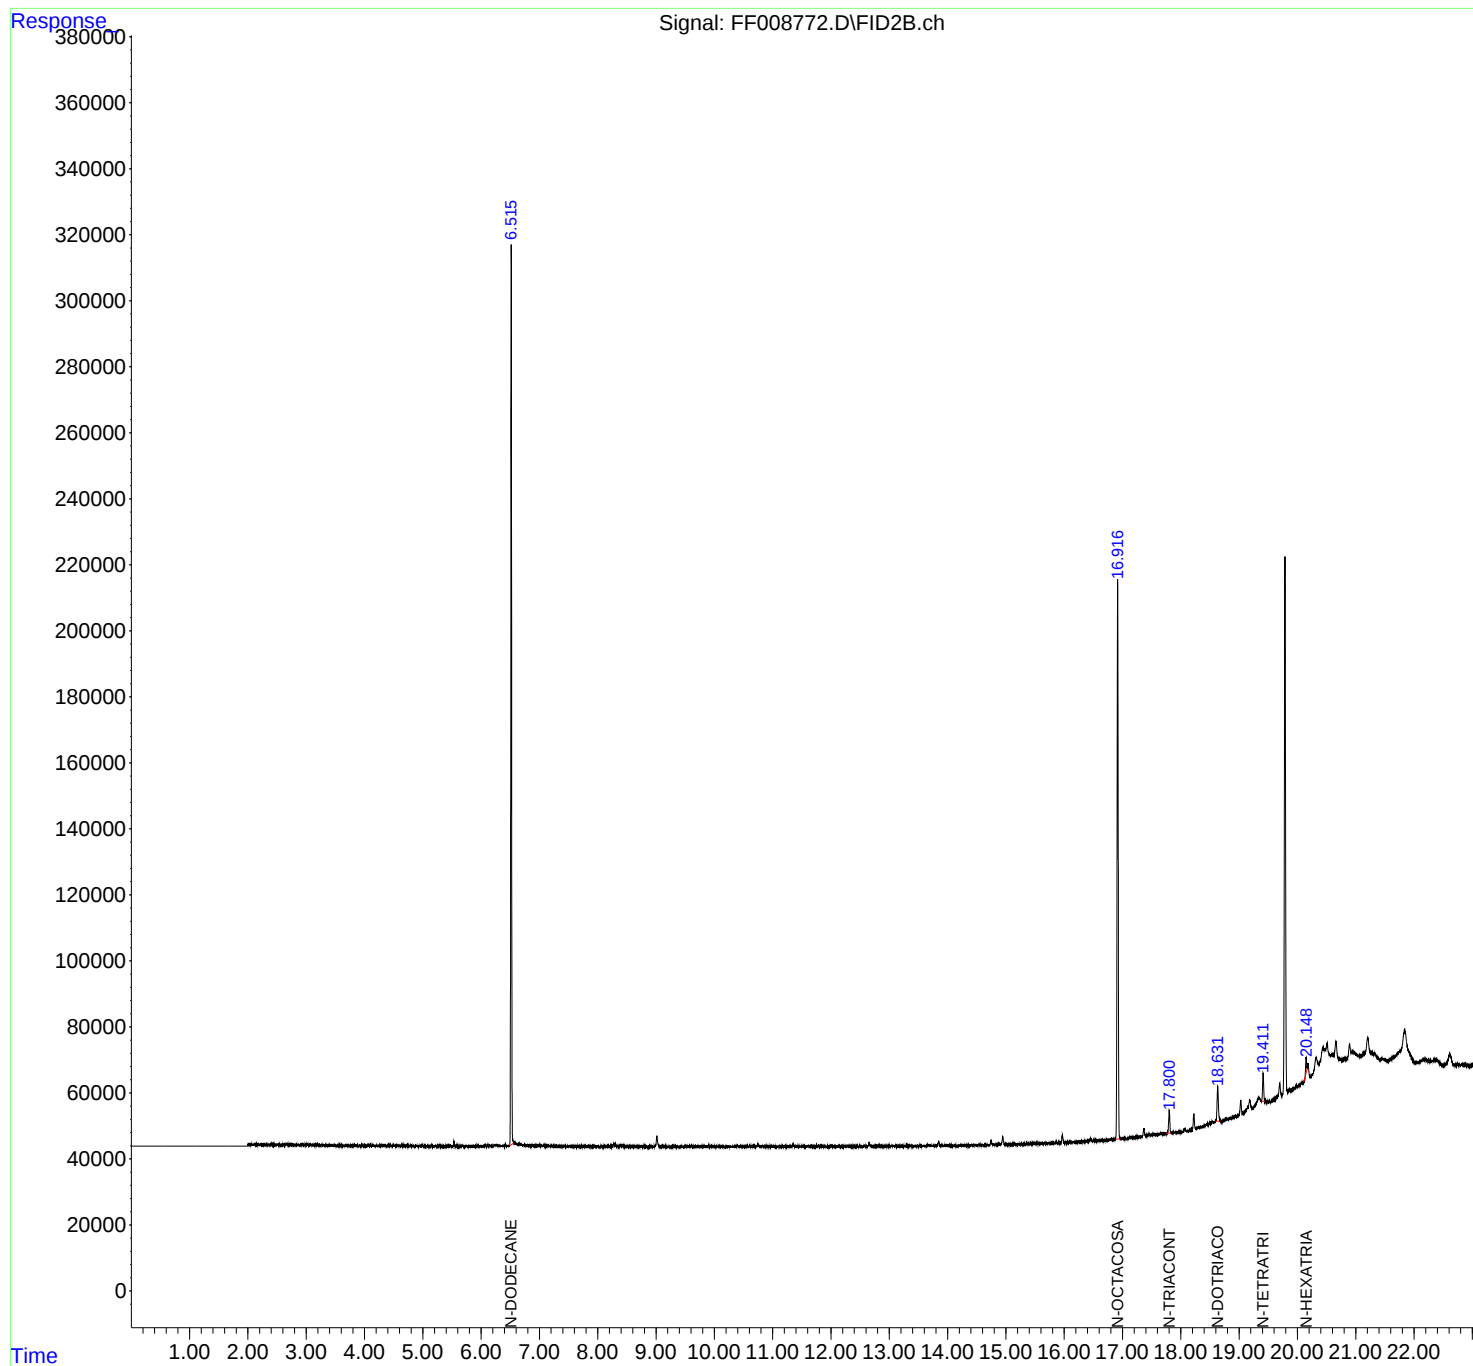


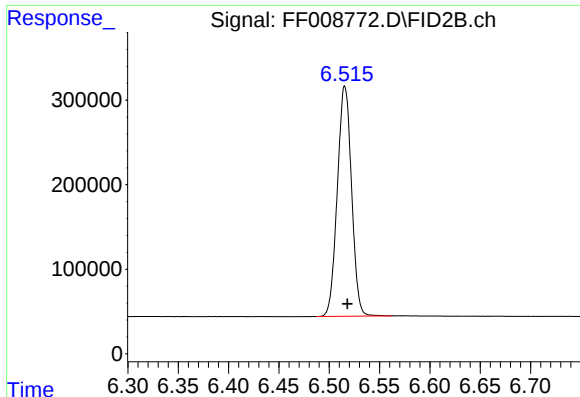

#3 N-DODECANE


R.T.: 6.515 min
Delta R.T.: -0.003 min
Response: 2682083
Conc: 19.72 ug/ml

Instrument :
FID_F
ClientSampleId :

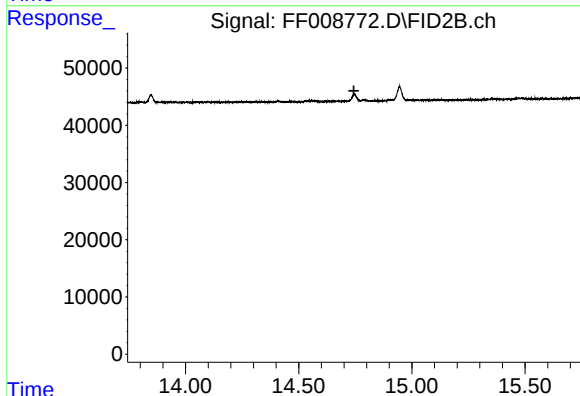


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.744 min
Response: 0
Conc: N.D.

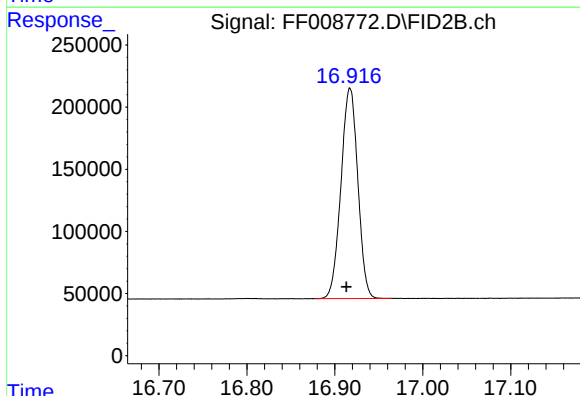


#12 N-OCTACOSANE

R.T.: 16.917 min
Delta R.T.: 0.004 min
Response: 2255196
Conc: 18.23 ug/ml

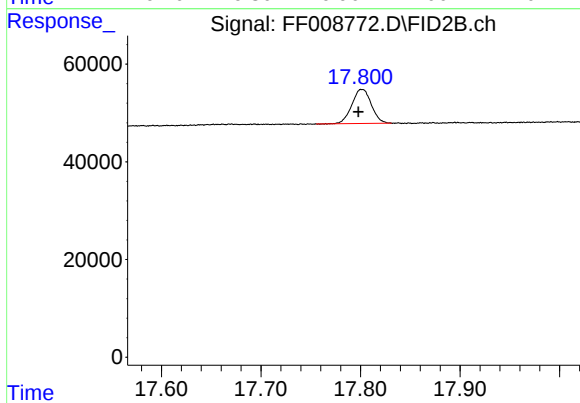

#13 N-TRIACONTANE


R.T.: 17.800 min
Delta R.T.: 0.003 min
Response: 95051
Conc: 0.79 ug/ml

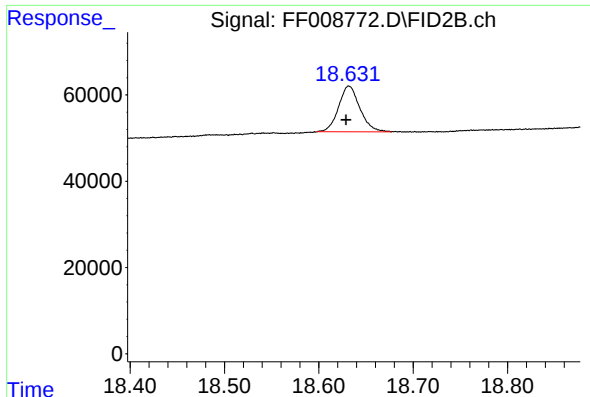

#14 N-DOTRIACONTANE


R.T.: 18.632 min
Delta R.T.: 0.003 min
Response: 166941
Conc: 1.42 ug/ml

Instrument :
FID_F
ClientSampleId :

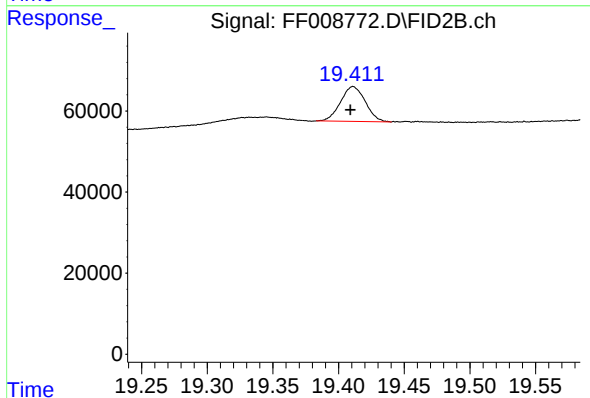

#15 N-TETRATRIACONTANE

R.T.: 19.411 min
Delta R.T.: 0.002 min
Response: 112864
Conc: 1.08 ug/ml

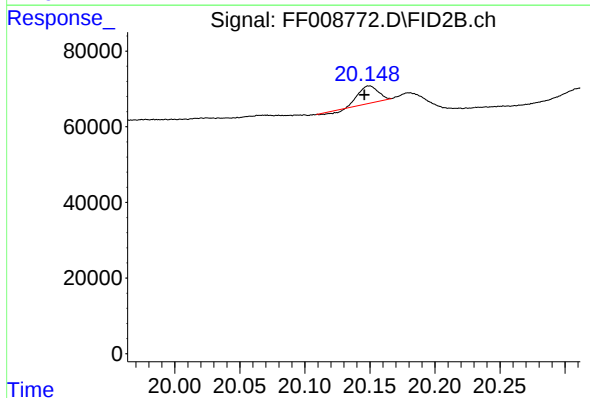

#16 N-HEXATRIACONTANE

R.T.: 20.150 min
Delta R.T.: 0.005 min
Response: 45017
Conc: 0.48 ug/ml