

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001326.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 11:51
 Operator : AJ\SJ
 Sample : J3948-01 100X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 14:52:22 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.459	449999	4.177 ug/ml
Target Compounds			
4) N-TETRADECANE	7.994	417720	3.321 ug/ml
6) N-OCTADECANE	11.129f	459205	3.664 ug/ml
7) N-EICOSANE	12.414	6598737	53.048 ug/ml
8) N-DOCOSANE	13.571	614426	4.983 ug/ml
10) N-TETRACOSANE	14.630	3787011	31.065 ug/ml
11) N-HEXACOSANE	15.703	236492	1.951 ug/ml
12) N-OCTACOSANE	16.626	529190	4.393 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001326.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 11:51
Operator : AJ\SJ
Sample : J3948-01 100X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 14:52:22 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

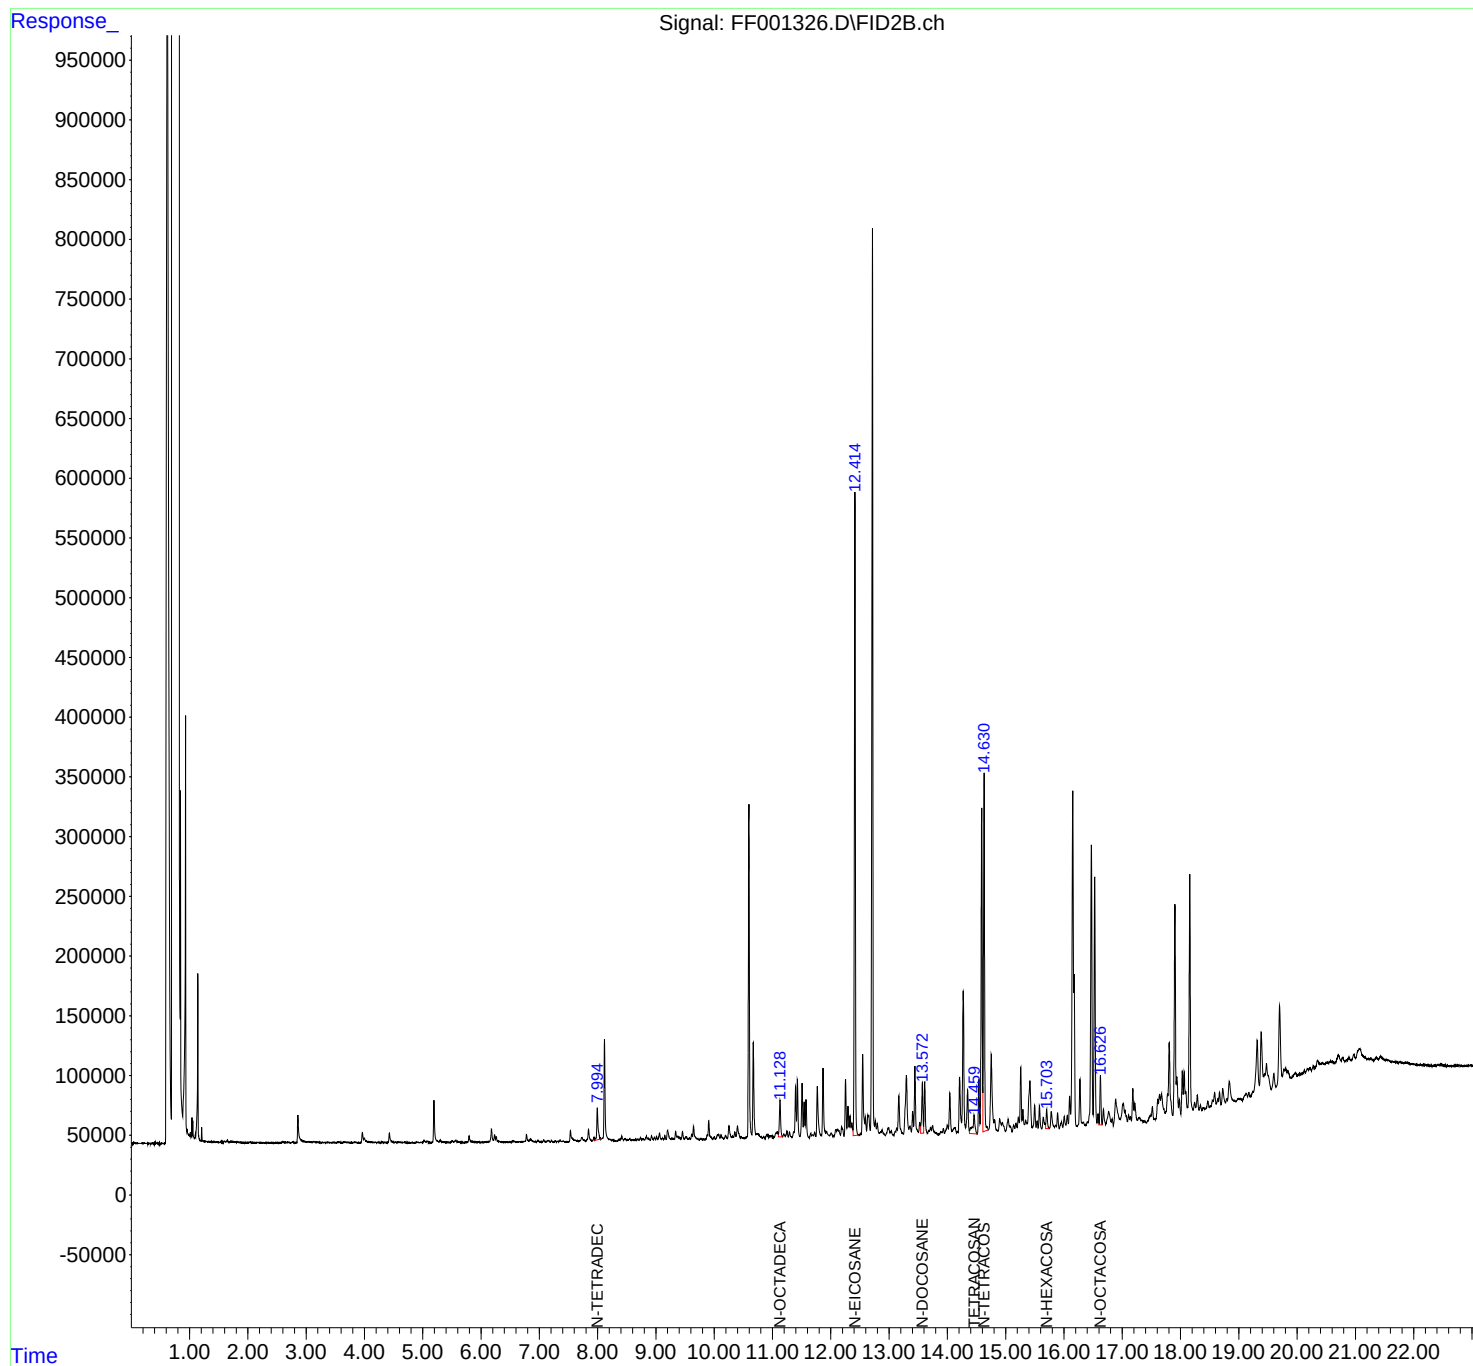


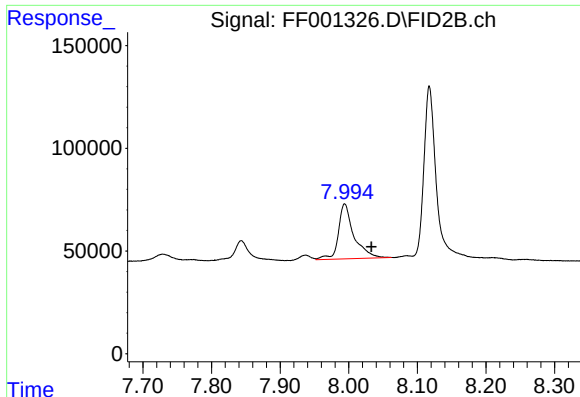

#4 N-TETRADECANE


R.T.: 7.994 min
Delta R.T.: -0.039 min
Response: 417720
Conc: 3.32 ug/ml

Instrument :
FID_F
ClientSampleId :

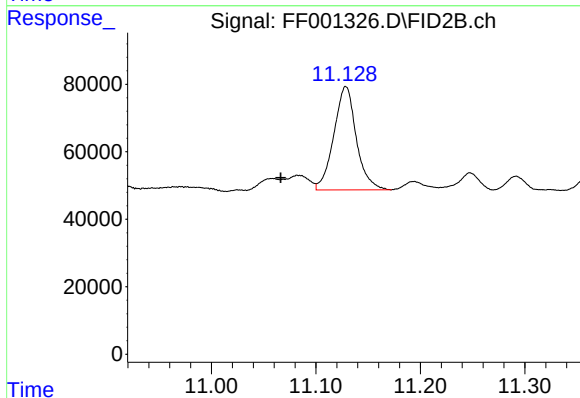


#6 N-OCTADECANE

R.T.: 11.129 min
Delta R.T.: 0.062 min
Response: 459205
Conc: 3.66 ug/ml

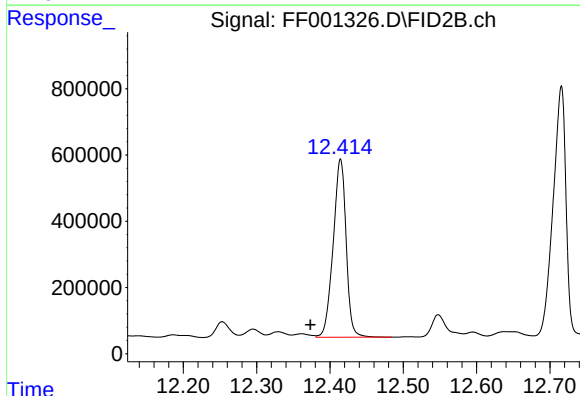


#7 N-EICOSANE

R.T.: 12.414 min
Delta R.T.: 0.041 min
Response: 6598737
Conc: 53.05 ug/ml

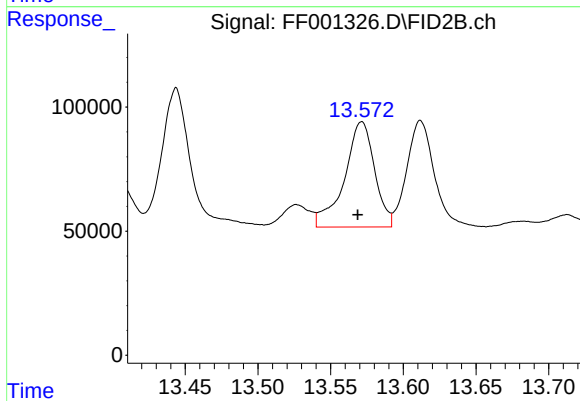

#8 N-DOCOSANE


R.T.: 13.571 min
Delta R.T.: 0.003 min
Response: 614426
Conc: 4.98 ug/ml

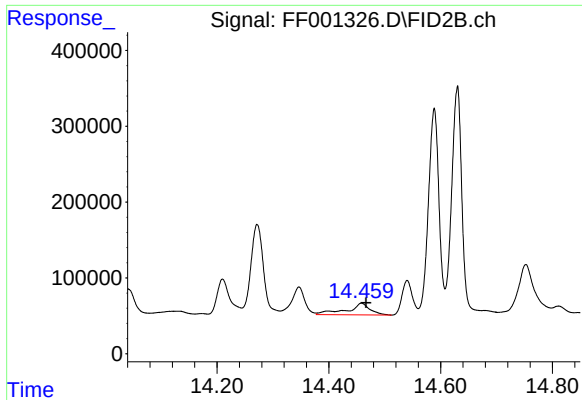

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.459 min
Delta R.T.: -0.008 min
Response: 449999
Conc: 4.18 ug/ml

Instrument :
FID_F
ClientSampleId :

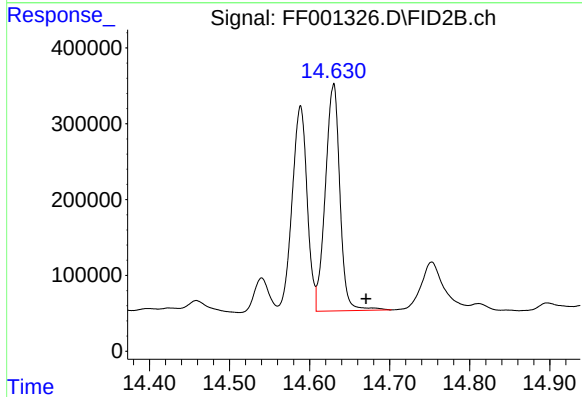


#10 N-TETRACOSANE

R.T.: 14.630 min
Delta R.T.: -0.041 min
Response: 3787011
Conc: 31.06 ug/ml

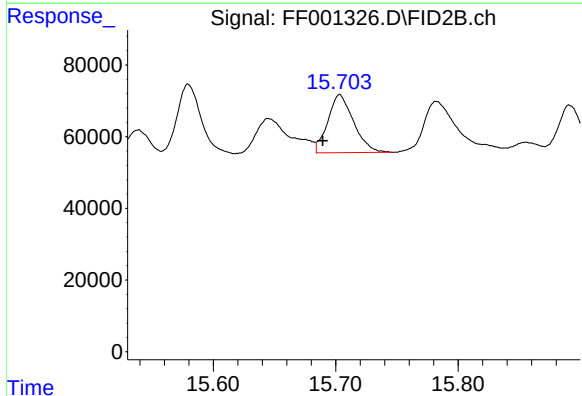

#11 N-HEXACOSANE

R.T.: 15.703 min
Delta R.T.: 0.014 min
Response: 236492
Conc: 1.95 ug/ml

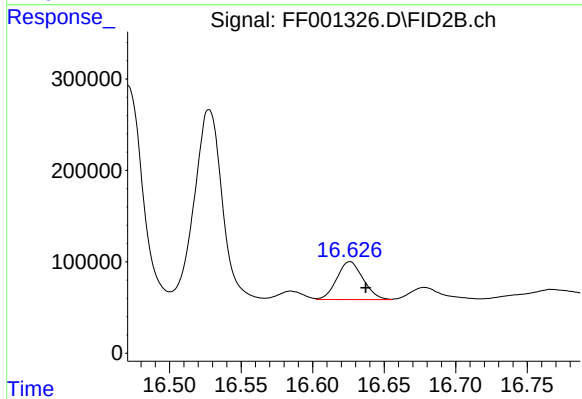

#12 N-OCTACOSANE

R.T.: 16.626 min
Delta R.T.: -0.011 min
Response: 529190
Conc: 4.39 ug/ml