

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001327.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 12:21
Operator : AJ\SJ
Sample : J3948-05 50X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 14:52:29 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.410	1808924	14.542 ug/ml
8)	N-DOCOSANE	13.572	359306	2.914 ug/ml
10)	N-TETRACOSANE	14.625	977833	8.021 ug/ml
14)	N-DOTRIACONTANE	18.289f	301365	2.556 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001327.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 12:21
Operator : AJ\SJ
Sample : J3948-05 50X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 14:52:29 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

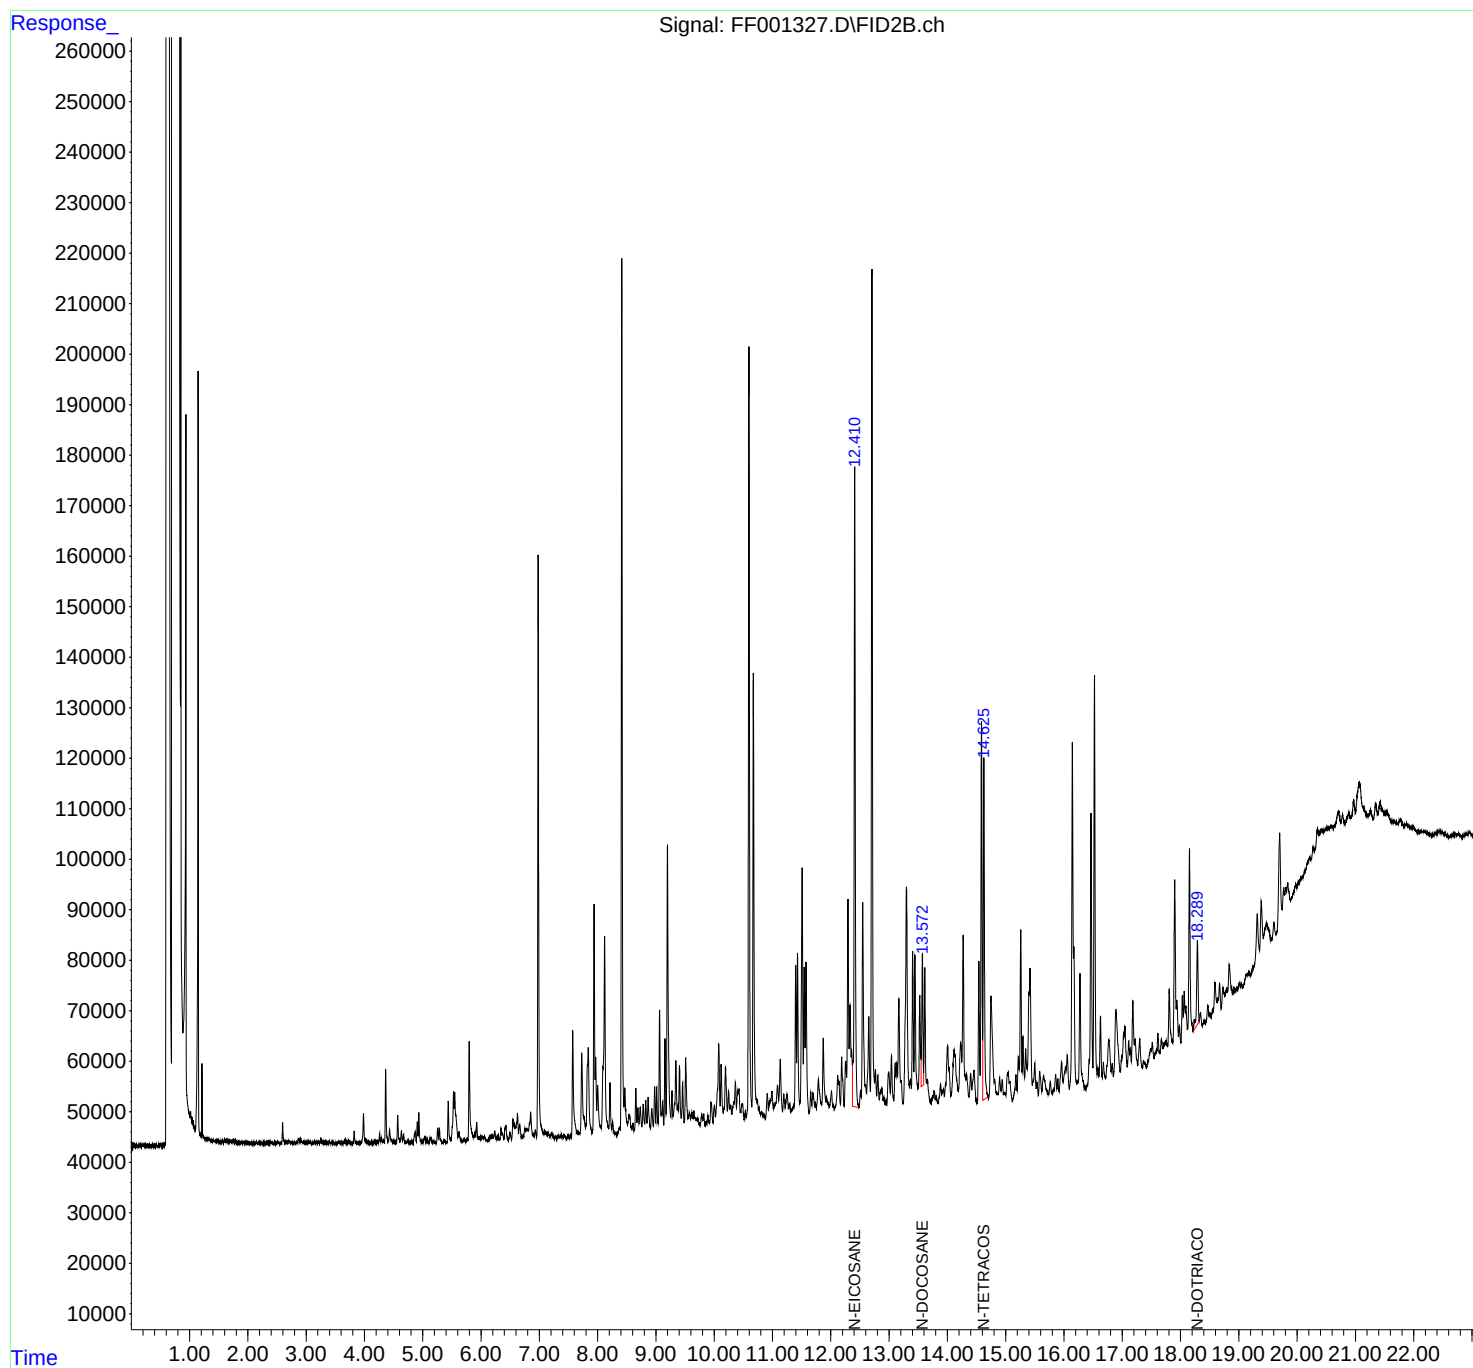


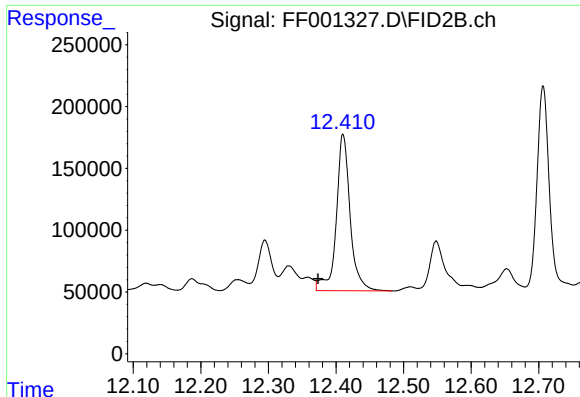

#7 N-EICOSANE


R.T.: 12.410 min
Delta R.T.: 0.037 min
Response: 1808924
Conc: 14.54 ug/ml

Instrument :
FID_F
ClientSampleId :

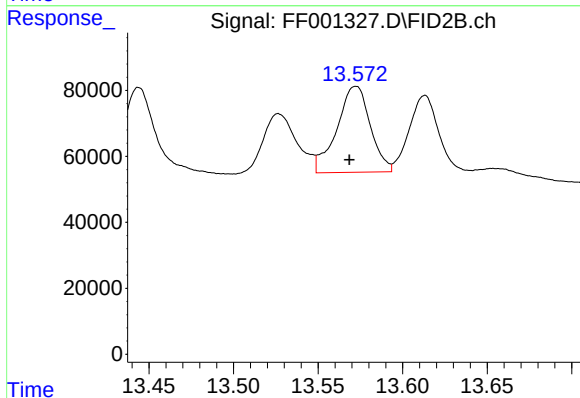


#8 N-DOCOSANE

R.T.: 13.572 min
Delta R.T.: 0.004 min
Response: 359306
Conc: 2.91 ug/ml

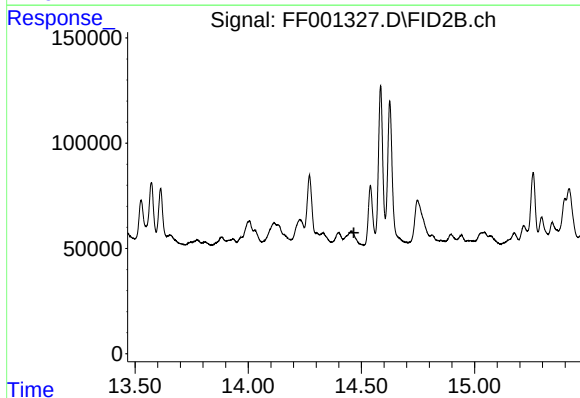


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.467 min
Response: 0
Conc: N.D.

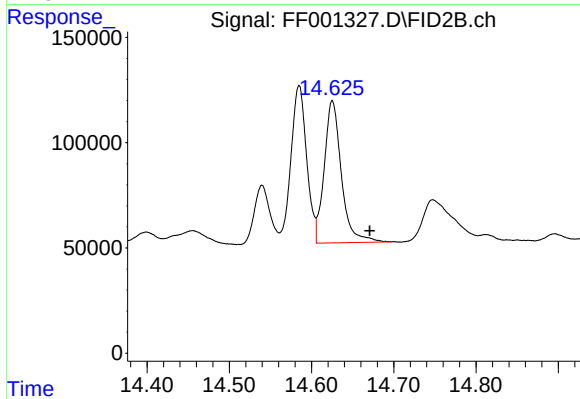

#10 N-TETRACOSANE

R.T.: 14.625 min
Delta R.T.: -0.045 min
Response: 977833
Conc: 8.02 ug/ml

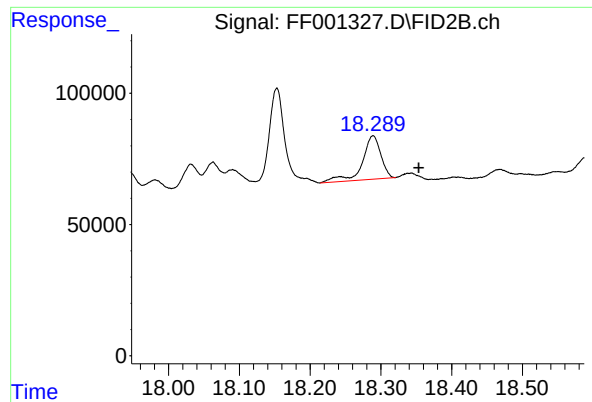

#14 N-DOTRIACONTANE

R.T.: 18.289 min
Delta R.T.: -0.064 min
Response: 301365
Conc: 2.56 ug/ml

Instrument :
FID_F
ClientSampleId :