

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001328.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 12:51
 Operator : AJ\SJ
 Sample : J3948-03 2X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 14:52:36 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.456	884155	8.208 ug/ml
Target Compounds			
4) N-TETRADECANE	8.080	367726	2.924 ug/ml
6) N-OCTADECANE	11.132f	251750	2.009 ug/ml
7) N-EICOSANE	12.413	3274302	26.323 ug/ml
8) N-DOCOSANE	13.573	326695	2.649 ug/ml
10) N-TETRACOSANE	14.627	1562225	12.815 ug/ml
12) N-OCTACOSANE	16.626	380726	3.160 ug/ml
13) N-TRIACONTANE	17.511	300100	2.496 ug/ml
14) N-DOTRIACONTANE	18.337	388191	3.292 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001328.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 12:51
Operator : AJ\SJ
Sample : J3948-03 2X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 14:52:36 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

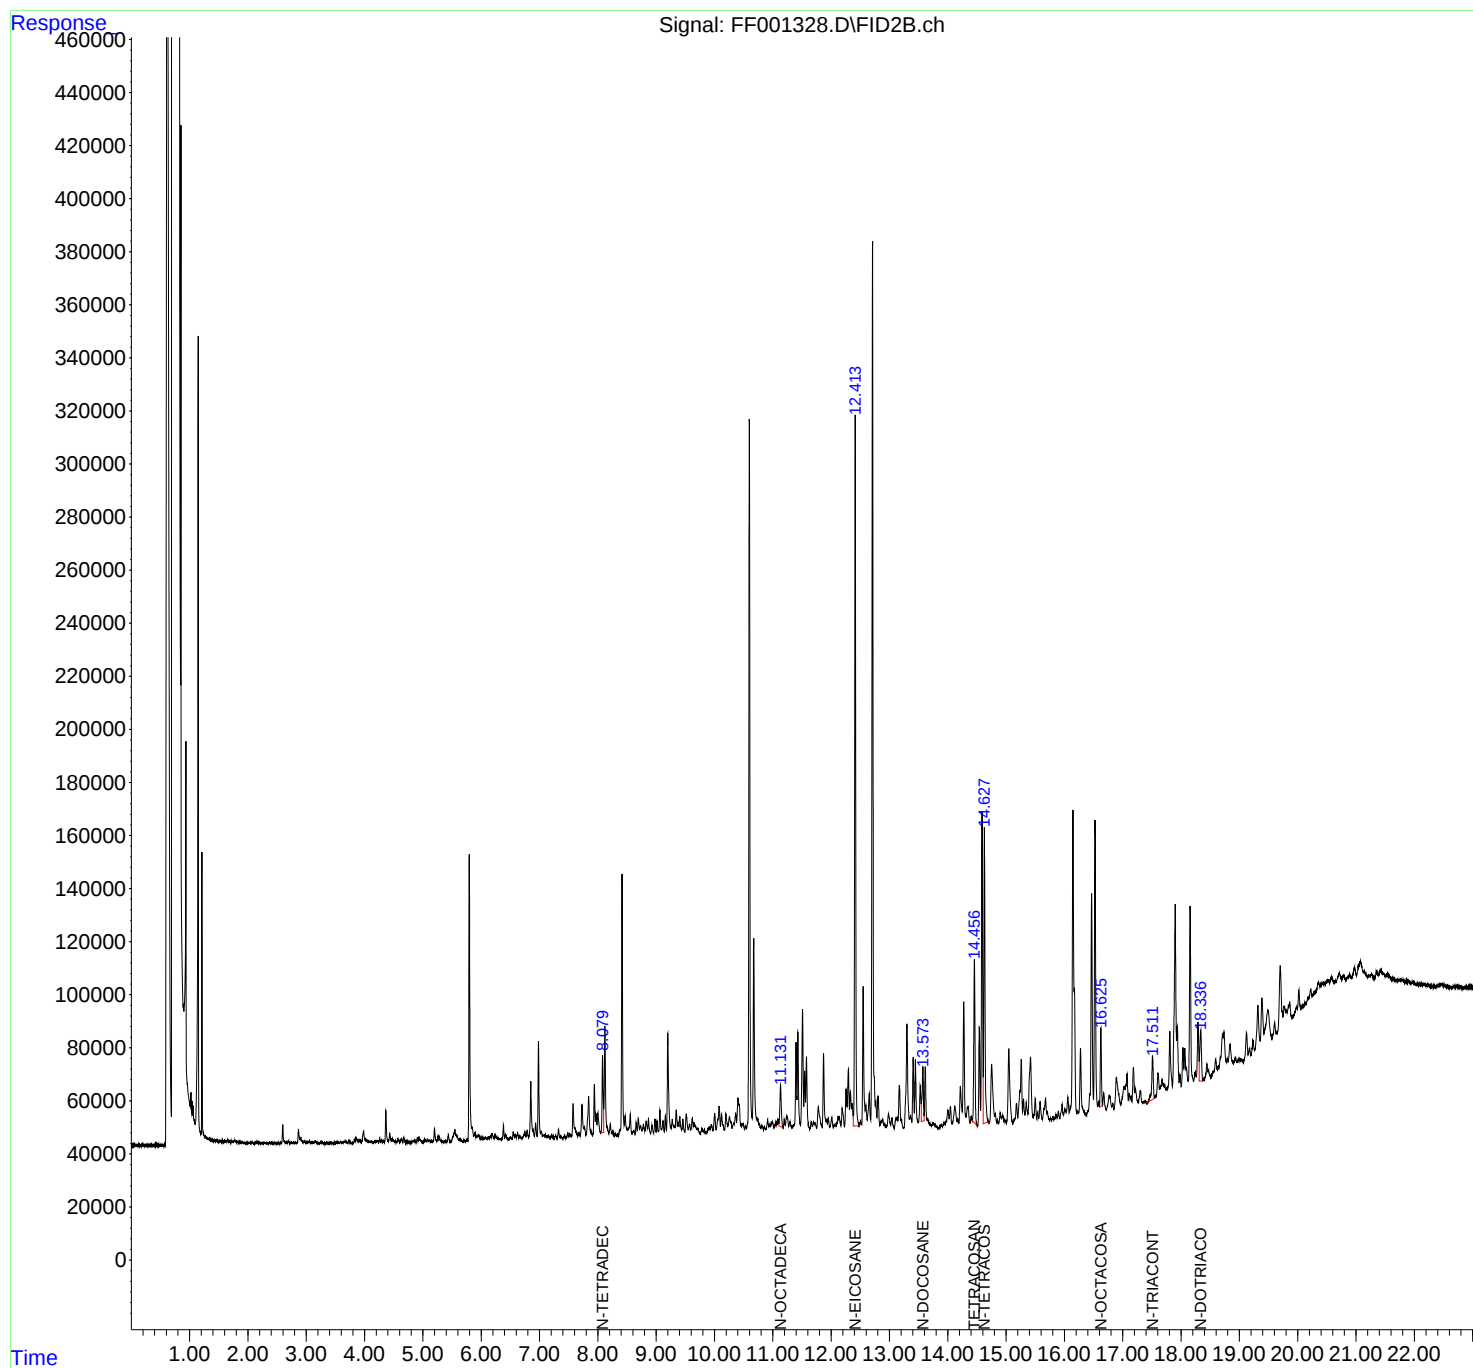


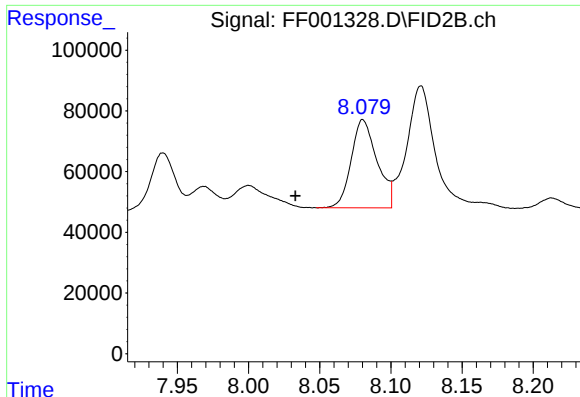

#4 N-TETRADECANE


R.T.: 8.080 min
Delta R.T.: 0.048 min
Response: 367726
Conc: 2.92 ug/ml

Instrument :
FID_F
ClientSampleId :

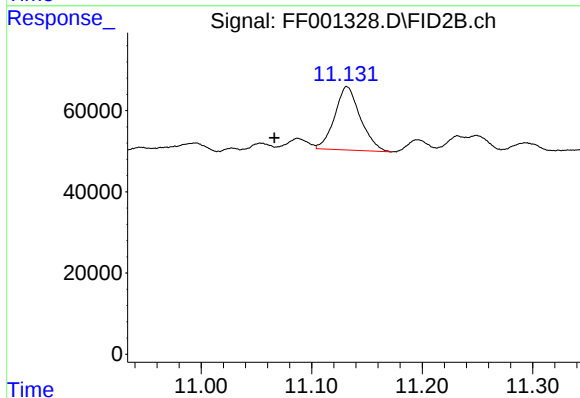


#6 N-OCTADECANE

R.T.: 11.132 min
Delta R.T.: 0.066 min
Response: 251750
Conc: 2.01 ug/ml

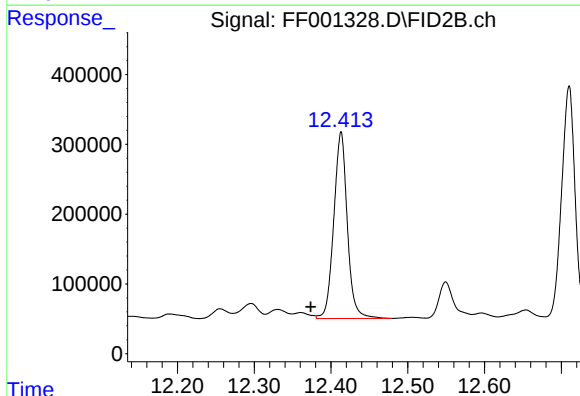


#7 N-EICOSANE

R.T.: 12.413 min
Delta R.T.: 0.040 min
Response: 3274302
Conc: 26.32 ug/ml

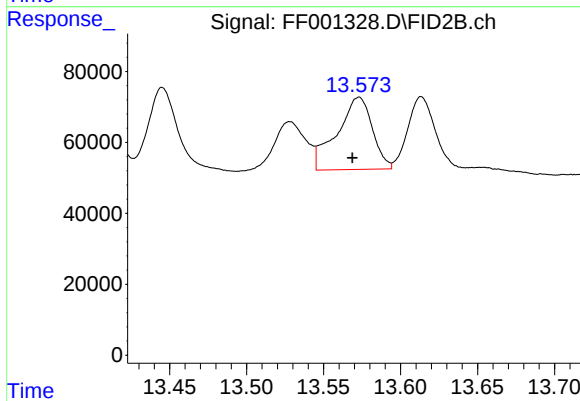

#8 N-DOCOSANE


R.T.: 13.573 min
Delta R.T.: 0.004 min
Response: 326695
Conc: 2.65 ug/ml

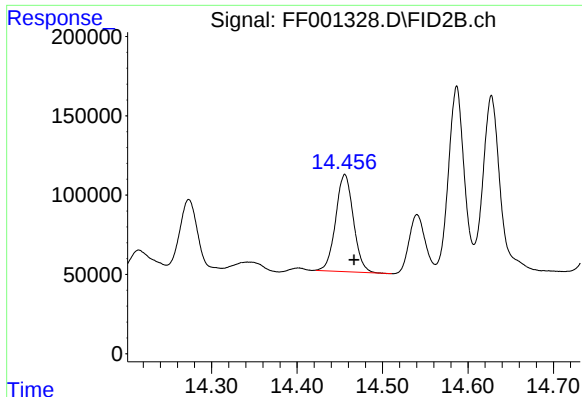

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.456 min
Delta R.T.: -0.011 min
Response: 884155
Conc: 8.21 ug/ml

Instrument :
FID_F
ClientSampleId :

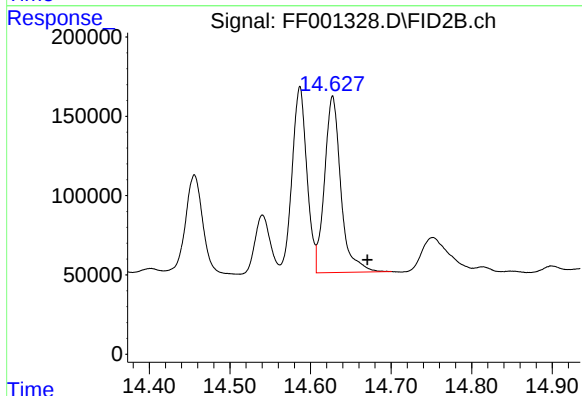


#10 N-TETRACOSANE

R.T.: 14.627 min
Delta R.T.: -0.043 min
Response: 1562225
Conc: 12.81 ug/ml

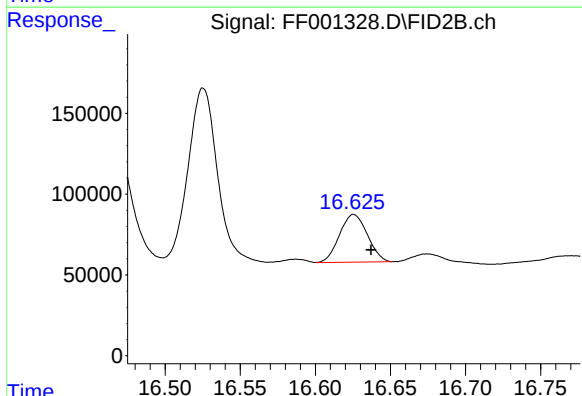


#12 N-OCTACOSANE

R.T.: 16.626 min
Delta R.T.: -0.012 min
Response: 380726
Conc: 3.16 ug/ml

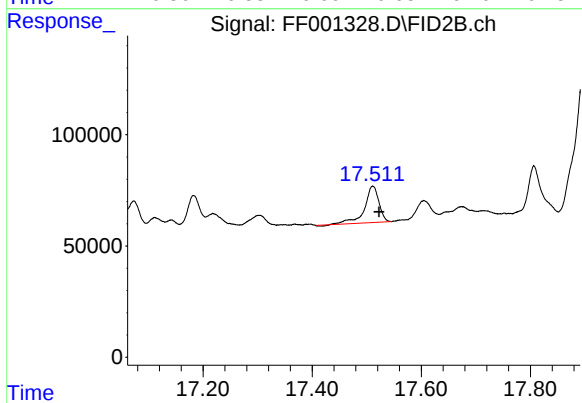

#13 N-TRIACONTANE

R.T.: 17.511 min
Delta R.T.: -0.012 min
Response: 300100
Conc: 2.50 ug/ml

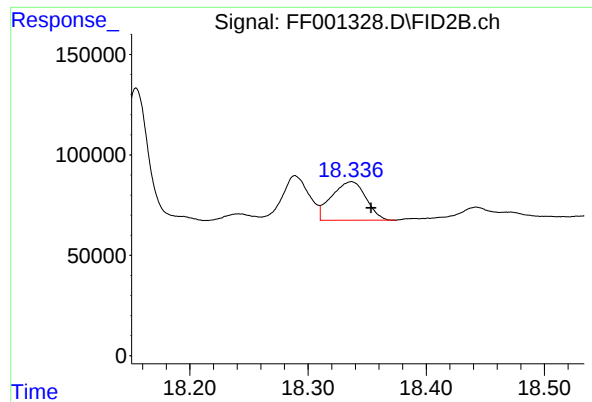

#14 N-DOTRIACONTANE

R.T.: 18.337 min
Delta R.T.: -0.017 min
Response: 388191
Conc: 3.29 ug/ml

Instrument :
FID_F
ClientSampleId :