

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001330.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 13:51
 Operator : AJ\SJ
 Sample : J3947-04 2X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 14:52:50 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.456	945848	8.780 ug/ml
Target Compounds			
4) N-TETRADECANE	8.079	513313	4.081 ug/ml
7) N-EICOSANE	12.412	326427	2.624 ug/ml
10) N-TETRACOSANE	14.627	459577	3.770 ug/ml
12) N-OCTACOSANE	16.627	308793	2.563 ug/ml
13) N-TRIACONTANE	17.512	422763	3.517 ug/ml
14) N-DOTRIACONTANE	18.340	622476	5.280 ug/ml
15) N-TETRATRIACONTANE	19.137	490358	4.172 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001330.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 13:51
Operator : AJ\SJ
Sample : J3947-04 2X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 14:52:50 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

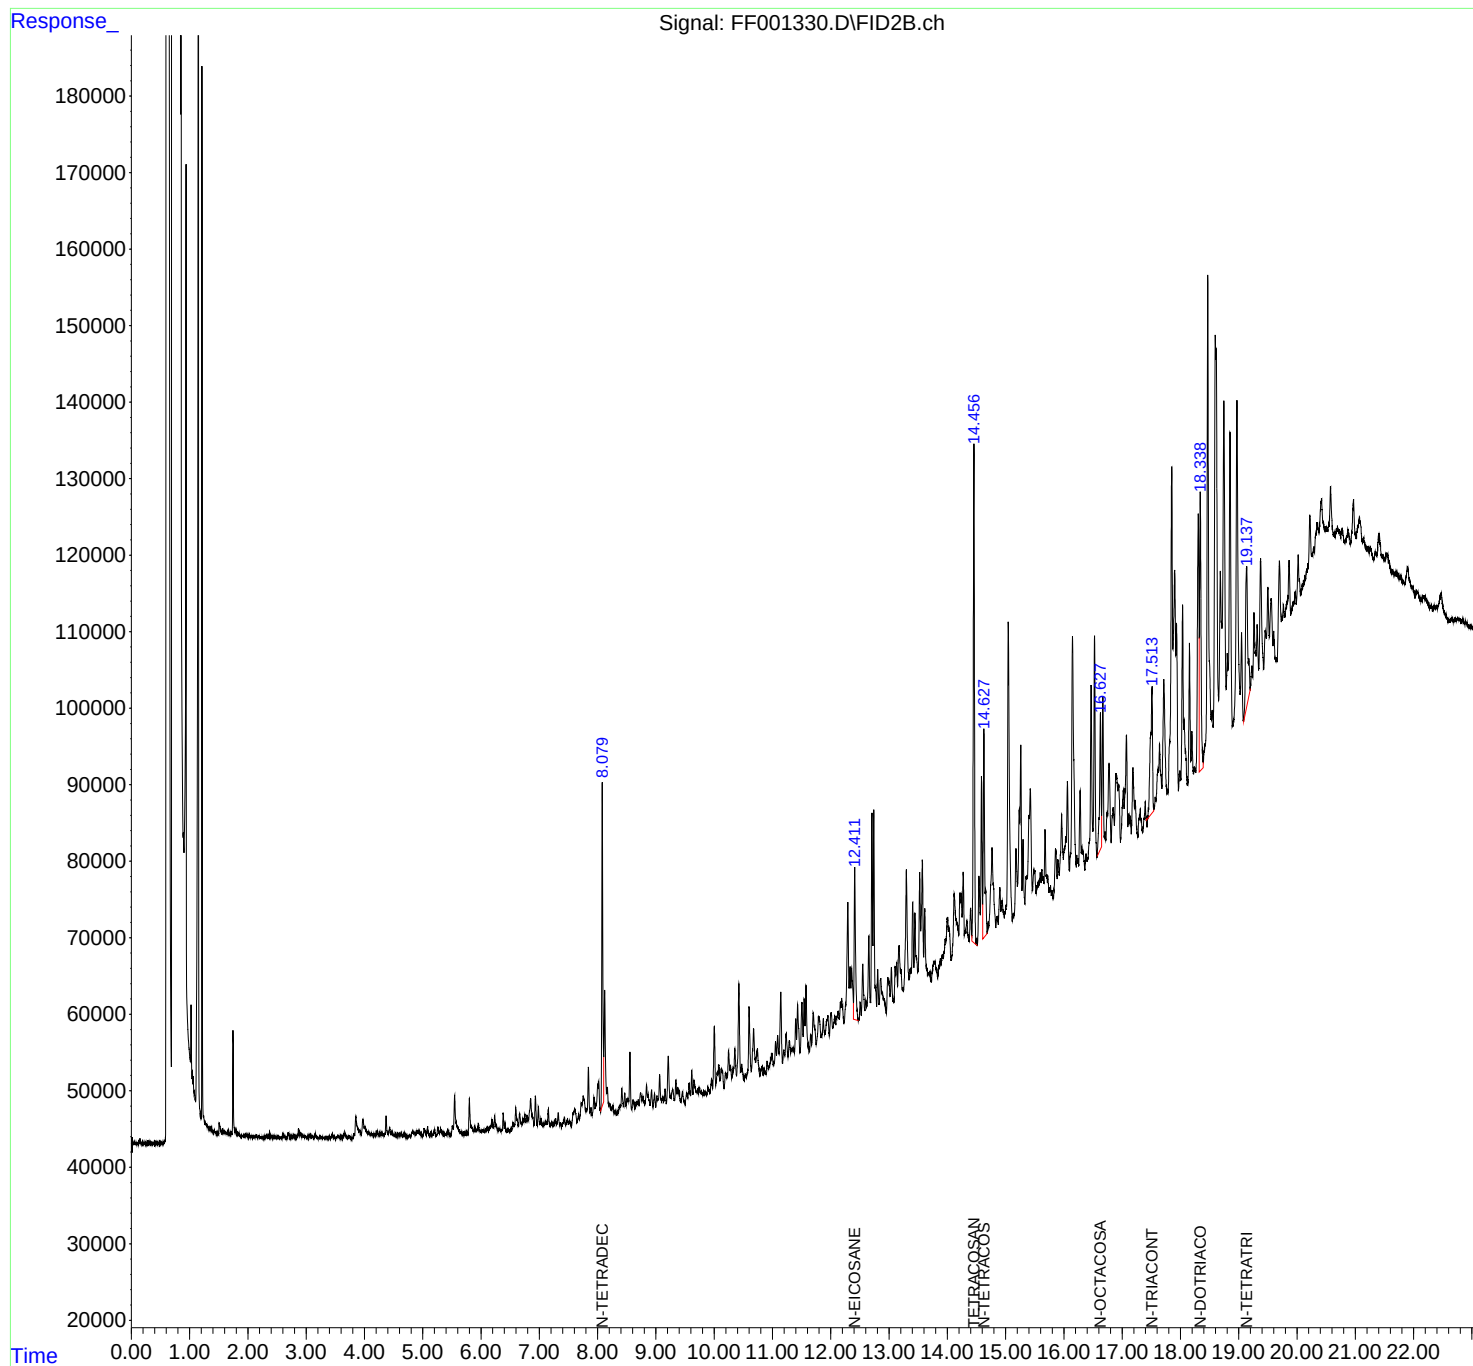


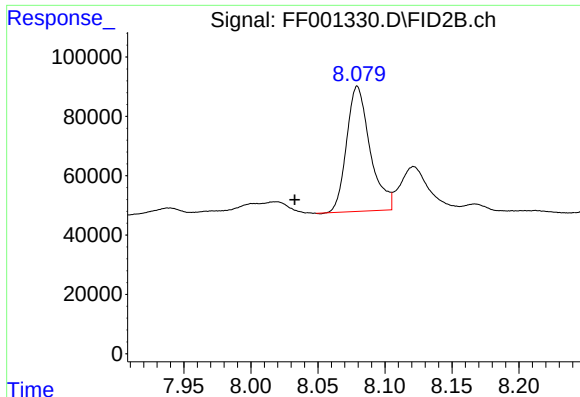

#4 N-TETRADECANE


R.T.: 8.079 min
Delta R.T.: 0.047 min
Response: 513313
Conc: 4.08 ug/ml

Instrument :
FID_F
ClientSampleId :

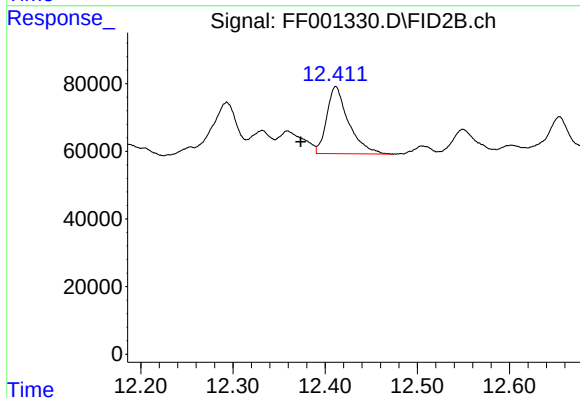


#7 N-EICOSANE

R.T.: 12.412 min
Delta R.T.: 0.038 min
Response: 326427
Conc: 2.62 ug/ml

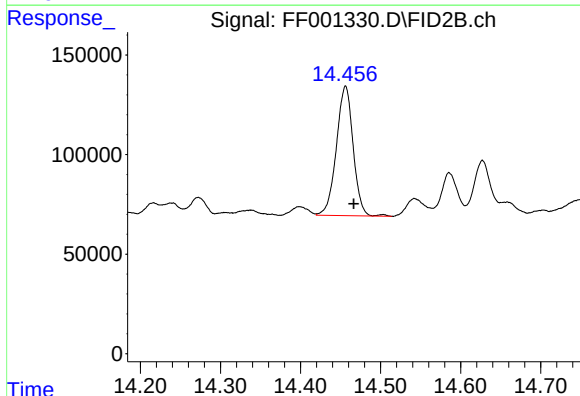


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.456 min
Delta R.T.: -0.010 min
Response: 945848
Conc: 8.78 ug/ml

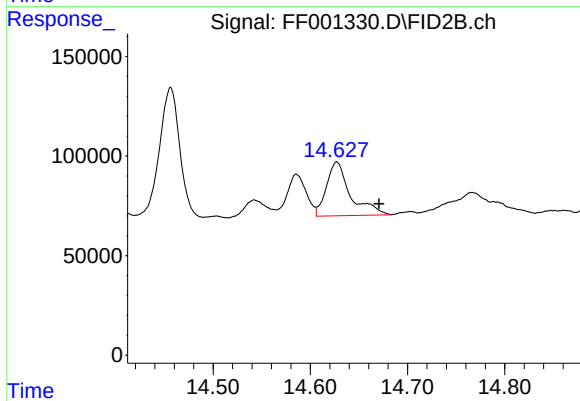

#10 N-TETRACOSANE


R.T.: 14.627 min
Delta R.T.: -0.043 min
Response: 459577
Conc: 3.77 ug/ml

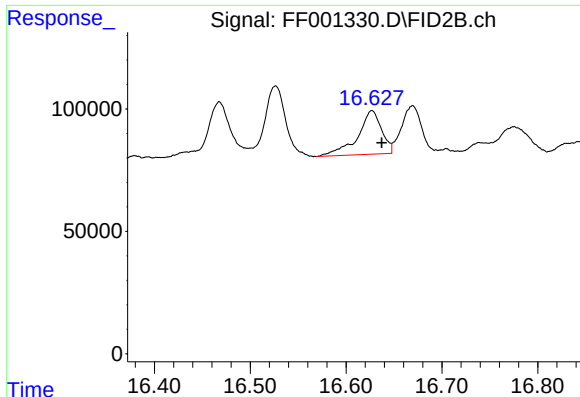

#12 N-OCTACOSANE


R.T.: 16.627 min
Delta R.T.: -0.010 min
Response: 308793
Conc: 2.56 ug/ml

Instrument :
FID_F
ClientSampleId :

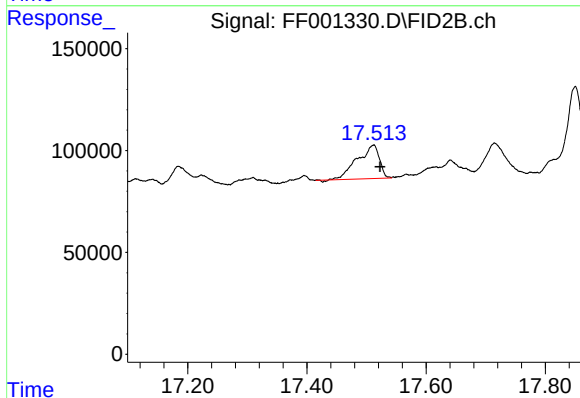


#13 N-TRIACONTANE

R.T.: 17.512 min
Delta R.T.: -0.011 min
Response: 422763
Conc: 3.52 ug/ml

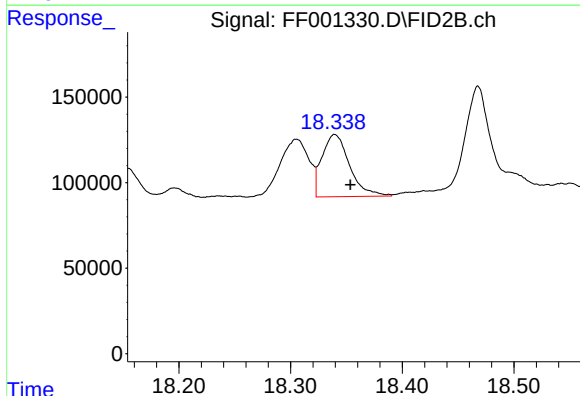

#14 N-DOTRIACONTANE

R.T.: 18.340 min
Delta R.T.: -0.014 min
Response: 622476
Conc: 5.28 ug/ml

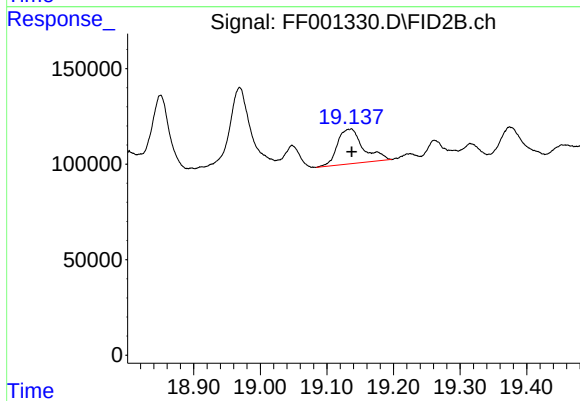

#15 N-TETRATRIACONTANE

R.T.: 19.137 min
Delta R.T.: 0.000 min
Response: 490358
Conc: 4.17 ug/ml