

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001333.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 15:21
 Operator : AJ\SJ
 Sample : J3927-03 2X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 15:43:14 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.455	888565	8.249 ug/ml
Target Compounds			
4) N-TETRADECANE	8.080	337436	2.683 ug/ml
7) N-EICOSANE	12.411	353309	2.840 ug/ml
10) N-TETRACOSANE	14.628	330922	2.715 ug/ml
12) N-OCTACOSANE	16.626	287247	2.384 ug/ml
13) N-TRIACONTANE	17.512	409767	3.409 ug/ml
14) N-DOTRIACONTANE	18.341	464554	3.940 ug/ml
15) N-TETRATRIACONTANE	19.129	178332	1.517 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001333.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 15:21
Operator : AJ\SJ
Sample : J3927-03 2X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 15:43:14 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

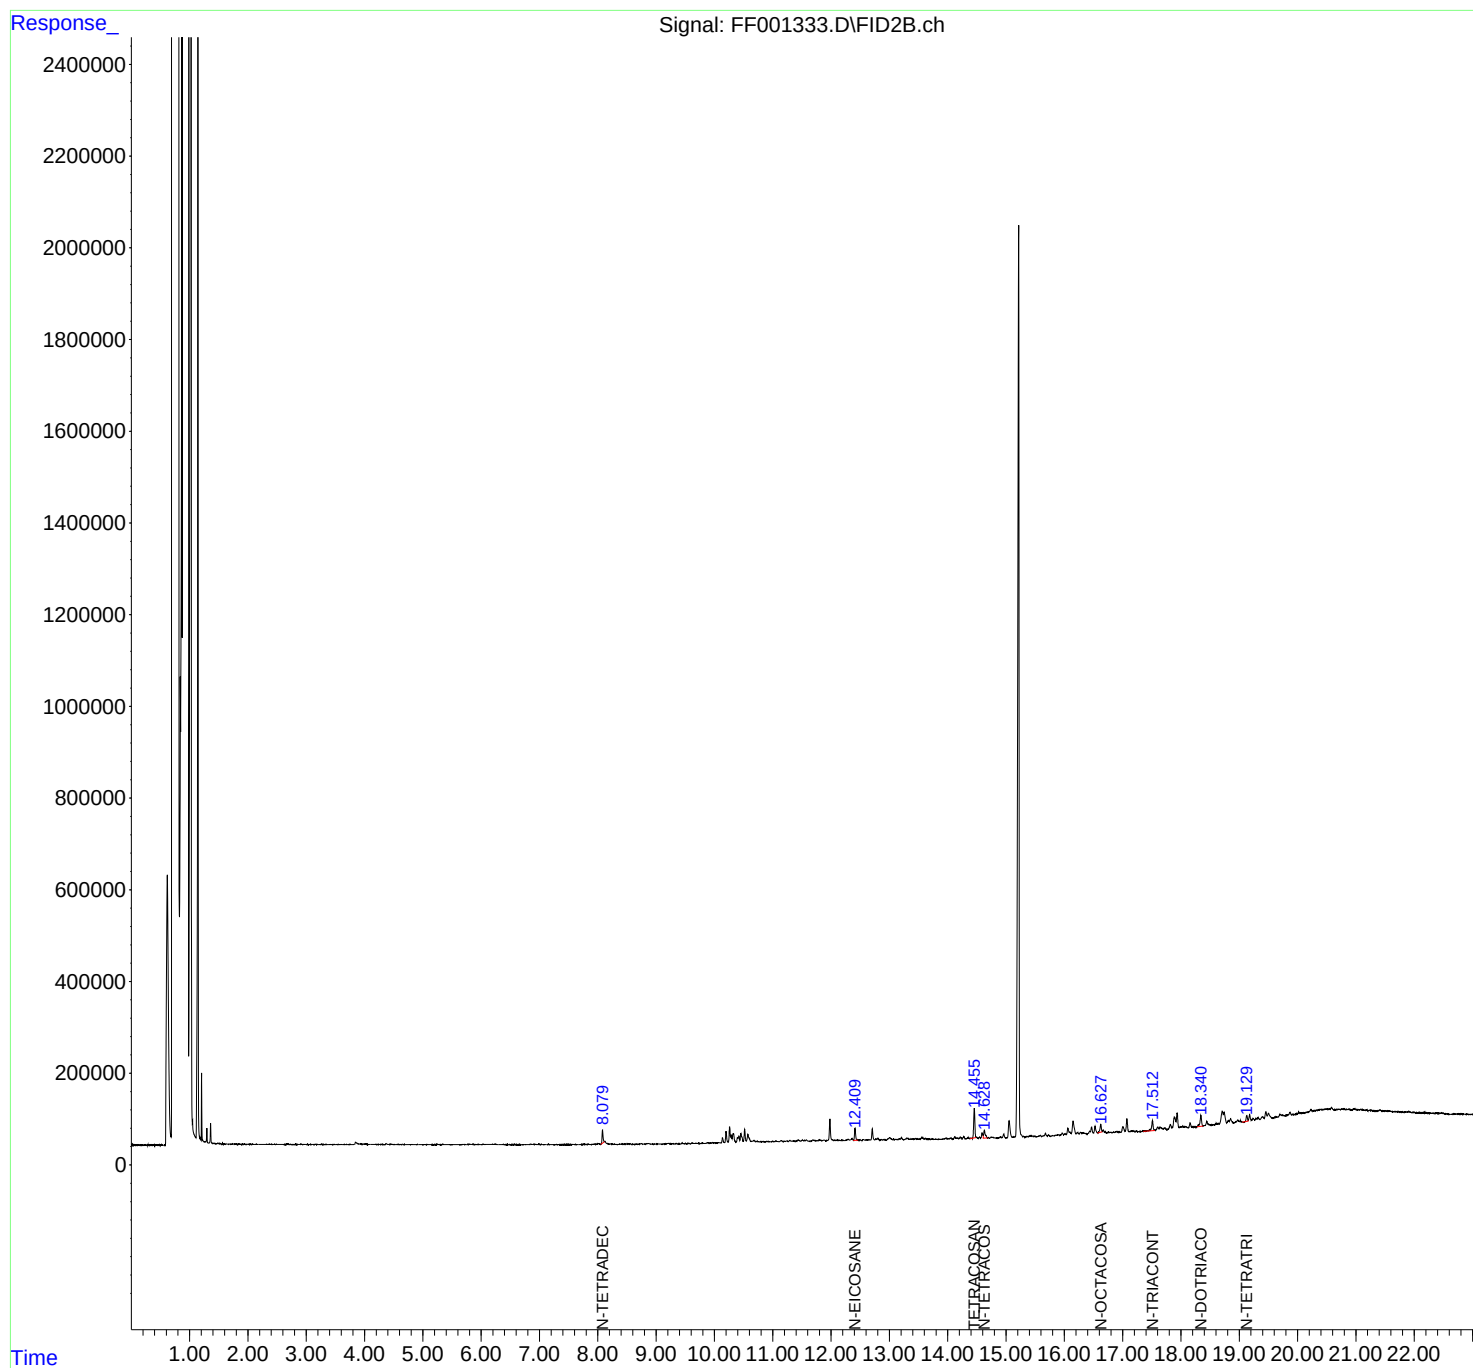


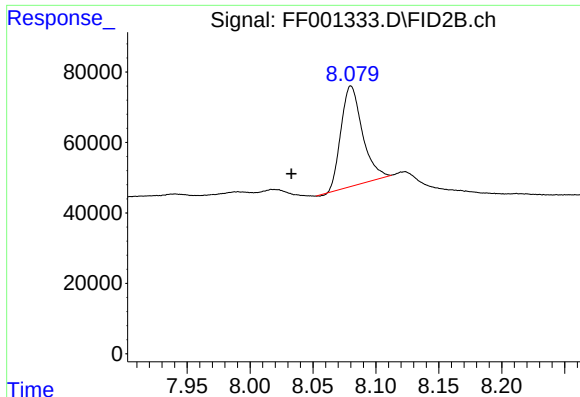

#4 N-TETRADECANE


R.T.: 8.080 min
Delta R.T.: 0.047 min
Response: 337436
Conc: 2.68 ug/ml

Instrument :
FID_F
ClientSampleId :

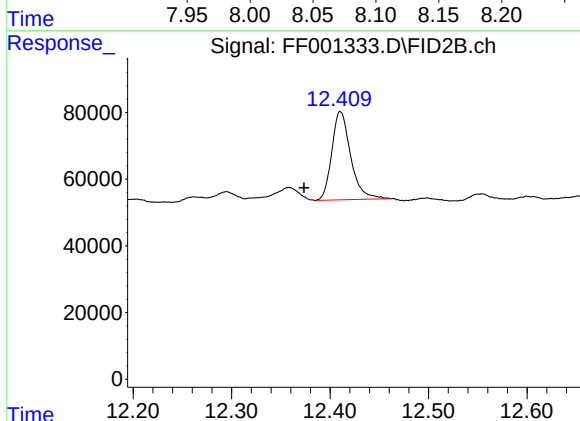


#7 N-EICOSANE

R.T.: 12.411 min
Delta R.T.: 0.037 min
Response: 353309
Conc: 2.84 ug/ml

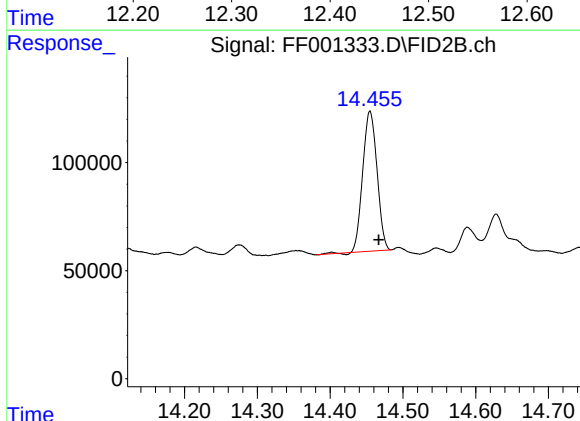


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.455 min
Delta R.T.: -0.012 min
Response: 888565
Conc: 8.25 ug/ml

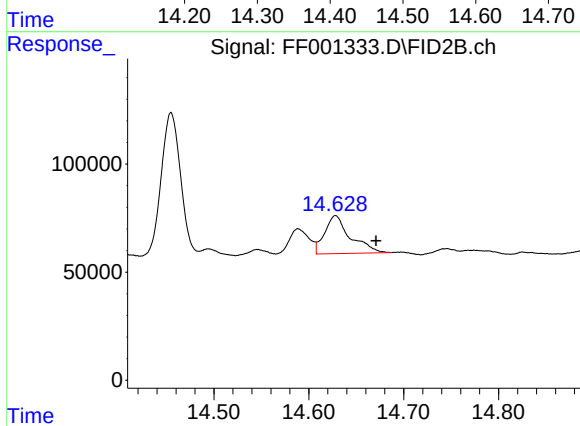

#10 N-TETRACOSANE


R.T.: 14.628 min
Delta R.T.: -0.043 min
Response: 330922
Conc: 2.71 ug/ml

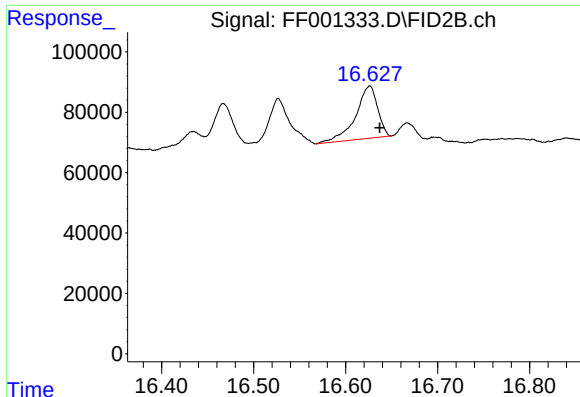

#12 N-OCTACOSANE


R.T.: 16.626 min
Delta R.T.: -0.011 min
Response: 287247
Conc: 2.38 ug/ml

Instrument :
FID_F
ClientSampleId :

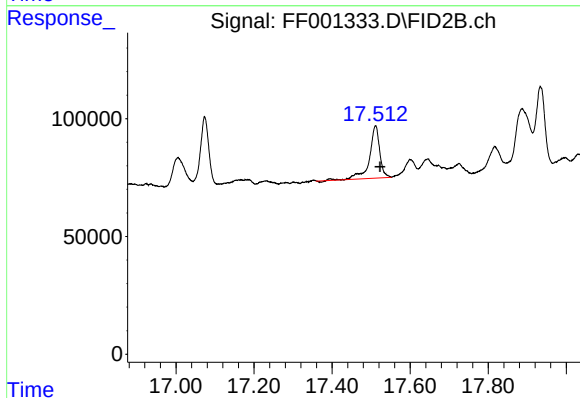


#13 N-TRIACONTANE

R.T.: 17.512 min
Delta R.T.: -0.011 min
Response: 409767
Conc: 3.41 ug/ml

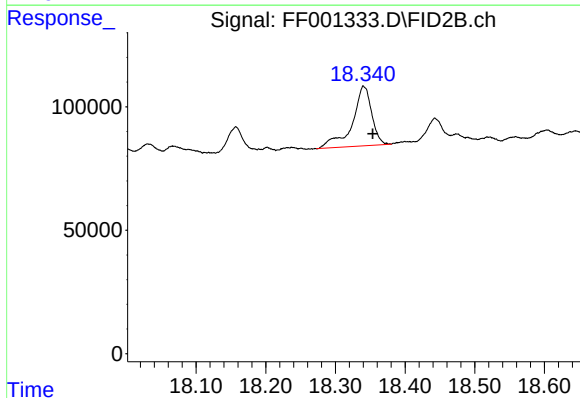

#14 N-DOTRIACONTANE

R.T.: 18.341 min
Delta R.T.: -0.013 min
Response: 464554
Conc: 3.94 ug/ml

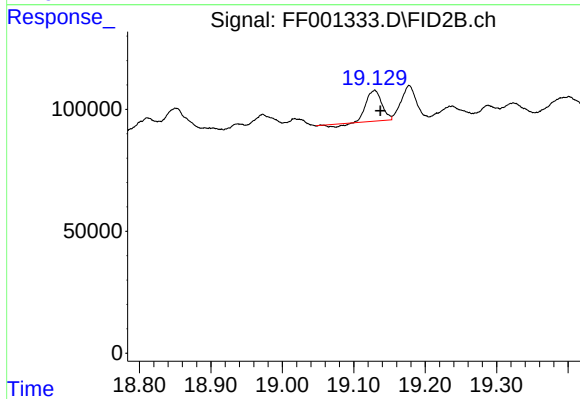

#15 N-TETRATRIACONTANE

R.T.: 19.129 min
Delta R.T.: -0.008 min
Response: 178332
Conc: 1.52 ug/ml