

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001338.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 18:29
 Operator : AJ\SJ
 Sample : J3820-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 23:06:41 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.453	1775897	16.486 ug/ml
Target Compounds			
4) N-TETRADECANE	8.077	557467	4.432 ug/ml
7) N-EICOSANE	12.407	1511638	12.152 ug/ml
8) N-DOCOSANE	13.570	543622	4.409 ug/ml
10) N-TETRACOSANE	14.624	1070008	8.777 ug/ml
12) N-OCTACOSANE	16.625	339527	2.818 ug/ml
13) N-TRIACONTANE	17.509	416171	3.462 ug/ml
14) N-DOTRIACONTANE	18.338	260007	2.205 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001338.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 18:29
Operator : AJ\SJ
Sample : J3820-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 23:06:41 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

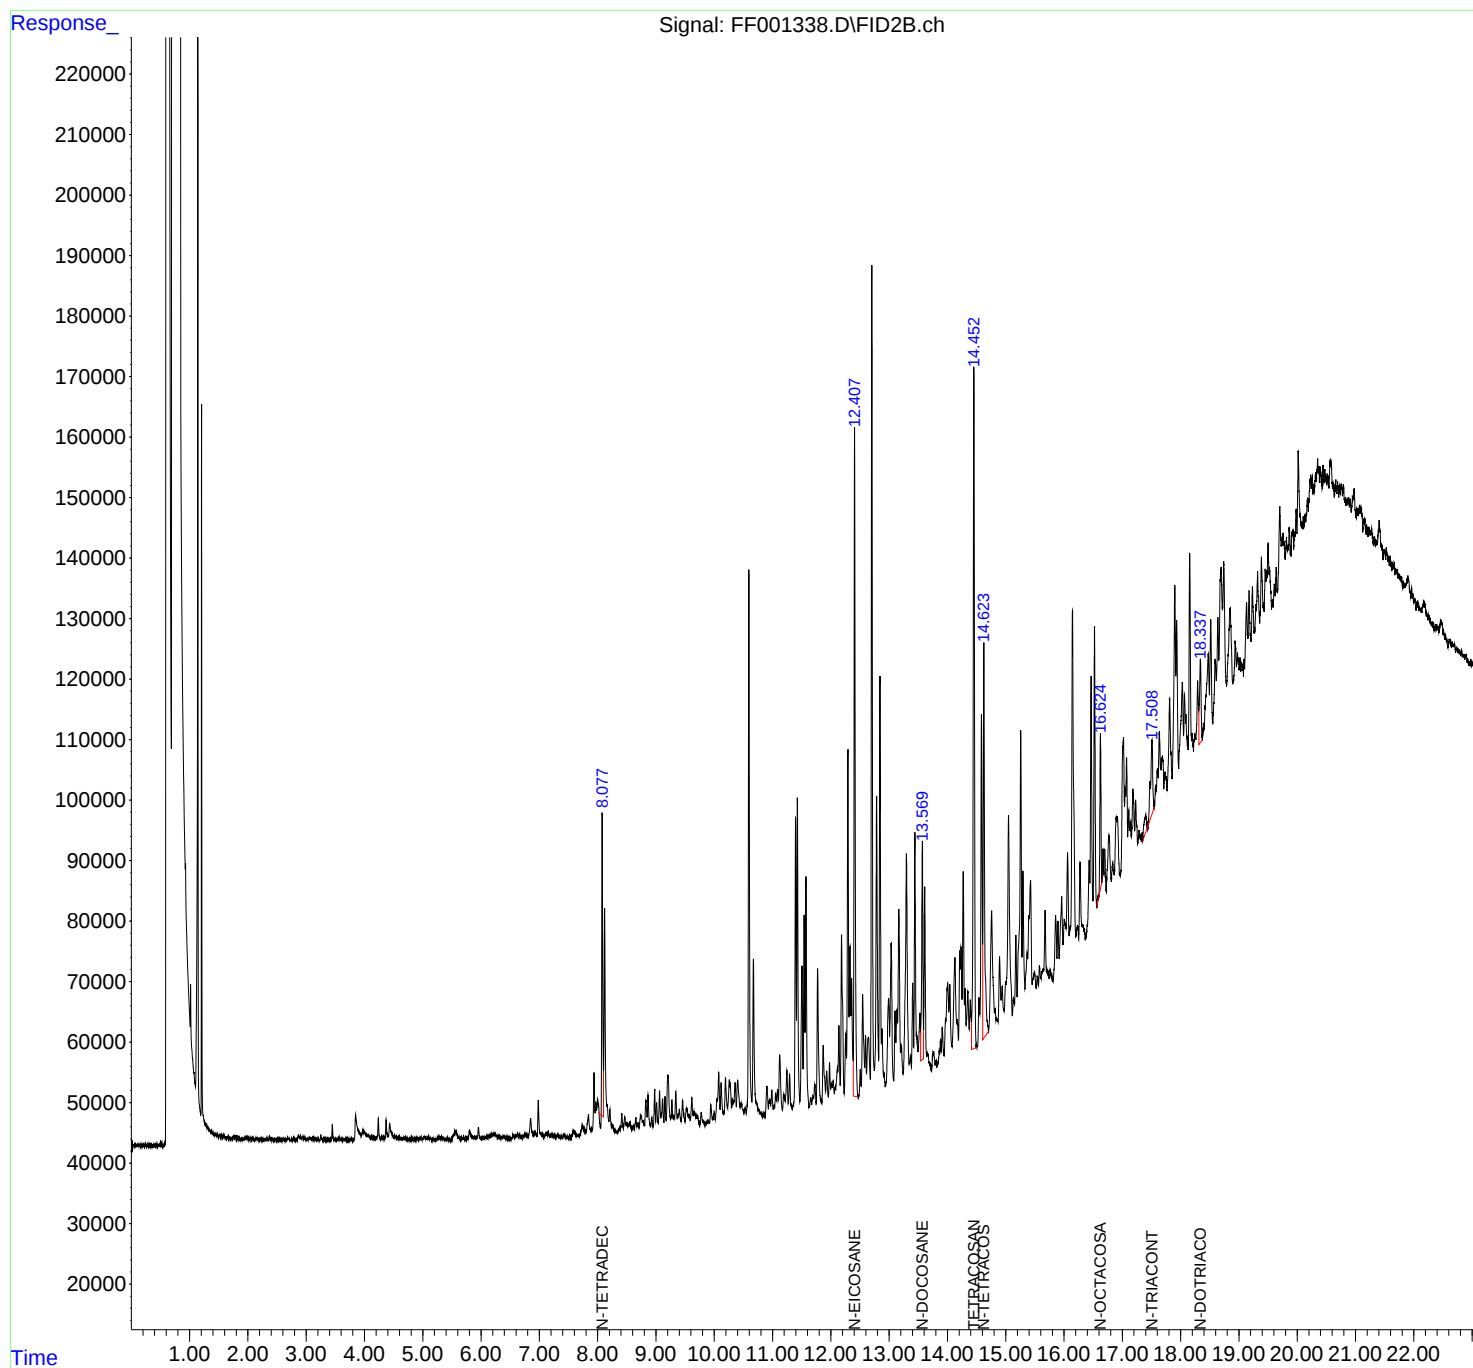


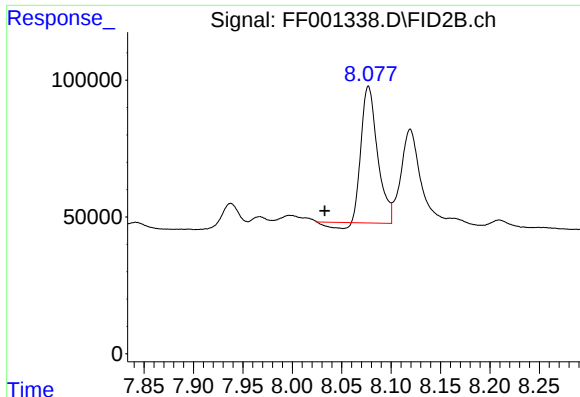

#4 N-TETRADECANE


R.T.: 8.077 min
Delta R.T.: 0.044 min
Response: 557467
Conc: 4.43 ug/ml

Instrument :
FID_F
ClientSampleId :

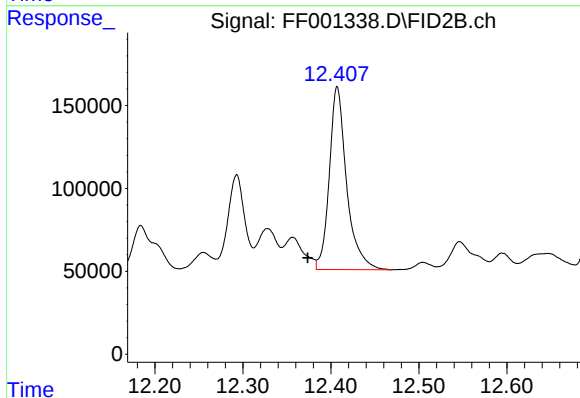


#7 N-EICOSANE

R.T.: 12.407 min
Delta R.T.: 0.034 min
Response: 1511638
Conc: 12.15 ug/ml

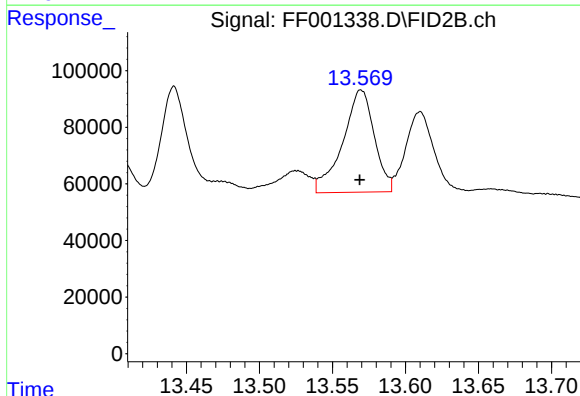


#8 N-DOCOSANE

R.T.: 13.570 min
Delta R.T.: 0.000 min
Response: 543622
Conc: 4.41 ug/ml

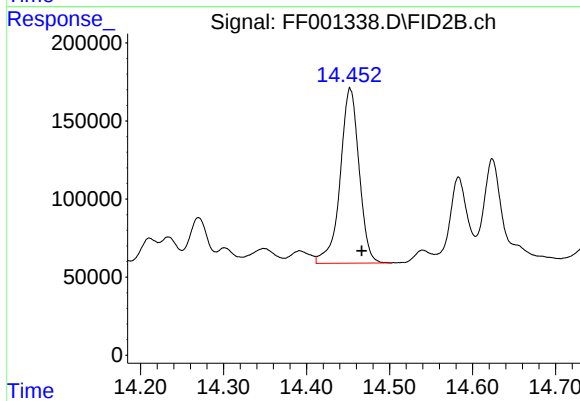

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.453 min
Delta R.T.: -0.014 min
Response: 1775897
Conc: 16.49 ug/ml

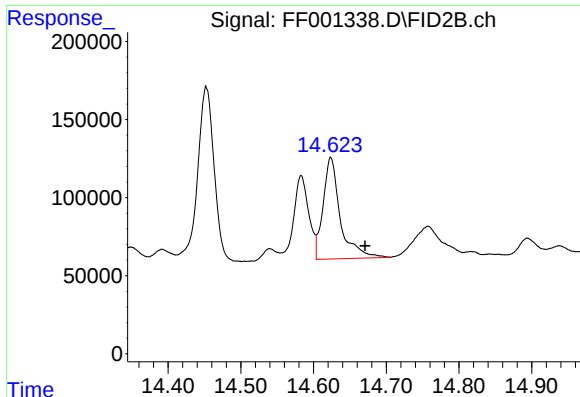

#10 N-TETRACOSANE


R.T.: 14.624 min
Delta R.T.: -0.047 min
Response: 1070008
Conc: 8.78 ug/ml

Instrument :
FID_F
ClientSampleId :

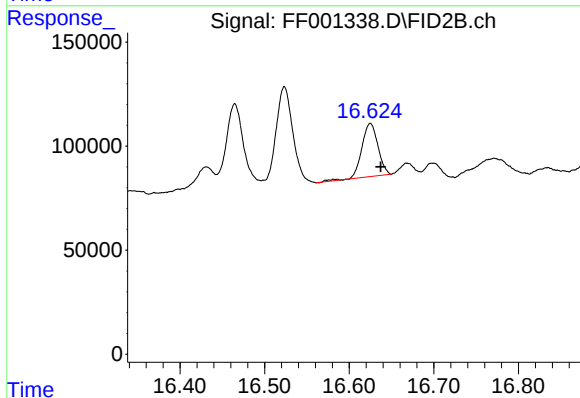


#12 N-OCTACOSANE

R.T.: 16.625 min
Delta R.T.: -0.012 min
Response: 339527
Conc: 2.82 ug/ml

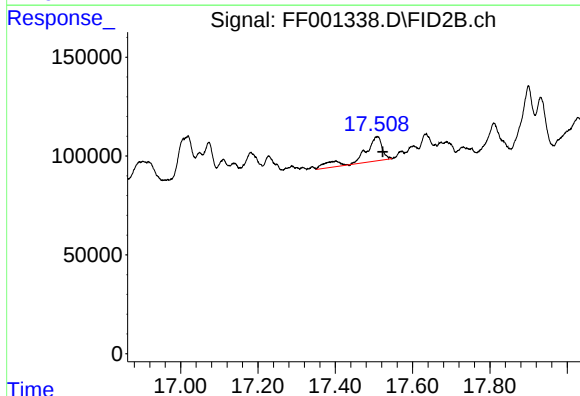

#13 N-TRIACONTANE

R.T.: 17.509 min
Delta R.T.: -0.014 min
Response: 416171
Conc: 3.46 ug/ml

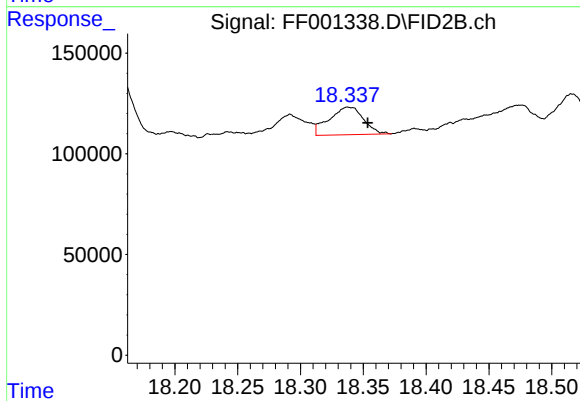

#14 N-DOTRIACONTANE

R.T.: 18.338 min
Delta R.T.: -0.016 min
Response: 260007
Conc: 2.21 ug/ml