

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001339.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 18:59
 Operator : AJ\SJ
 Sample : J3975-01
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 23:06:55 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.455	1670673	15.509 ug/ml
Target Compounds			
4) N-TETRADECANE	8.019	320015	2.544 ug/ml
5) N-HEXADECANE	9.615	438280	3.508 ug/ml
6) N-OCTADECANE	11.054	338659	2.702 ug/ml
7) N-EICOSANE	12.361	307490	2.472 ug/ml
8) N-DOCOSANE	13.558	173752	1.409 ug/ml
10) N-TETRACOSANE	14.628	105633	0.866 ug/ml
11) N-HEXACOSANE	15.675	507877	4.190 ug/ml
12) N-OCTACOSANE	16.627	402664	3.342 ug/ml
13) N-TRIACONTANE	17.509	347995	2.895 ug/ml
14) N-DOTRIACONTANE	18.305	1518743	12.881 ug/ml
15) N-TETRATRIACONTANE	19.125	396848	3.377 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001339.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 18:59
Operator : AJ\SJ
Sample : J3975-01
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 23:06:55 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

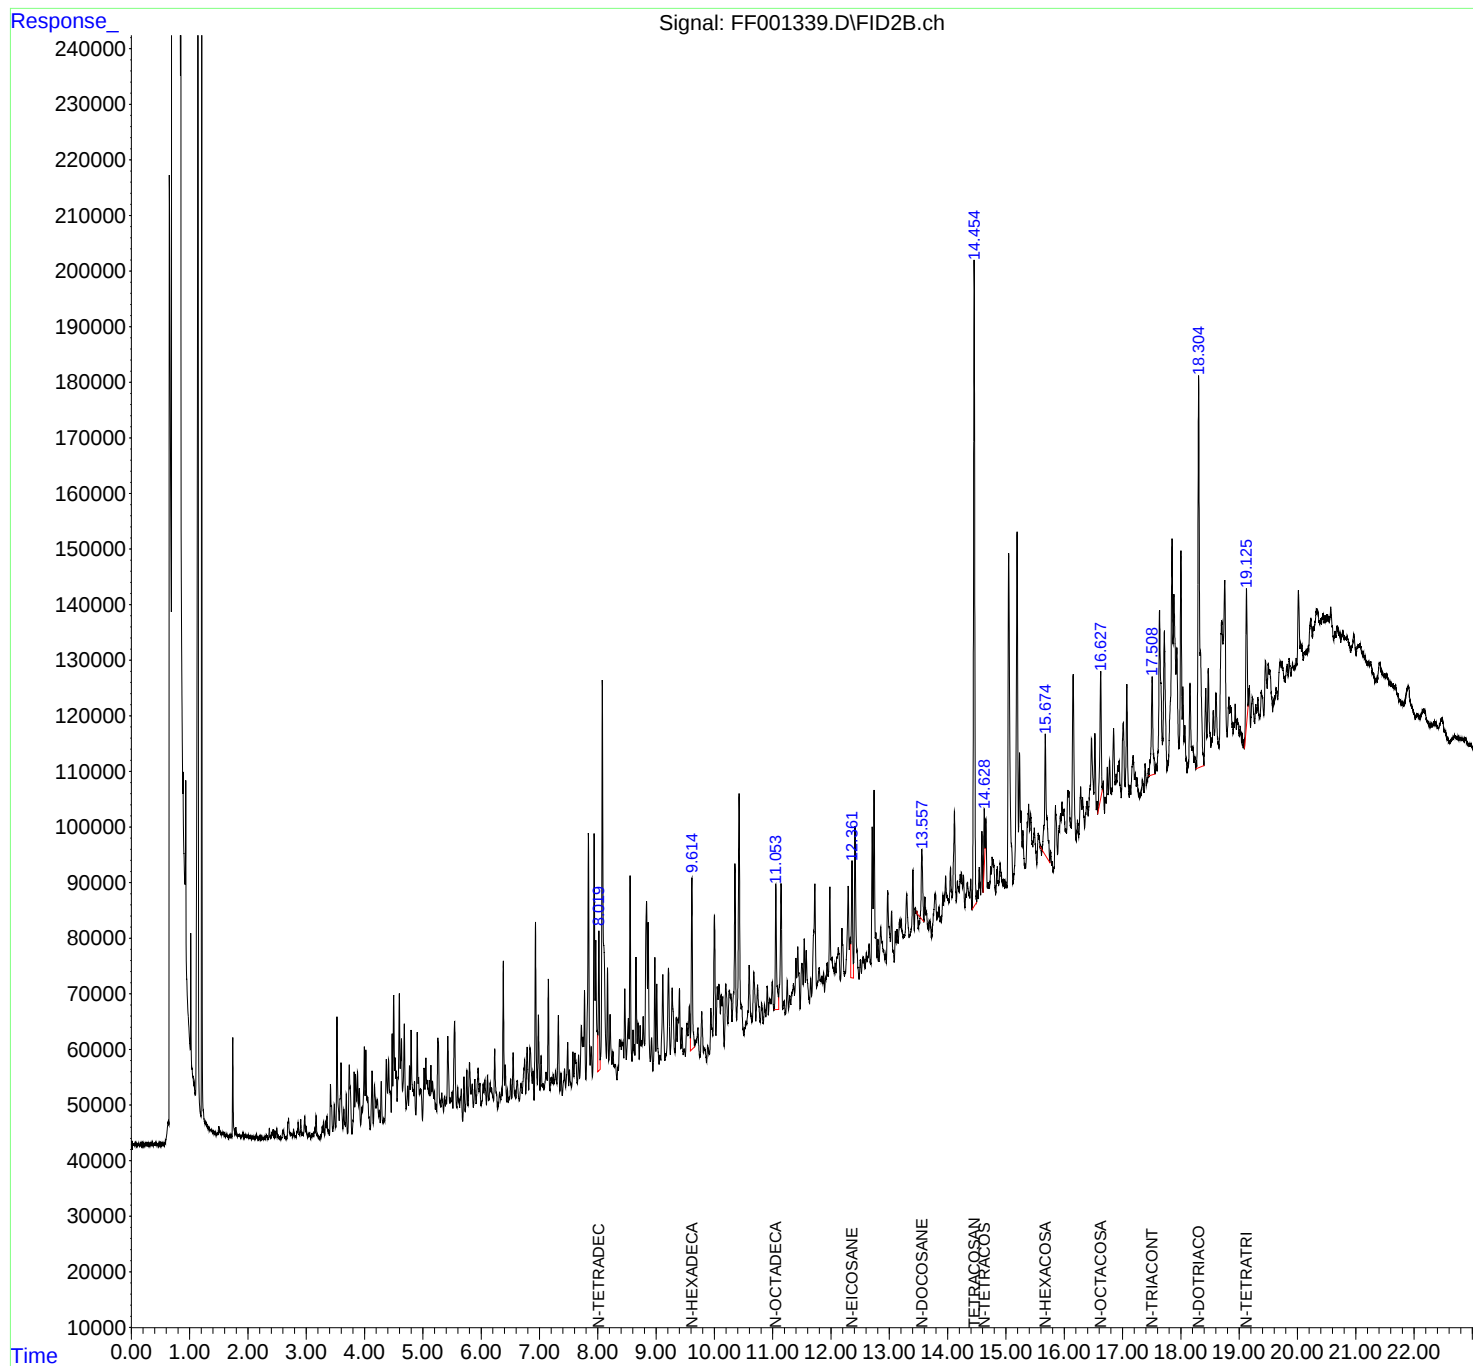


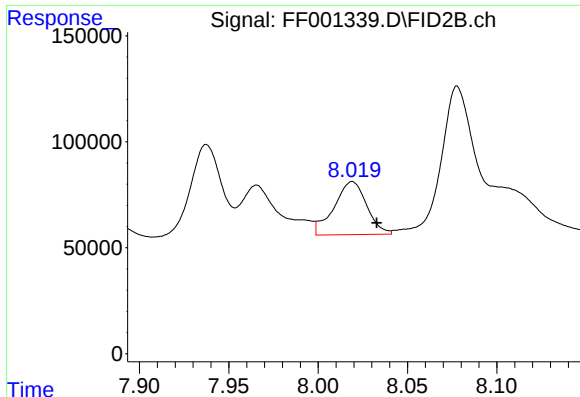

#4 N-TETRADECANE


R.T.: 8.019 min
Delta R.T.: -0.014 min
Response: 320015
Conc: 2.54 ug/ml

Instrument :
FID_F
ClientSampleId :

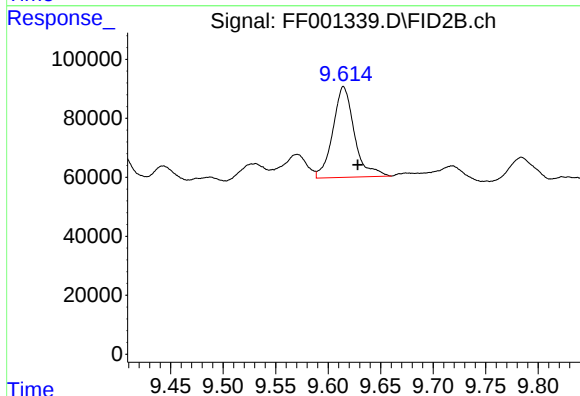


#5 N-HEXADECANE

R.T.: 9.615 min
Delta R.T.: -0.014 min
Response: 438280
Conc: 3.51 ug/ml

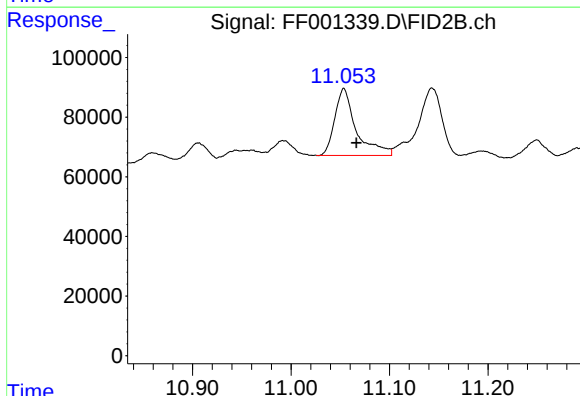


#6 N-OCTADECANE

R.T.: 11.054 min
Delta R.T.: -0.013 min
Response: 338659
Conc: 2.70 ug/ml

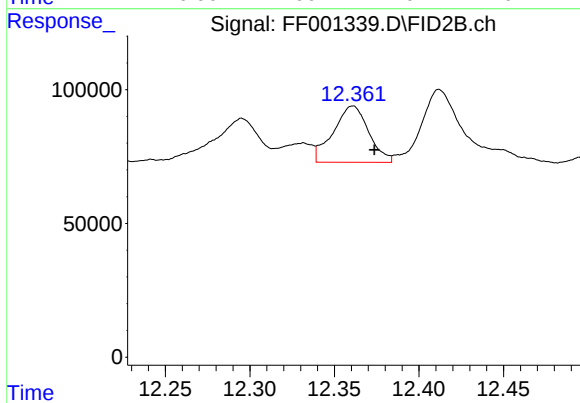

#7 N-EICOSANE


R.T.: 12.361 min
Delta R.T.: -0.013 min
Response: 307490
Conc: 2.47 ug/ml

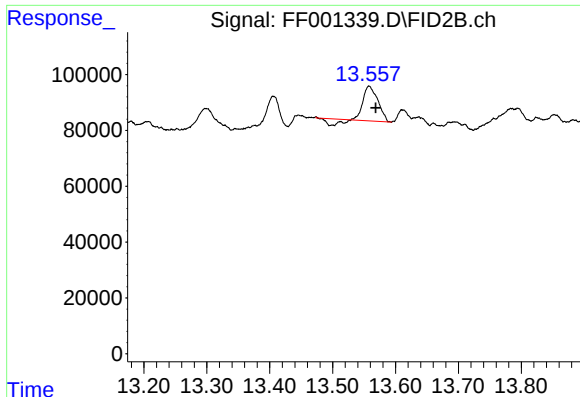

#8 N-DOCOSANE


R.T.: 13.558 min
Delta R.T.: -0.011 min
Response: 173752
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

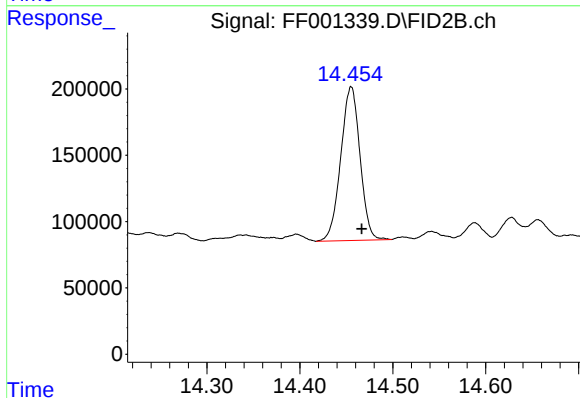


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.455 min
Delta R.T.: -0.011 min
Response: 1670673
Conc: 15.51 ug/ml

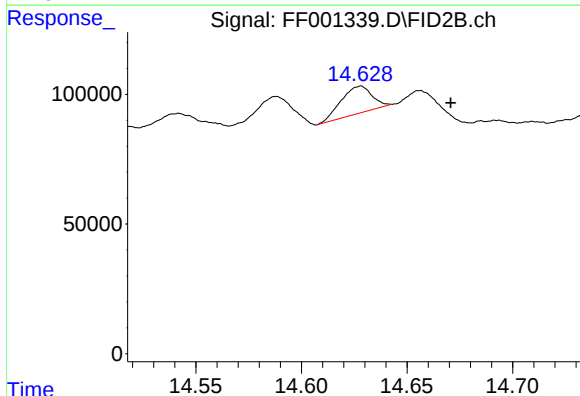


#10 N-TETRACOSANE

R.T.: 14.628 min
Delta R.T.: -0.043 min
Response: 105633
Conc: 0.87 ug/ml

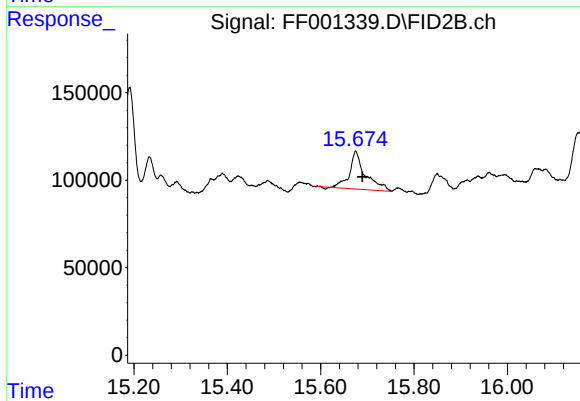

#11 N-HEXACOSANE


R.T.: 15.675 min
Delta R.T.: -0.014 min
Response: 507877
Conc: 4.19 ug/ml

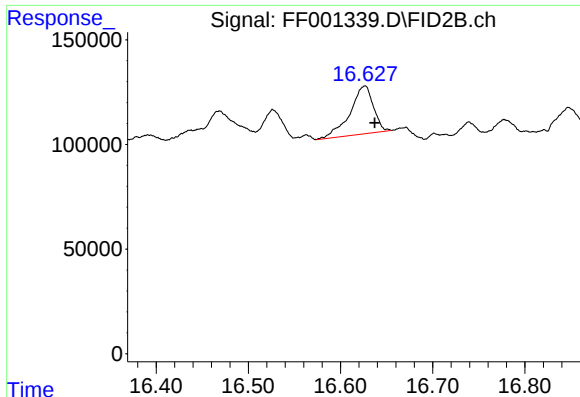

#12 N-OCTACOSANE


R.T.: 16.627 min
Delta R.T.: -0.011 min
Response: 402664
Conc: 3.34 ug/ml

Instrument :
FID_F
ClientSampleId :

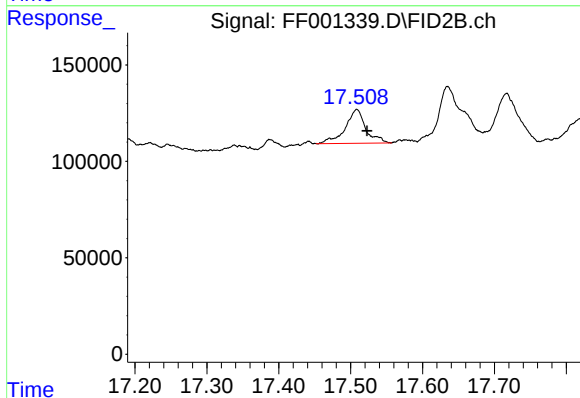


#13 N-TRIACONTANE

R.T.: 17.509 min
Delta R.T.: -0.014 min
Response: 347995
Conc: 2.89 ug/ml

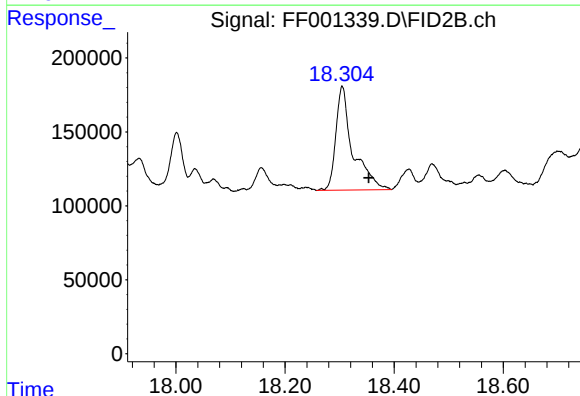

#14 N-DOTRIACONTANE

R.T.: 18.305 min
Delta R.T.: -0.048 min
Response: 1518743
Conc: 12.88 ug/ml

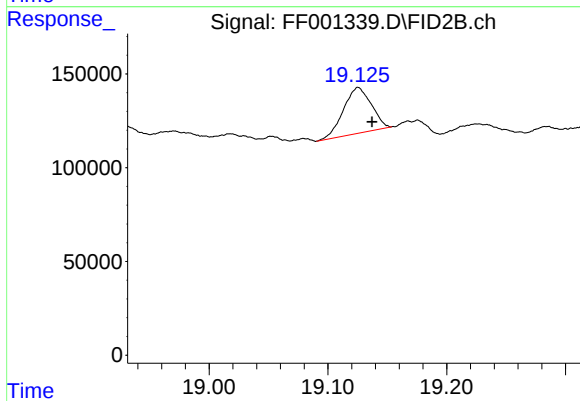

#15 N-TETRATRIACONTANE

R.T.: 19.125 min
Delta R.T.: -0.012 min
Response: 396848
Conc: 3.38 ug/ml