

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001340.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 19:29
 Operator : AJ\SJ
 Sample : J3975-02
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 23:07:14 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.454	1622553	15.062 ug/ml
Target Compounds			
4) N-TETRADECANE	8.019	317785	2.527 ug/ml
5) N-HEXADECANE	9.614	425476	3.405 ug/ml
6) N-OCTADECANE	11.053	344332	2.748 ug/ml
7) N-EICOSANE	12.359	397576	3.196 ug/ml
8) N-DOCOSANE	13.558	249098	2.020 ug/ml
10) N-TETRACOSANE	14.627	105314	0.864 ug/ml
11) N-HEXACOSANE	15.675	557873	4.602 ug/ml
12) N-OCTACOSANE	16.624	414429	3.440 ug/ml
13) N-TRIACONTANE	17.507	582828	4.848 ug/ml
14) N-DOTRIACONTANE	18.334	441957	3.748 ug/ml
15) N-TETRATRIACONTANE	19.123	366935	3.122 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001340.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 19:29
Operator : AJ\SJ
Sample : J3975-02
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 23:07:14 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

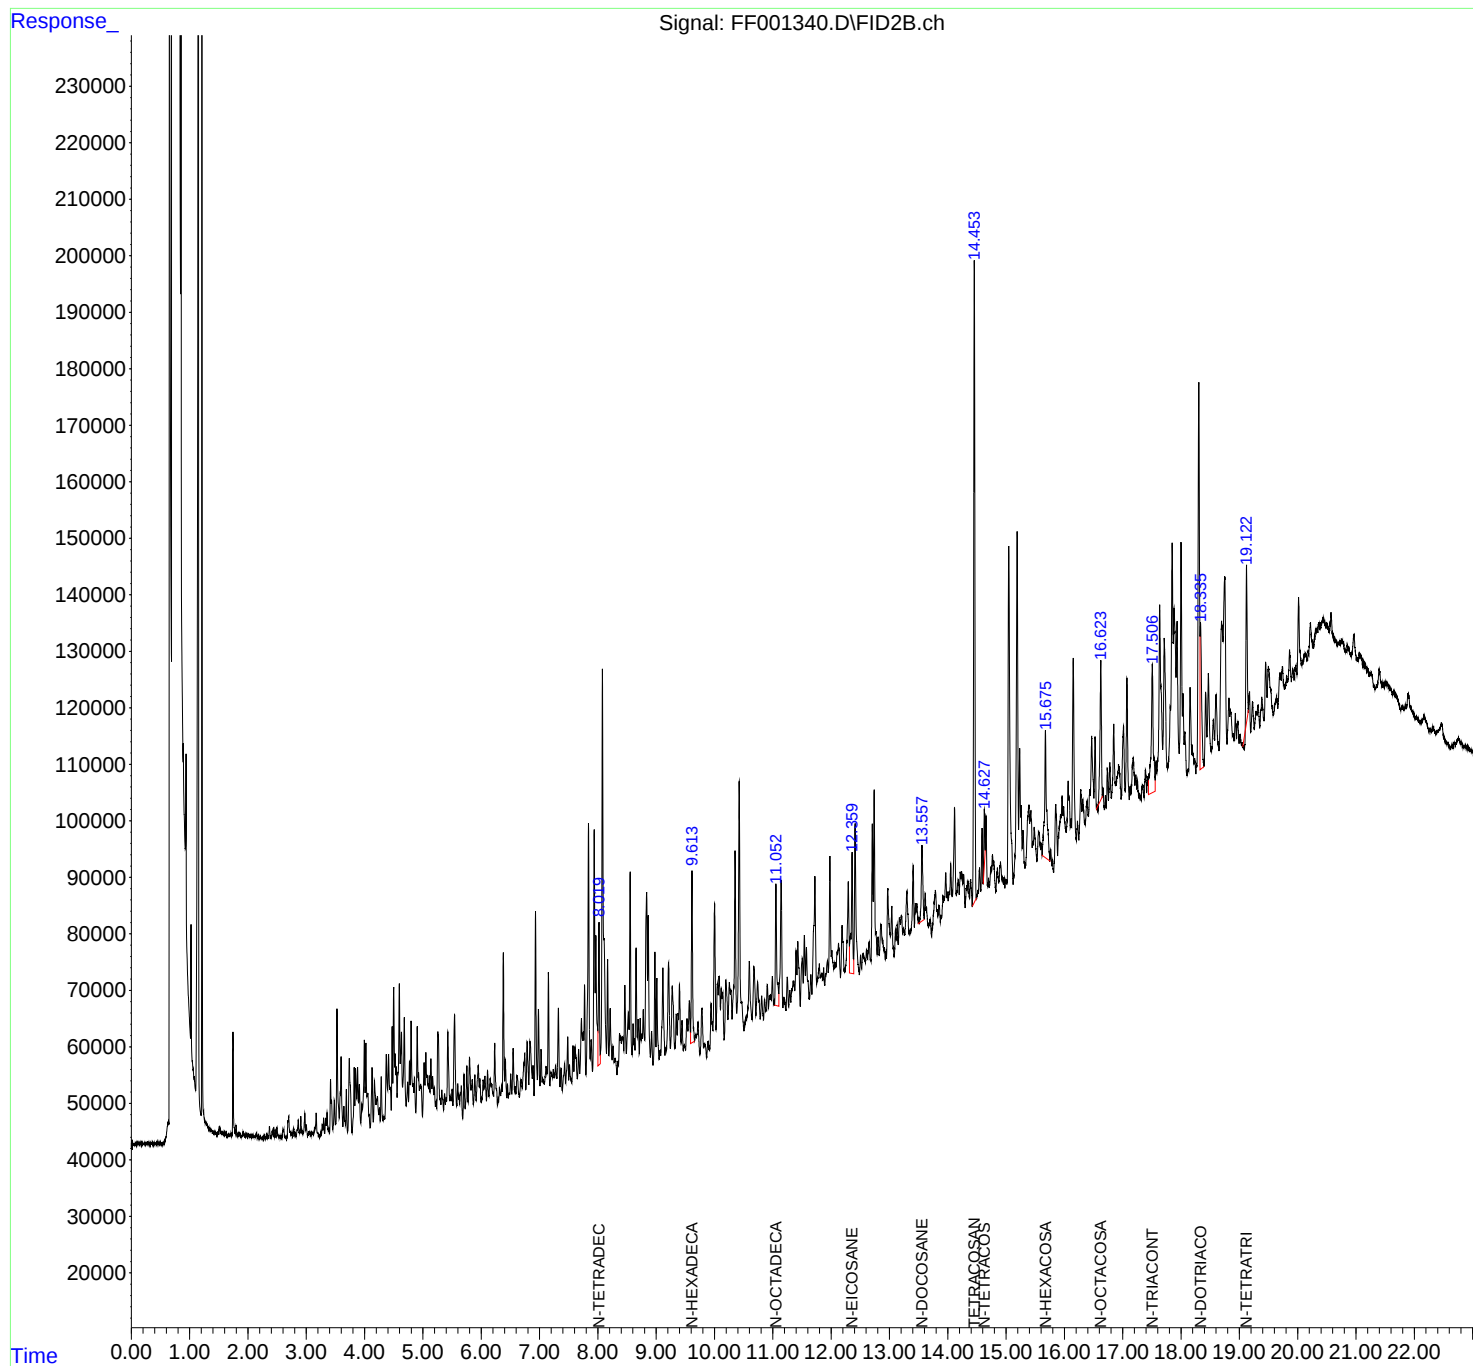


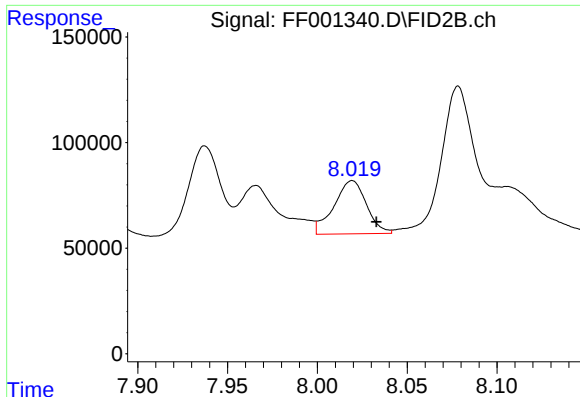

#4 N-TETRADECANE


R.T.: 8.019 min
Delta R.T.: -0.013 min
Response: 317785
Conc: 2.53 ug/ml

Instrument :
FID_F
ClientSampleId :

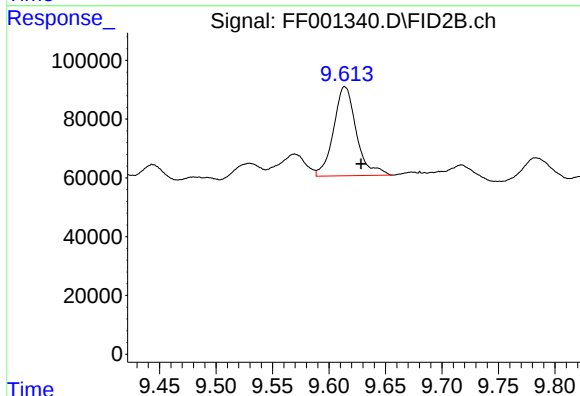


#5 N-HEXADECANE

R.T.: 9.614 min
Delta R.T.: -0.014 min
Response: 425476
Conc: 3.41 ug/ml

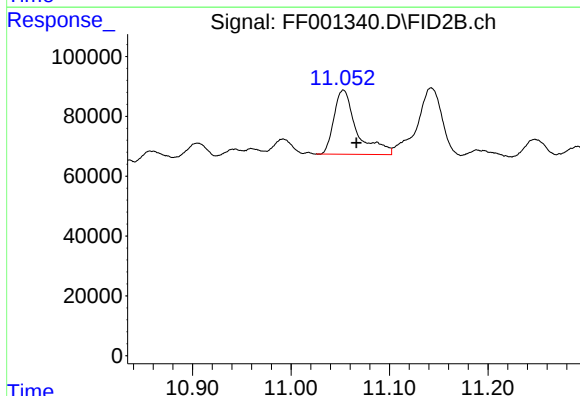


#6 N-OCTADECANE

R.T.: 11.053 min
Delta R.T.: -0.013 min
Response: 344332
Conc: 2.75 ug/ml

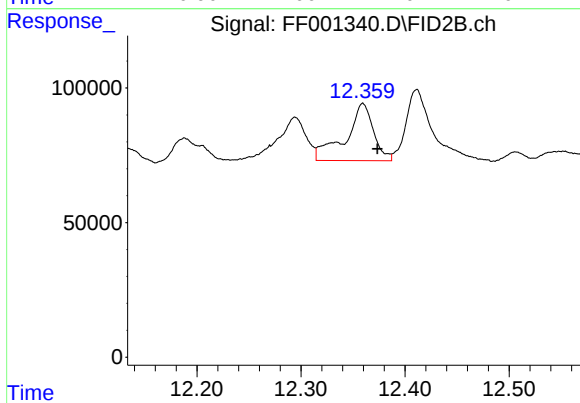

#7 N-EICOSANE


R.T.: 12.359 min
Delta R.T.: -0.014 min
Response: 397576
Conc: 3.20 ug/ml

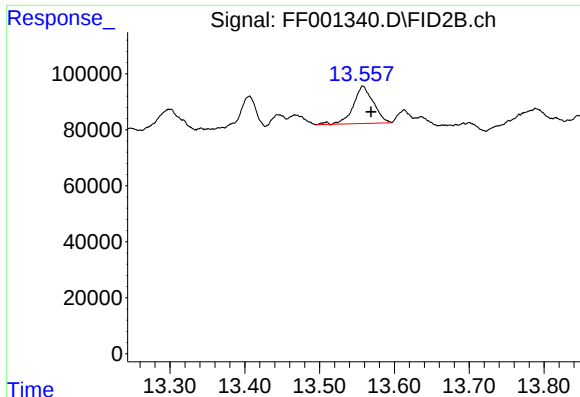

#8 N-DOCOSANE


R.T.: 13.558 min
Delta R.T.: -0.011 min
Response: 249098
Conc: 2.02 ug/ml

Instrument :
FID_F
ClientSampleId :

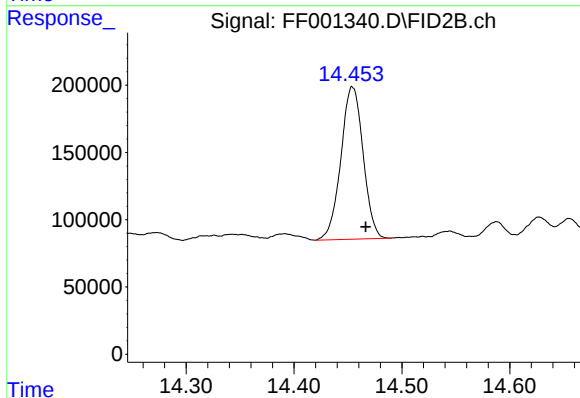


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.454 min
Delta R.T.: -0.012 min
Response: 1622553
Conc: 15.06 ug/ml

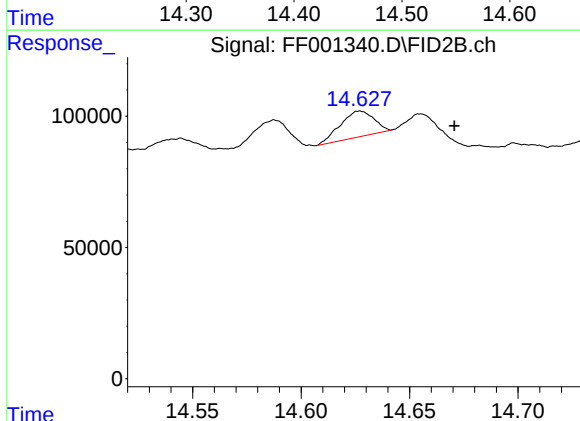


#10 N-TETRACOSANE

R.T.: 14.627 min
Delta R.T.: -0.044 min
Response: 105314
Conc: 0.86 ug/ml

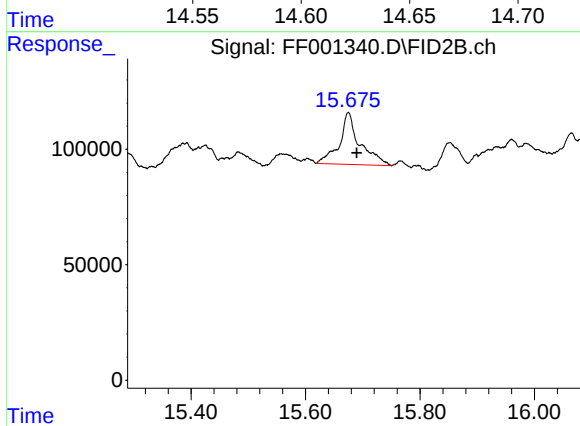

#11 N-HEXACOSANE


R.T.: 15.675 min
Delta R.T.: -0.015 min
Response: 557873
Conc: 4.60 ug/ml

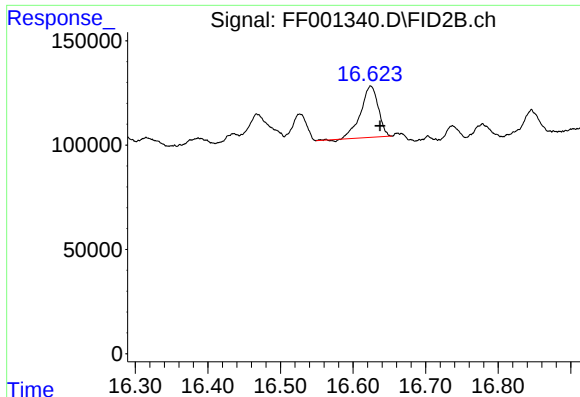

#12 N-OCTACOSANE


R.T.: 16.624 min
Delta R.T.: -0.013 min
Response: 414429
Conc: 3.44 ug/ml

Instrument :
FID_F
ClientSampleId :

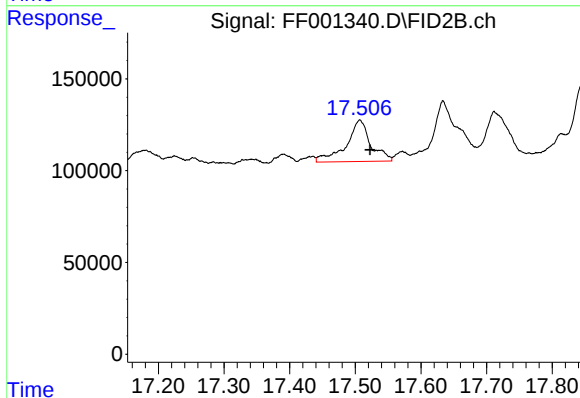


#13 N-TRIACONTANE

R.T.: 17.507 min
Delta R.T.: -0.016 min
Response: 582828
Conc: 4.85 ug/ml

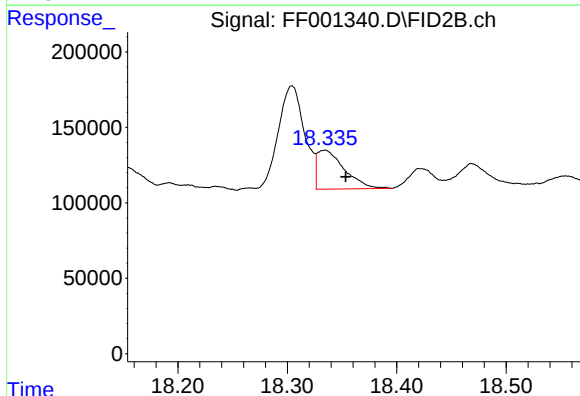

#14 N-DOTRIACONTANE

R.T.: 18.334 min
Delta R.T.: -0.019 min
Response: 441957
Conc: 3.75 ug/ml

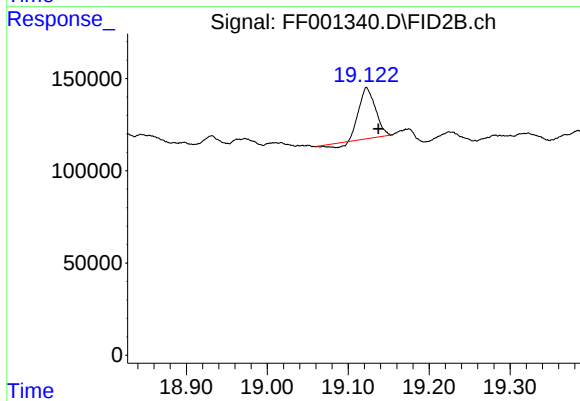

#15 N-TETRATRIACONTANE

R.T.: 19.123 min
Delta R.T.: -0.014 min
Response: 366935
Conc: 3.12 ug/ml