

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001341.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 19:59
 Operator : AJ\SJ
 Sample : J3975-03
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 23:07:31 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.458	2113569	19.620 ug/ml
Target Compounds			
3) N-DODECANE	6.231	200560	1.601 ug/ml
4) N-TETRADECANE	7.989	327298	2.602 ug/ml
5) N-HEXADECANE	9.617	378427	3.029 ug/ml
6) N-OCTADECANE	11.055	212346	1.694 ug/ml
7) N-EICOSANE	12.363	742782	5.971 ug/ml
8) N-DOCOSANE	13.561	879307	7.131 ug/ml
10) N-TETRACOSANE	14.657	516489	4.237 ug/ml
11) N-HEXACOSANE	15.680	1082823	8.933 ug/ml
12) N-OCTACOSANE	16.633	937991	7.786 ug/ml
13) N-TRIACONTANE	17.508	722944	6.014 ug/ml
14) N-DOTRIACONTANE	18.344	303494	2.574 ug/ml
15) N-TETRATRIACONTANE	19.137	1278008	10.874 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001341.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 19:59
Operator : AJ\SJ
Sample : J3975-03
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 23:07:31 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

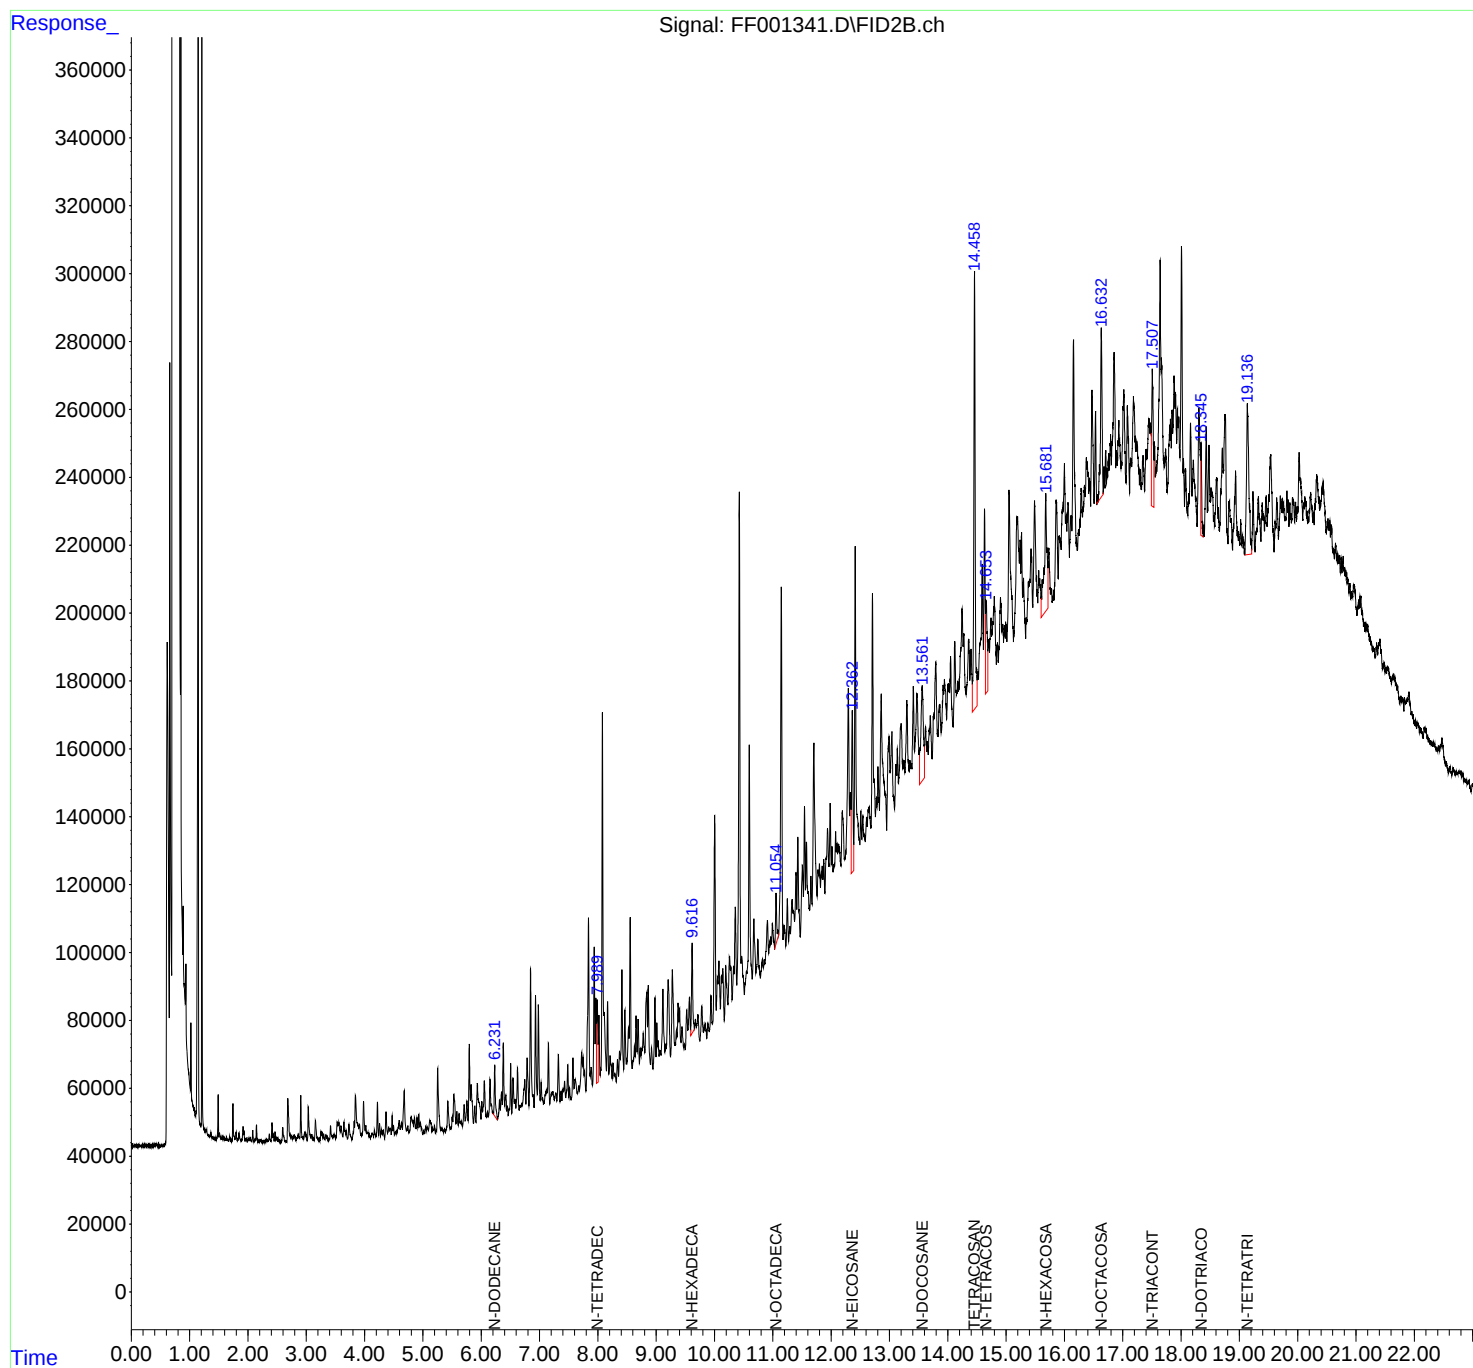


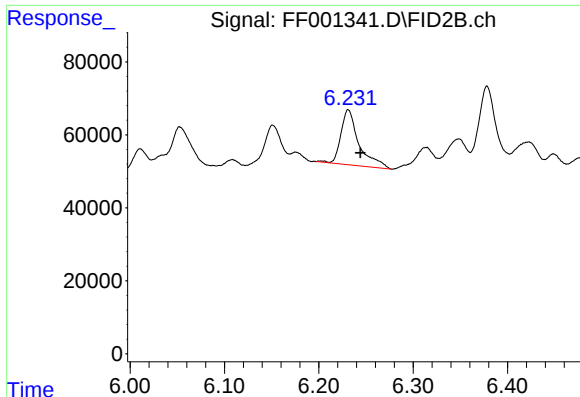

#3 N-DODECANE


R.T.: 6.231 min
Delta R.T.: -0.013 min
Response: 200560
Conc: 1.60 ug/ml

Instrument :
FID_F
ClientSampleId :

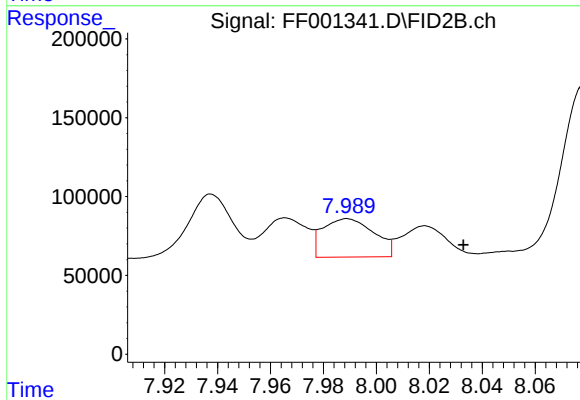


#4 N-TETRADECANE

R.T.: 7.989 min
Delta R.T.: -0.044 min
Response: 327298
Conc: 2.60 ug/ml

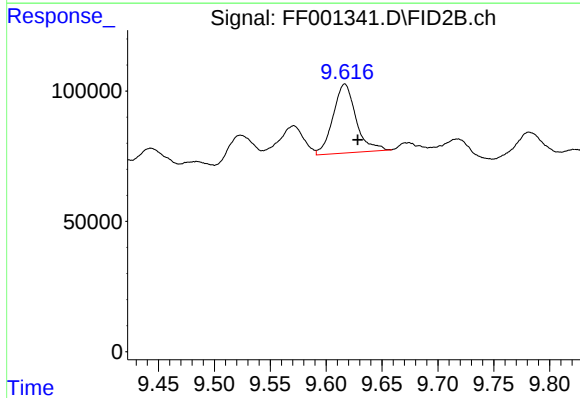


#5 N-HEXADECANE

R.T.: 9.617 min
Delta R.T.: -0.012 min
Response: 378427
Conc: 3.03 ug/ml

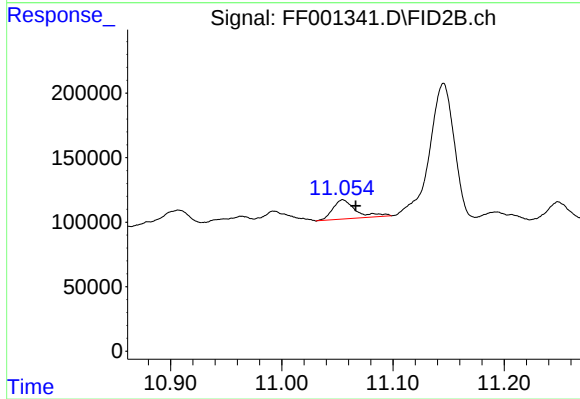

#6 N-OCTADECANE


R.T.: 11.055 min
Delta R.T.: -0.011 min
Response: 212346
Conc: 1.69 ug/ml

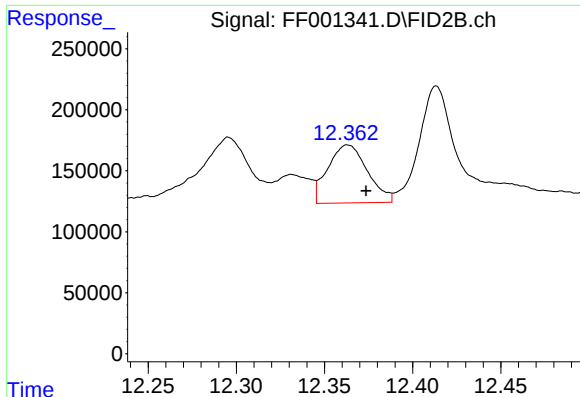

#7 N-EICOSANE


R.T.: 12.363 min
Delta R.T.: -0.010 min
Response: 742782
Conc: 5.97 ug/ml

Instrument :
FID_F
ClientSampleId :

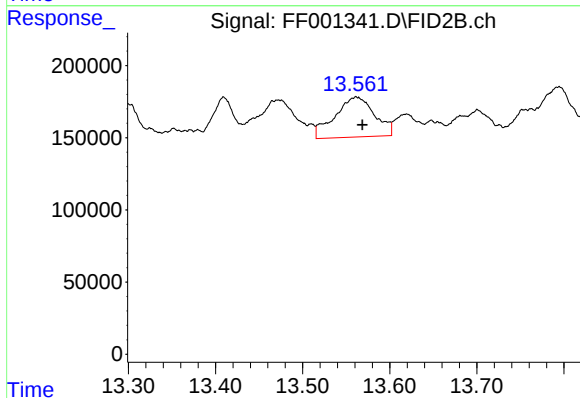


#8 N-DOCOSANE

R.T.: 13.561 min
Delta R.T.: -0.007 min
Response: 879307
Conc: 7.13 ug/ml

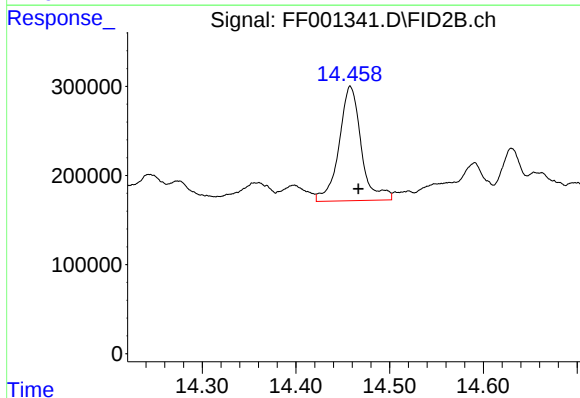


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.458 min
Delta R.T.: -0.009 min
Response: 2113569
Conc: 19.62 ug/ml

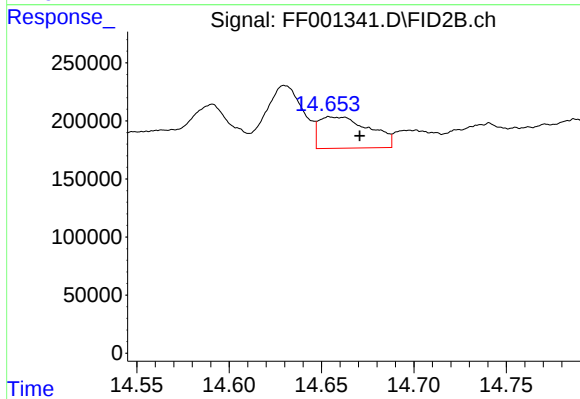

#10 N-TETRACOSANE


R.T.: 14.657 min
Delta R.T.: -0.014 min
Response: 516489
Conc: 4.24 ug/ml

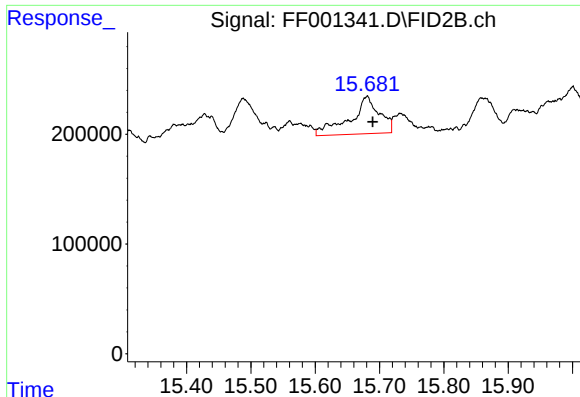

#11 N-HEXACOSANE


R.T.: 15.680 min
Delta R.T.: -0.009 min
Response: 1082823
Conc: 8.93 ug/ml

Instrument :
FID_F
ClientSampleId :

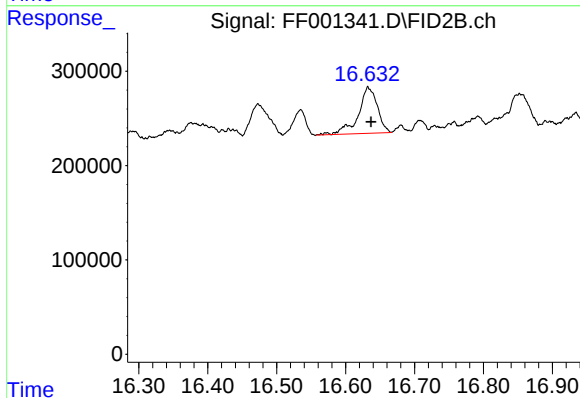


#12 N-OCTACOSANE

R.T.: 16.633 min
Delta R.T.: -0.004 min
Response: 937991
Conc: 7.79 ug/ml

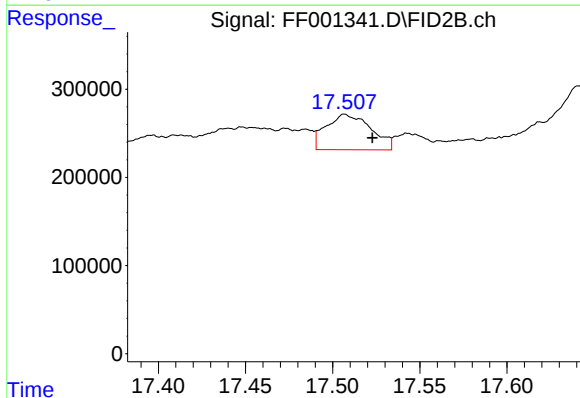


#13 N-TRIACONTANE

R.T.: 17.508 min
Delta R.T.: -0.015 min
Response: 722944
Conc: 6.01 ug/ml

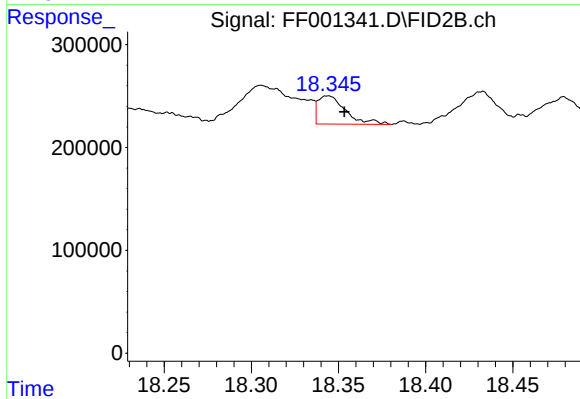

#14 N-DOTRIACONTANE

R.T.: 18.344 min
Delta R.T.: -0.010 min
Response: 303494
Conc: 2.57 ug/ml

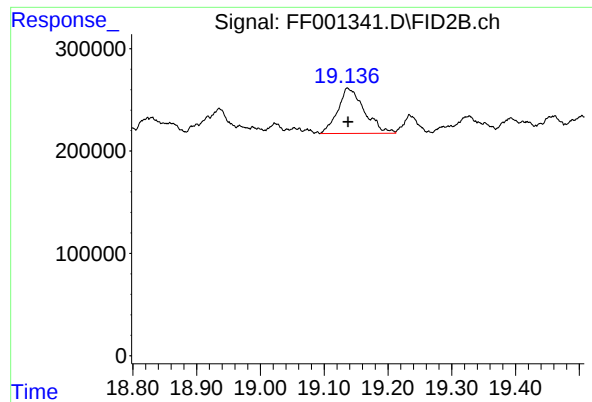

#15 N-TETRATRIACONTANE

R.T.: 19.137 min
Delta R.T.: 0.000 min
Response: 1278008
Conc: 10.87 ug/ml

Instrument :
FID_F
ClientSampleId :