

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001343.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jul 2018 20:59
 Operator : AJ\SJ
 Sample : J3975-05
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 23:08:04 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.455	2305669	21.404 ug/ml
Target Compounds			
4) N-TETRADECANE	8.079	895405	7.119 ug/ml
11) N-HEXACOSANE	15.675	194136	1.602 ug/ml
12) N-OCTACOSANE	16.622	297817	2.472 ug/ml
13) N-TRIACONTANE	17.508	326453	2.716 ug/ml
14) N-DOTRIACONTANE	18.338	282858	2.399 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001343.D
Signal(s) : FID2B.ch
Acq On : 13 Jul 2018 20:59
Operator : AJ\SJ
Sample : J3975-05
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 23:08:04 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

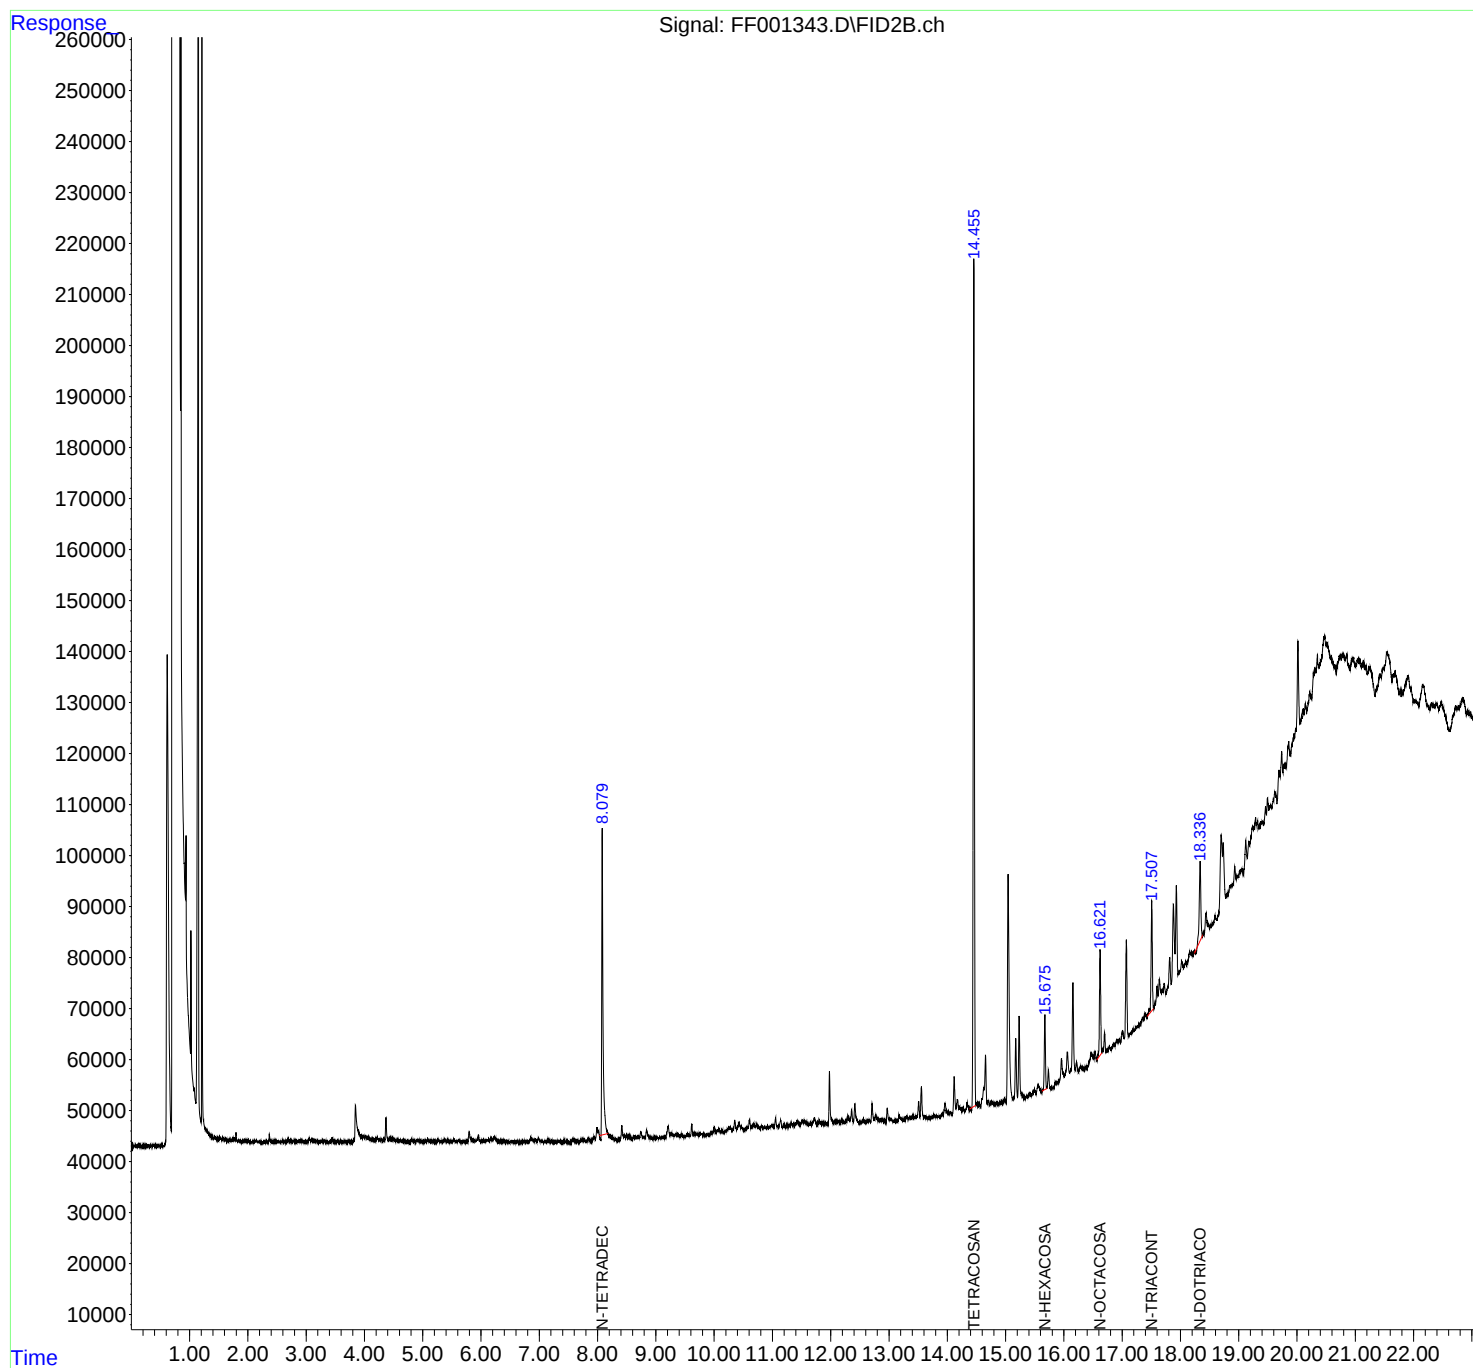


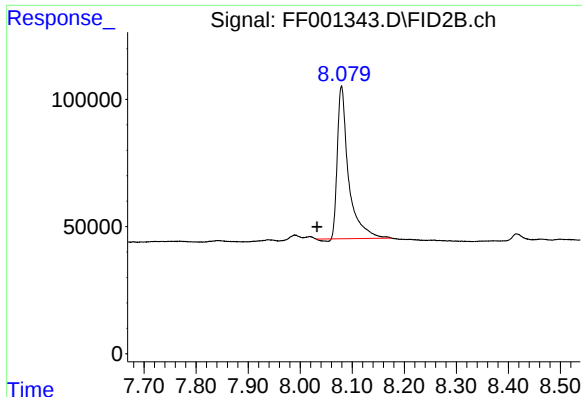

#4 N-TETRADECANE


R.T.: 8.079 min
Delta R.T.: 0.047 min
Response: 895405
Conc: 7.12 ug/ml

Instrument :
FID_F
ClientSampleId :

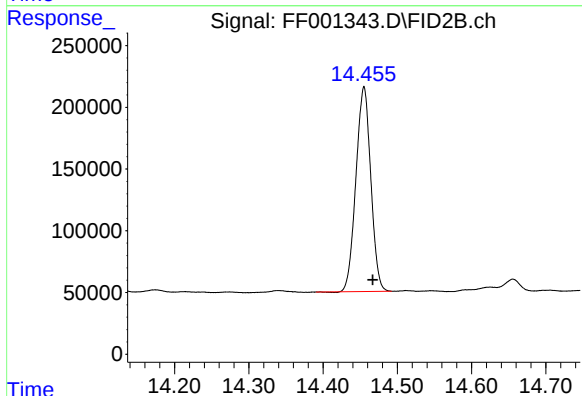


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.455 min
Delta R.T.: -0.011 min
Response: 2305669
Conc: 21.40 ug/ml

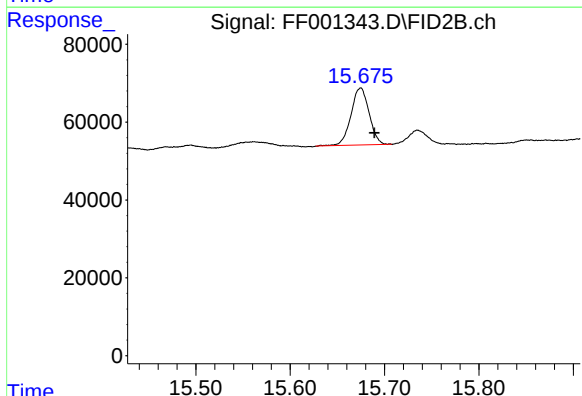


#11 N-HEXACOSANE

R.T.: 15.675 min
Delta R.T.: -0.015 min
Response: 194136
Conc: 1.60 ug/ml

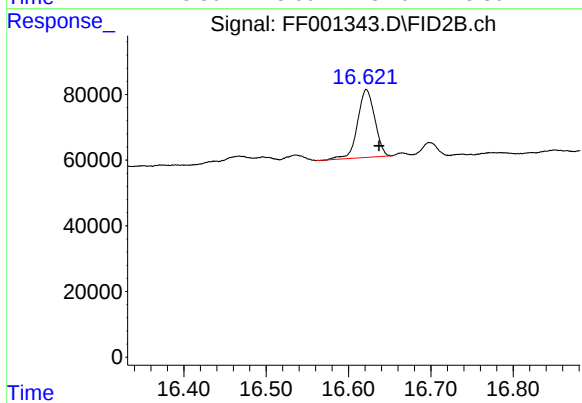

#12 N-OCTACOSANE


R.T.: 16.622 min
Delta R.T.: -0.015 min
Response: 297817
Conc: 2.47 ug/ml

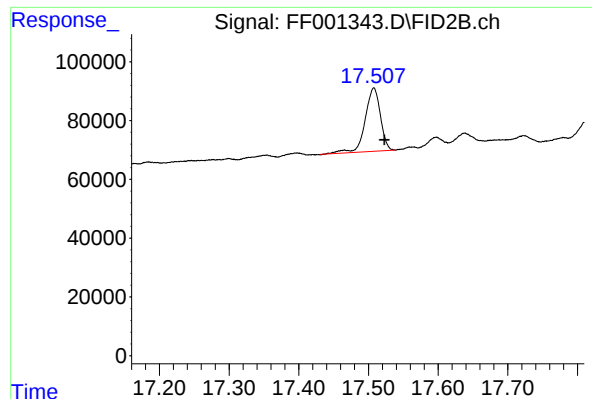

#13 N-TRIACONTANE

R.T.: 17.508 min
Delta R.T.: -0.015 min
Response: 326453
Conc: 2.72 ug/ml

Instrument :
FID_F
ClientSampleId :

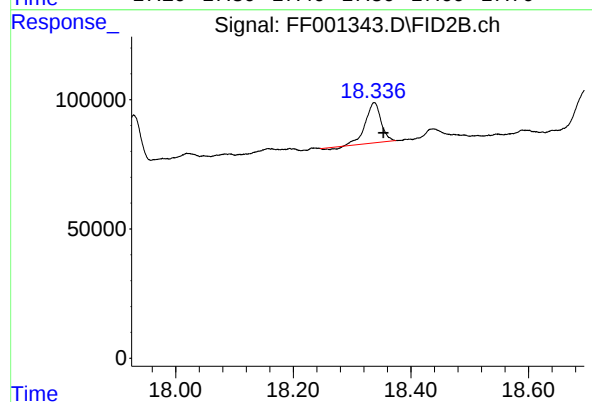

#14 N-DOTRIACONTANE

R.T.: 18.338 min
Delta R.T.: -0.016 min
Response: 282858
Conc: 2.40 ug/ml