

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF071318\  
 Data File : FF001353.D  
 Signal(s) : FID2B.ch  
 Acq On : 14 Jul 2018 02:00  
 Operator : AJ\SJ  
 Sample : J3975-07  
 Misc :  
 ALS Vial : 78 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jul 14 04:18:23 2018  
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_F\Method\FF070218.M  
 Quant Title :  
 QLast Update : Mon Jul 02 13:42:46 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.453 | 1557515  | 14.458 ug/ml |
| Target Compounds              |        |          |              |
| 4) N-TETRADECANE              | 8.077  | 455248   | 3.620 ug/ml  |
| 7) N-EICOSANE                 | 12.408 | 1619937  | 13.023 ug/ml |
| 10) N-TETRACOSANE             | 14.624 | 841496   | 6.903 ug/ml  |
| 11) N-HEXACOSANE              | 15.675 | 284009   | 2.343 ug/ml  |
| 12) N-OCTACOSANE              | 16.627 | 447214   | 3.712 ug/ml  |
| 13) N-TRIACONTANE             | 17.506 | 410000   | 3.411 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.336 | 282983   | 2.400 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.126 | 272144   | 2.315 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF071318\  
Data File : FF001353.D  
Signal(s) : FID2B.ch  
Acq On : 14 Jul 2018 02:00  
Operator : AJ\SJ  
Sample : J3975-07  
Misc :  
ALS Vial : 78 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 14 04:18:23 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_F\Method\FF070218.M  
Quant Title :  
QLast Update : Mon Jul 02 13:42:46 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

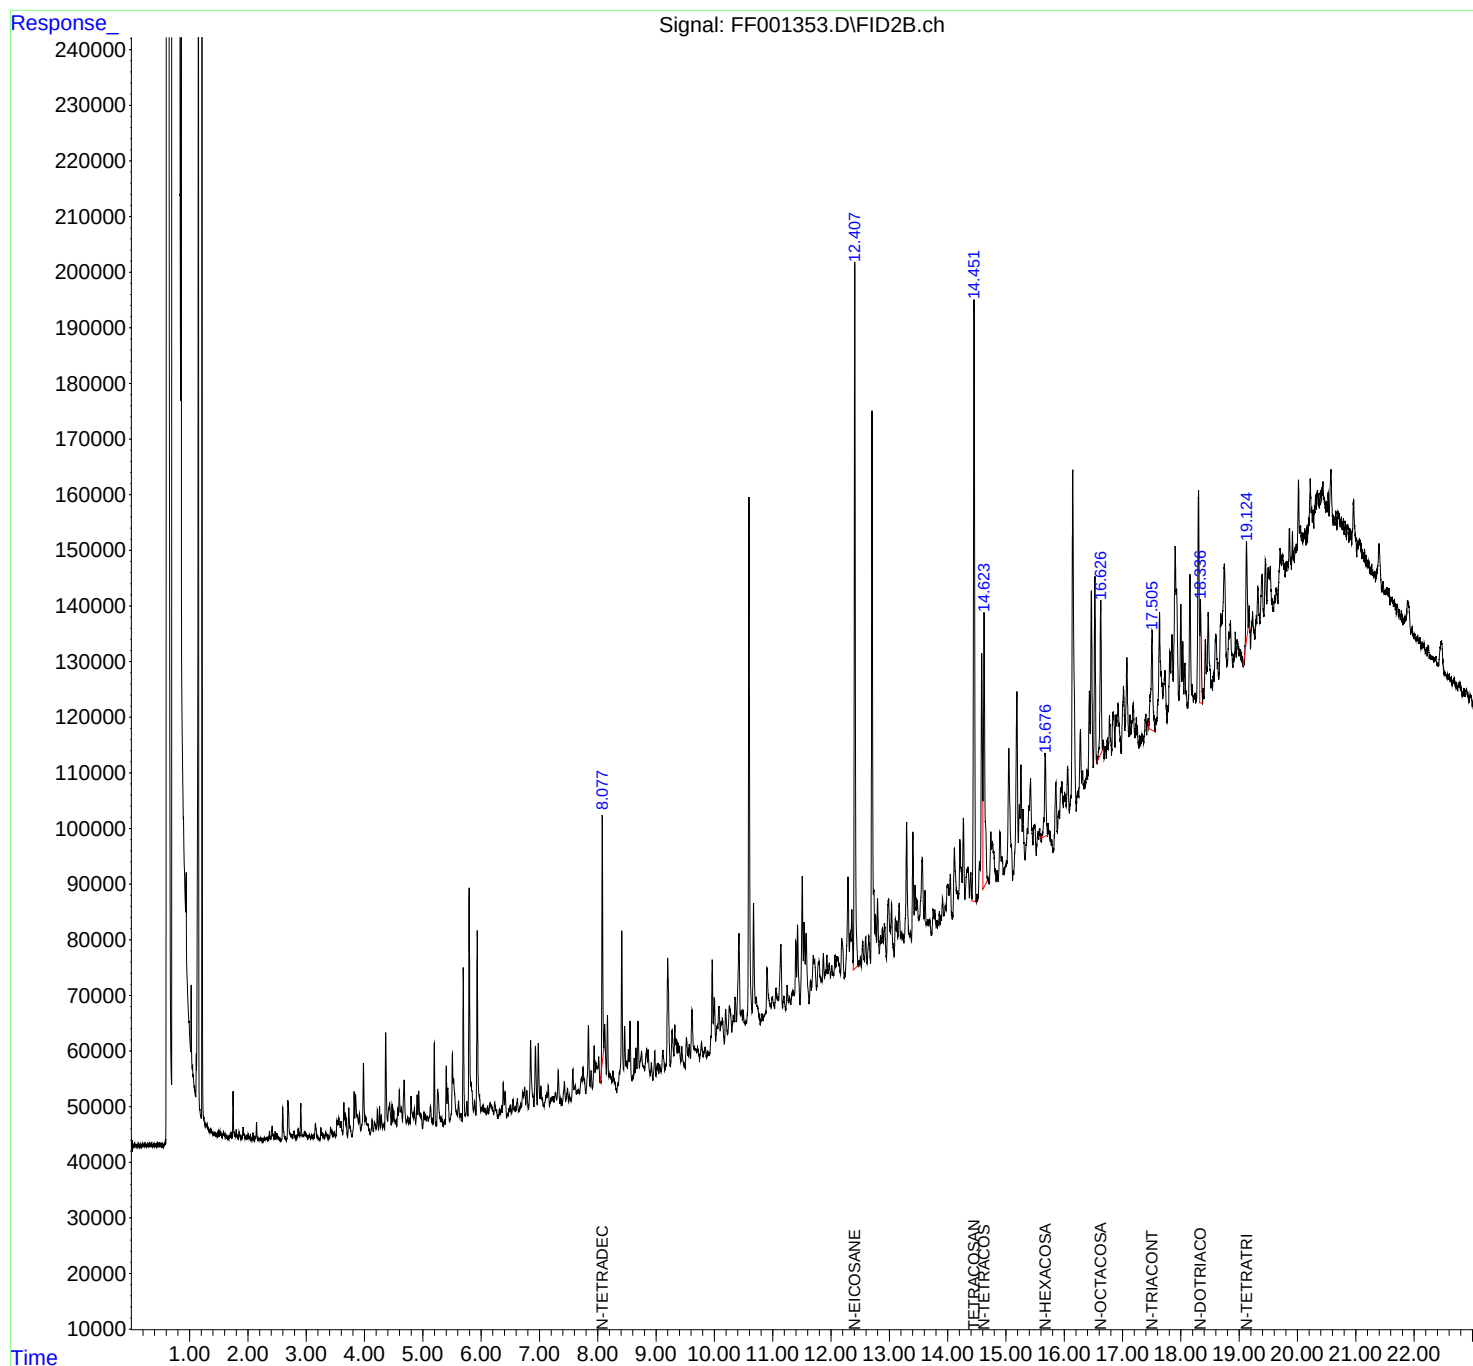


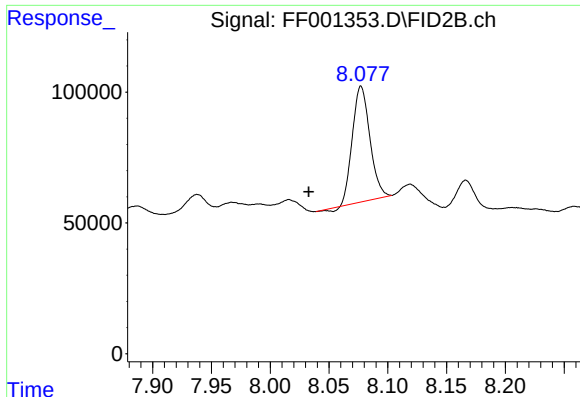

#4 N-TETRADECANE


R.T.: 8.077 min  
Delta R.T.: 0.044 min  
Response: 455248  
Conc: 3.62 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

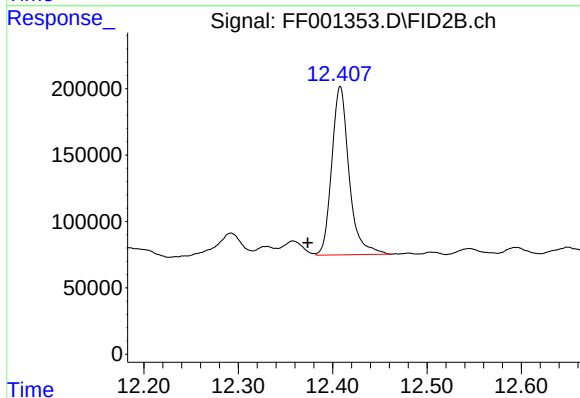


#7 N-EICOSANE

R.T.: 12.408 min  
Delta R.T.: 0.035 min  
Response: 1619937  
Conc: 13.02 ug/ml

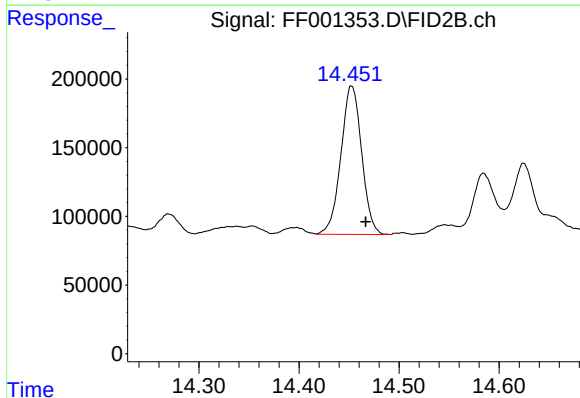


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.453 min  
Delta R.T.: -0.014 min  
Response: 1557515  
Conc: 14.46 ug/ml

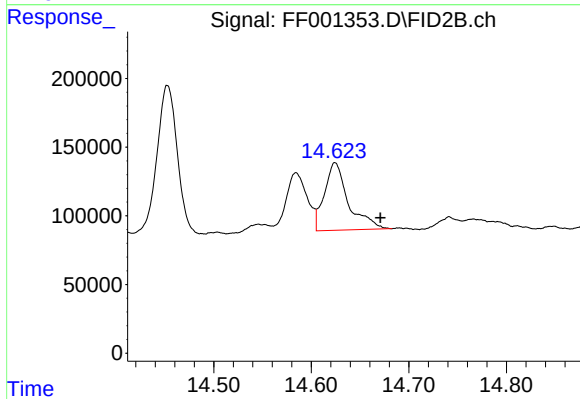

#10 N-TETRACOSANE


R.T.: 14.624 min  
Delta R.T.: -0.046 min  
Response: 841496  
Conc: 6.90 ug/ml

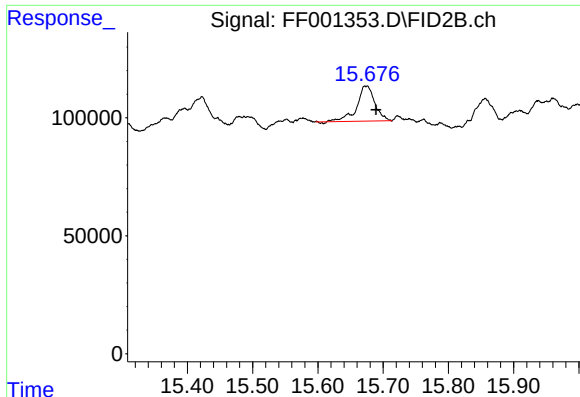

#11 N-HEXACOSANE


R.T.: 15.675 min  
Delta R.T.: -0.014 min  
Response: 284009  
Conc: 2.34 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

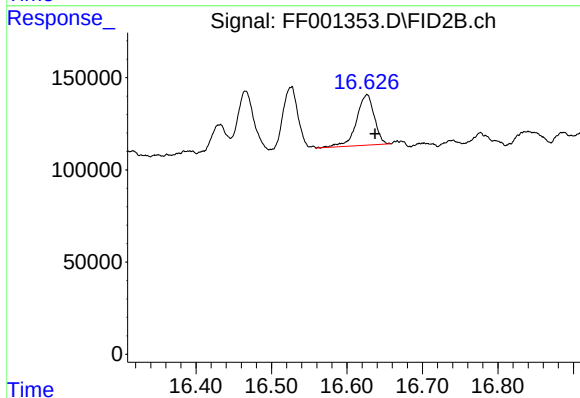


#12 N-OCTACOSANE

R.T.: 16.627 min  
Delta R.T.: -0.010 min  
Response: 447214  
Conc: 3.71 ug/ml

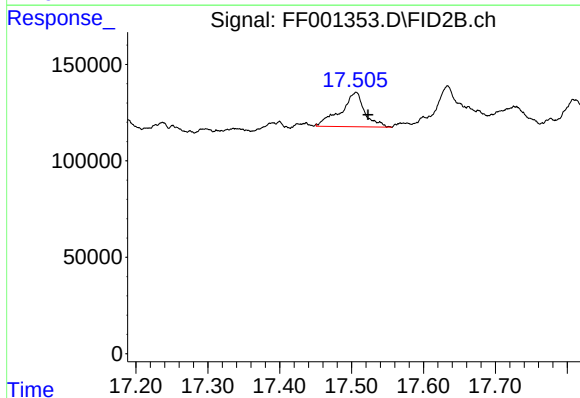


#13 N-TRIACONTANE

R.T.: 17.506 min  
Delta R.T.: -0.016 min  
Response: 410000  
Conc: 3.41 ug/ml

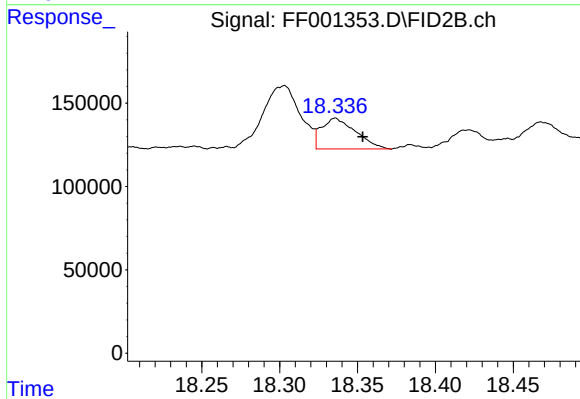

#14 N-DOTRIACONTANE

R.T.: 18.336 min  
Delta R.T.: -0.018 min  
Response: 282983  
Conc: 2.40 ug/ml

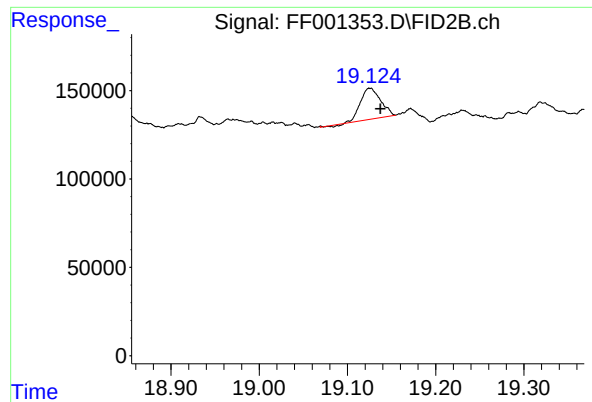

#15 N-TETRATRIACONTANE

R.T.: 19.126 min

Delta R.T.: -0.012 min

Response: 272144

Conc: 2.32 ug/ml

Instrument :  
FID\_F  
ClientSampleId :