

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
 Data File : FF001354.D
 Signal(s) : FID2B.ch
 Acq On : 14 Jul 2018 02:30
 Operator : AJ\SJ
 Sample : J3975-08
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 14 04:18:38 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.453	1553245	14.419 ug/ml
Target Compounds			
4) N-TETRADECANE	8.077	470654	3.742 ug/ml
7) N-EICOSANE	12.408	1641823	13.199 ug/ml
10) N-TETRACOSANE	14.625	845150	6.933 ug/ml
11) N-HEXACOSANE	15.675	318826	2.630 ug/ml
12) N-OCTACOSANE	16.626	493599	4.097 ug/ml
13) N-TRIACONTANE	17.505	413201	3.437 ug/ml
14) N-DOTRIACONTANE	18.338	345911	2.934 ug/ml
15) N-TETRATRIACONTANE	19.128	382637	3.256 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001354.D
Signal(s) : FID2B.ch
Acq On : 14 Jul 2018 02:30
Operator : AJ\SJ
Sample : J3975-08
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 14 04:18:38 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

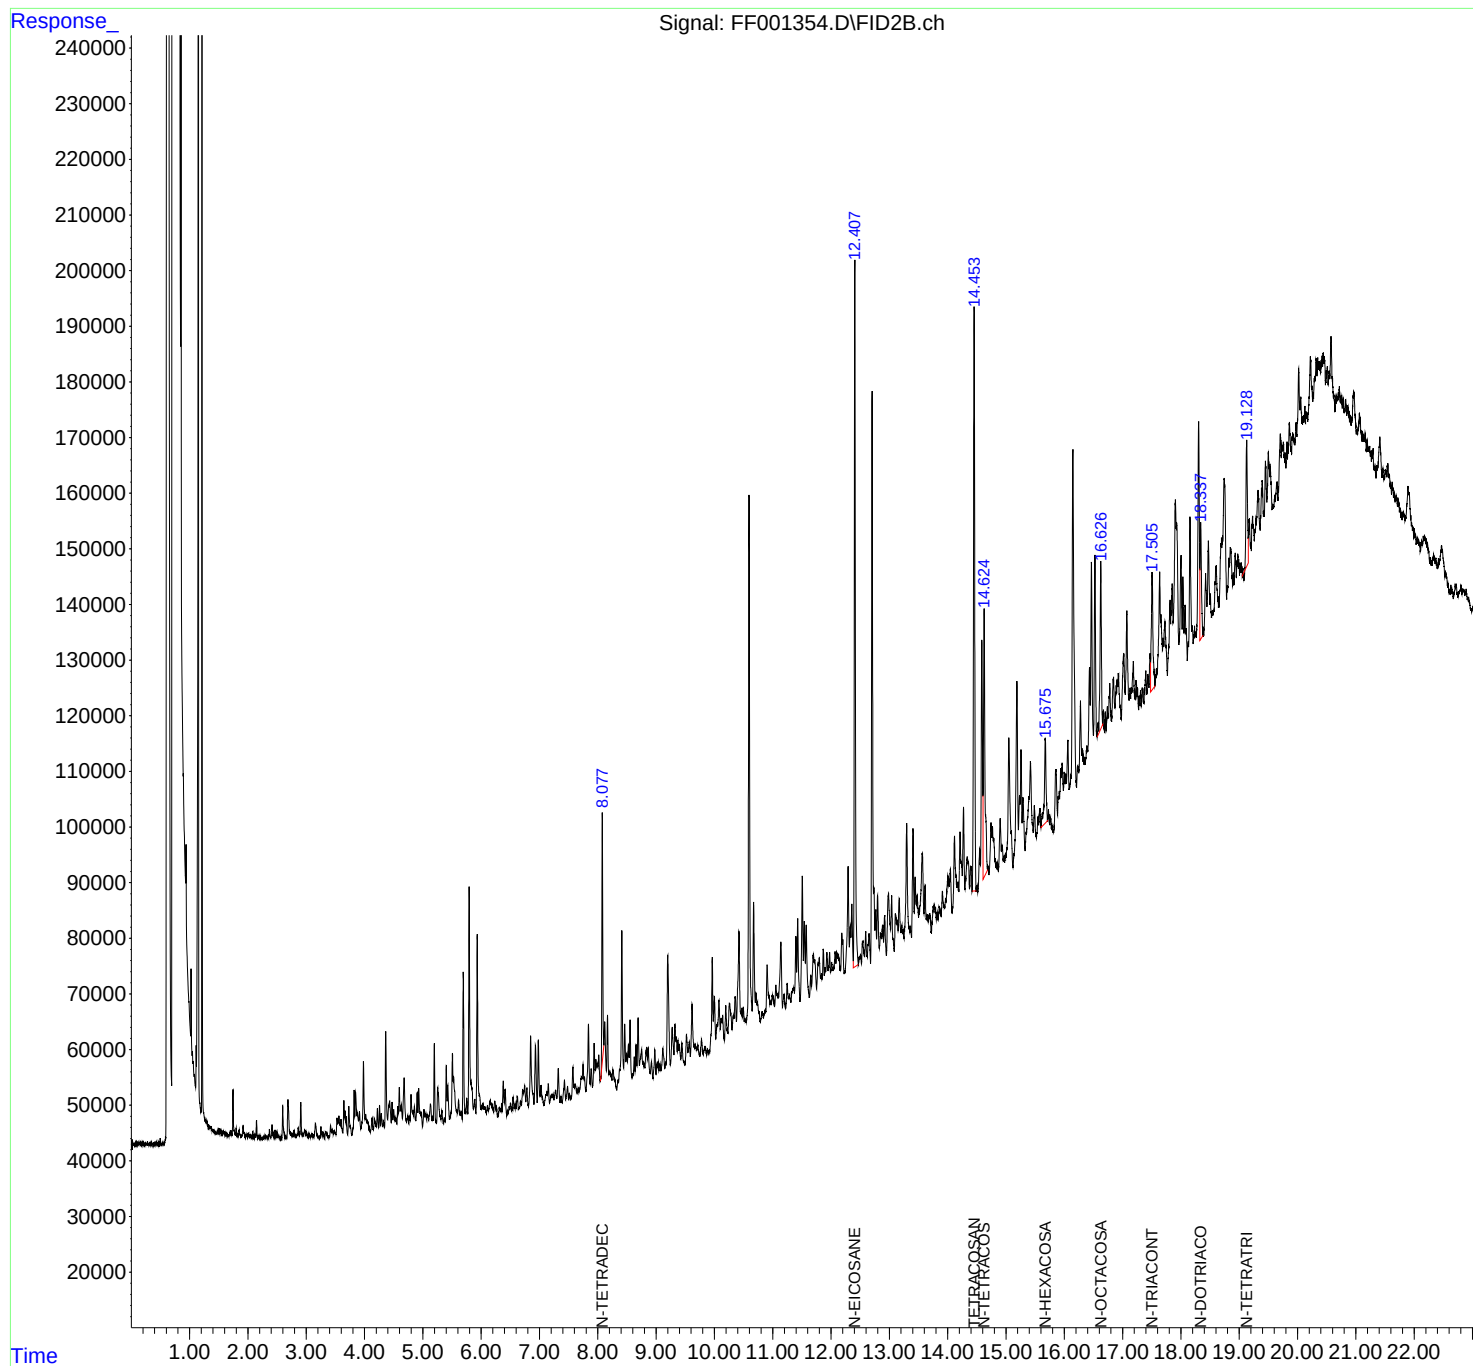


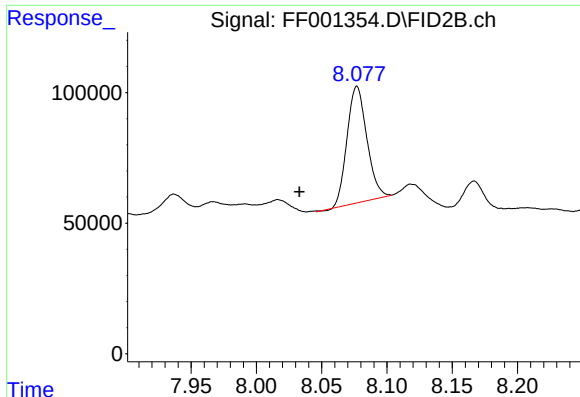

#4 N-TETRADECANE


R.T.: 8.077 min
Delta R.T.: 0.044 min
Response: 470654
Conc: 3.74 ug/ml

Instrument :
FID_F
ClientSampleId :

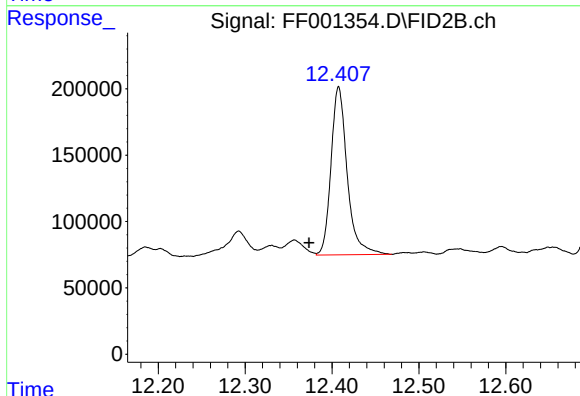


#7 N-EICOSANE

R.T.: 12.408 min
Delta R.T.: 0.034 min
Response: 1641823
Conc: 13.20 ug/ml

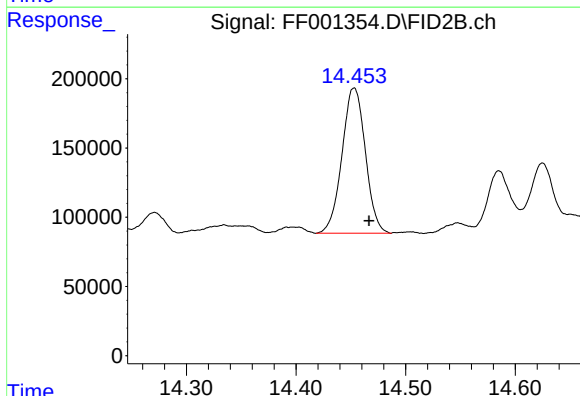


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.453 min
Delta R.T.: -0.014 min
Response: 1553245
Conc: 14.42 ug/ml

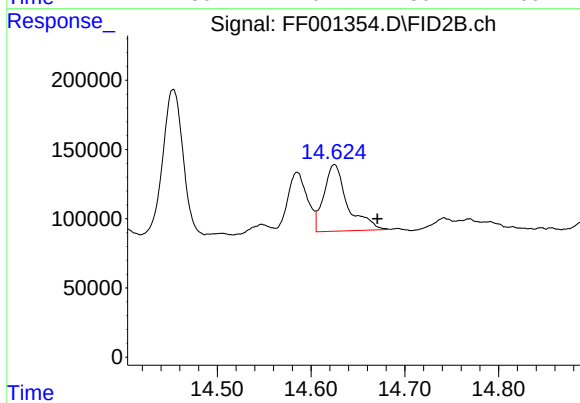

#10 N-TETRACOSANE


R.T.: 14.625 min
Delta R.T.: -0.046 min
Response: 845150
Conc: 6.93 ug/ml

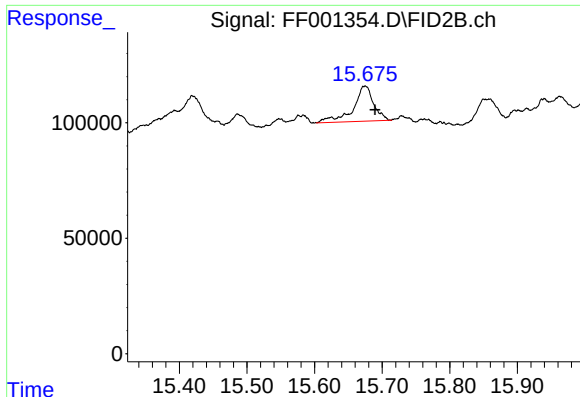

#11 N-HEXACOSANE


R.T.: 15.675 min
Delta R.T.: -0.015 min
Response: 318826
Conc: 2.63 ug/ml

Instrument :
FID_F
ClientSampleId :

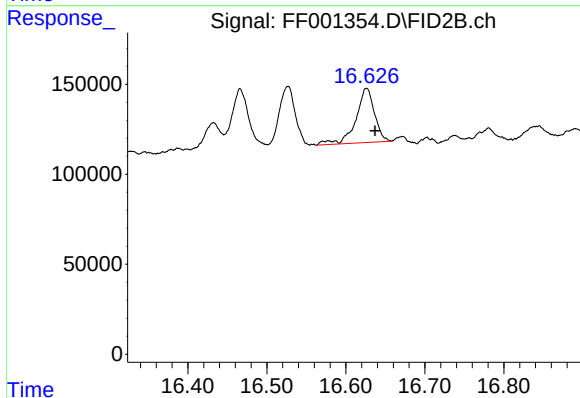


#12 N-OCTACOSANE

R.T.: 16.626 min
Delta R.T.: -0.011 min
Response: 493599
Conc: 4.10 ug/ml

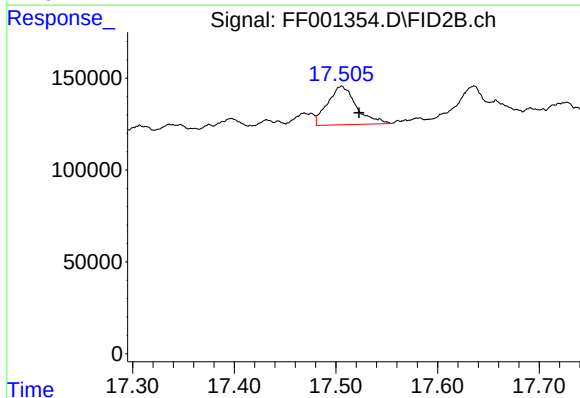


#13 N-TRIACONTANE

R.T.: 17.505 min
Delta R.T.: -0.017 min
Response: 413201
Conc: 3.44 ug/ml

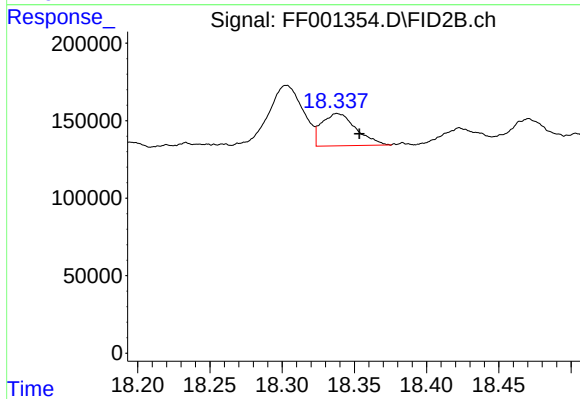

#14 N-DOTRIACONTANE

R.T.: 18.338 min
Delta R.T.: -0.015 min
Response: 345911
Conc: 2.93 ug/ml

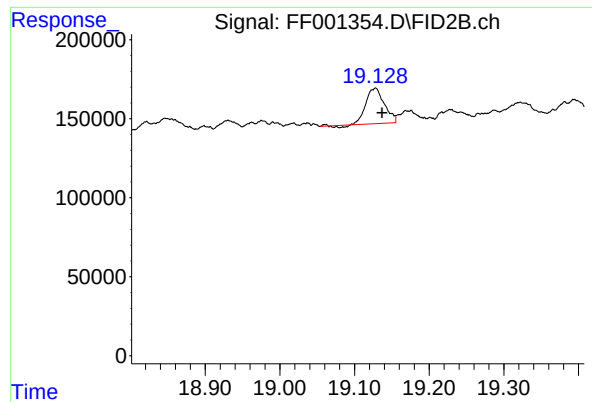

#15 N-TETRATRIACONTANE

R.T.: 19.128 min
Delta R.T.: -0.009 min
Response: 382637
Conc: 3.26 ug/ml

Instrument :
FID_F
ClientSampleId :