

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001355.D
Signal(s) : FID2B.ch
Acq On : 14 Jul 2018 03:00
Operator : AJ\SJ
Sample : J3821-01 10X
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 14 04:18:53 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.232	217072	1.732 ug/ml
4)	N-TETRADECANE	8.020	204586	1.627 ug/ml
7)	N-EICOSANE	12.407	1138569	9.153 ug/ml
10)	N-TETRACOSANE	14.624	760910	6.242 ug/ml
12)	N-OCTACOSANE	16.626	240086	1.993 ug/ml
13)	N-TRIACONTANE	17.507	341895	2.844 ug/ml
14)	N-DOTRIACONTANE	18.339	206494	1.751 ug/ml
15)	N-TETRATRIACONTANE	19.129	351436	2.990 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071318\
Data File : FF001355.D
Signal(s) : FID2B.ch
Acq On : 14 Jul 2018 03:00
Operator : AJ\SJ
Sample : J3821-01 10X
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 14 04:18:53 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

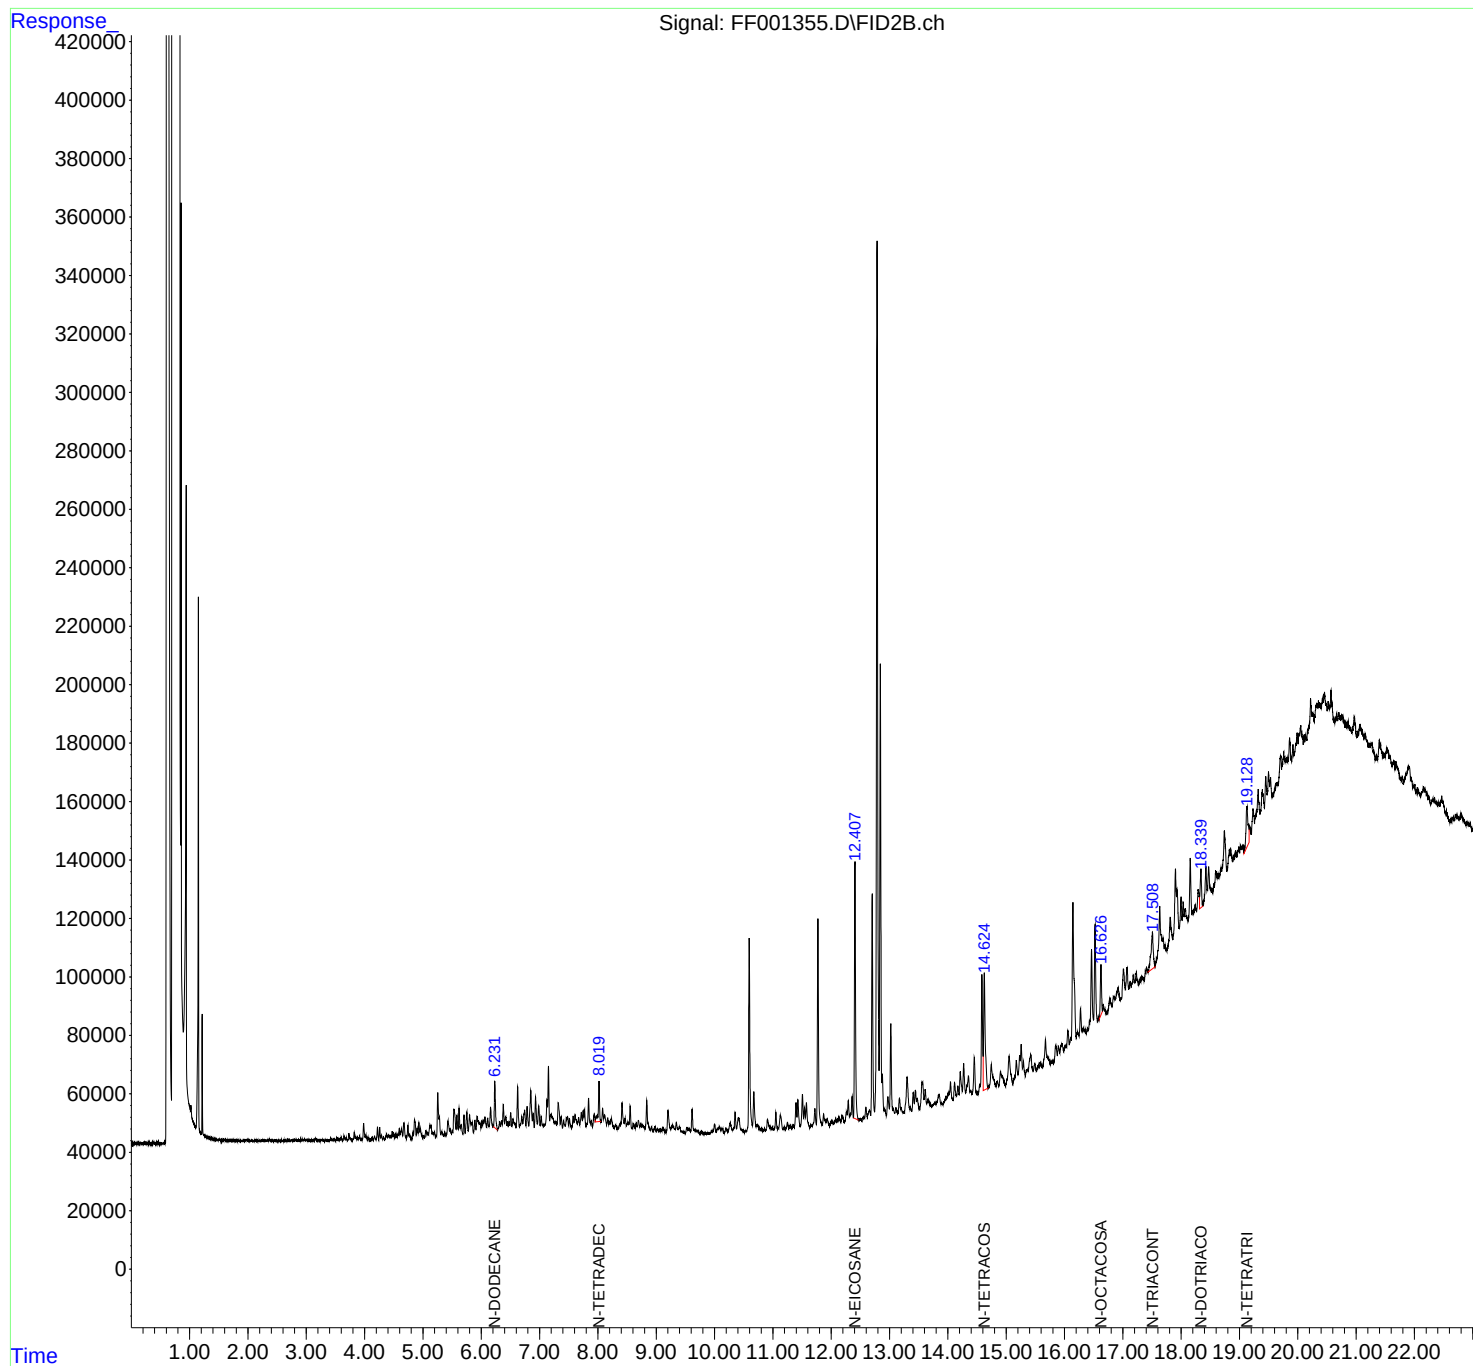


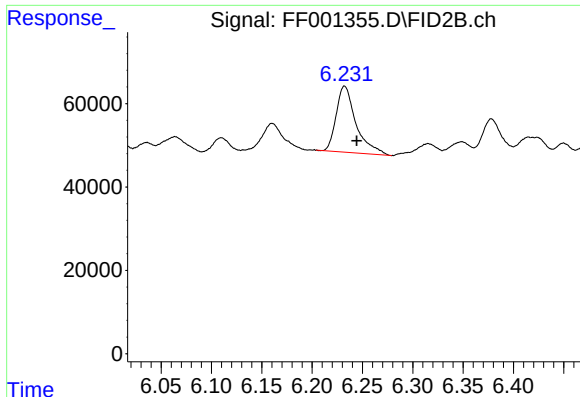

#3 N-DODECANE


R.T.: 6.232 min
Delta R.T.: -0.012 min
Response: 217072
Conc: 1.73 ug/ml

Instrument :
FID_F
ClientSampleId :

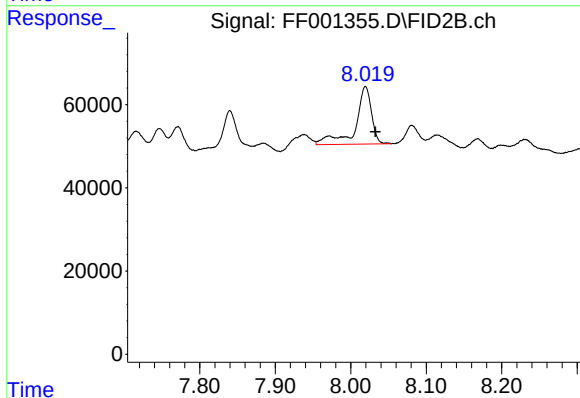


#4 N-TETRADECANE

R.T.: 8.020 min
Delta R.T.: -0.013 min
Response: 204586
Conc: 1.63 ug/ml

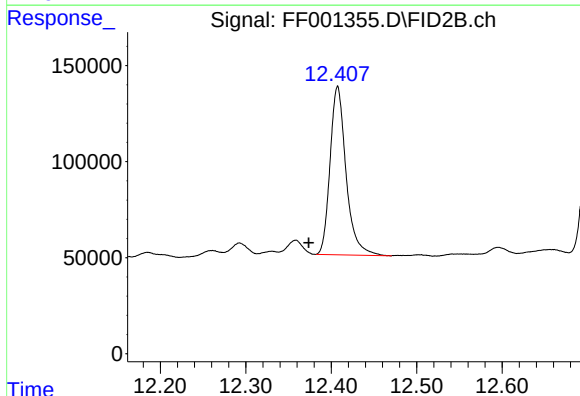


#7 N-EICOSANE

R.T.: 12.407 min
Delta R.T.: 0.034 min
Response: 1138569
Conc: 9.15 ug/ml

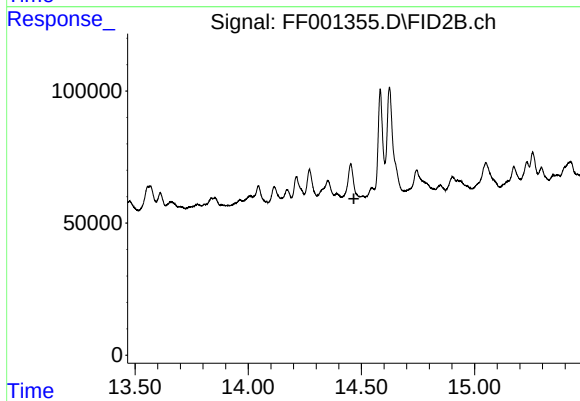

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.467 min
Response: 0
Conc: N.D.

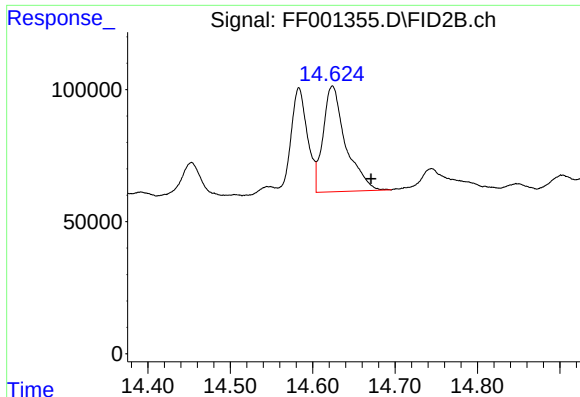

#10 N-TETRACOSANE


R.T.: 14.624 min
Delta R.T.: -0.047 min
Response: 760910
Conc: 6.24 ug/ml

Instrument :
FID_F
ClientSampleId :

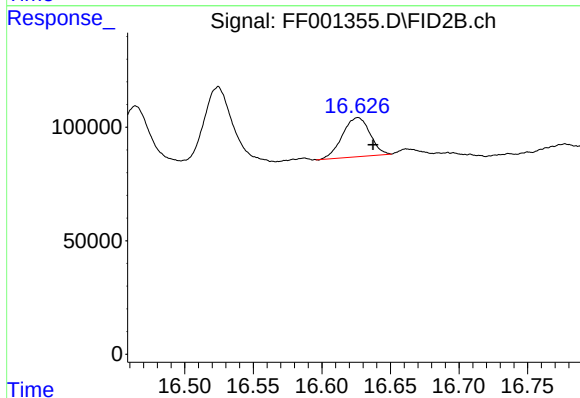


#12 N-OCTACOSANE

R.T.: 16.626 min
Delta R.T.: -0.011 min
Response: 240086
Conc: 1.99 ug/ml

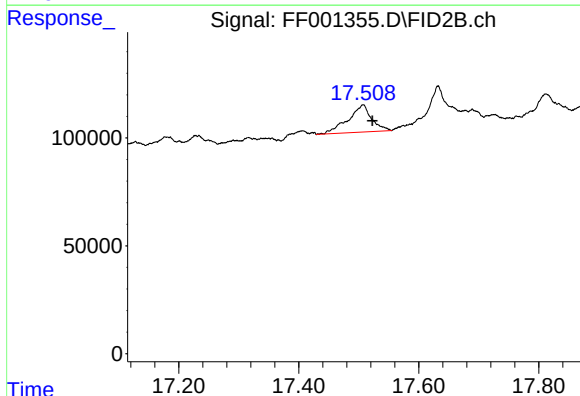


#13 N-TRIACONTANE

R.T.: 17.507 min
Delta R.T.: -0.015 min
Response: 341895
Conc: 2.84 ug/ml

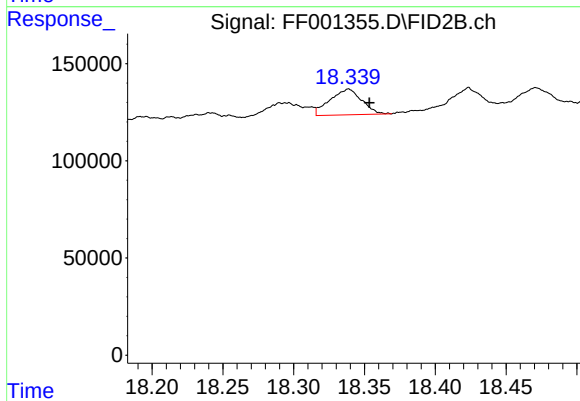

#14 N-DOTRIACONTANE

R.T.: 18.339 min
Delta R.T.: -0.015 min
Response: 206494
Conc: 1.75 ug/ml

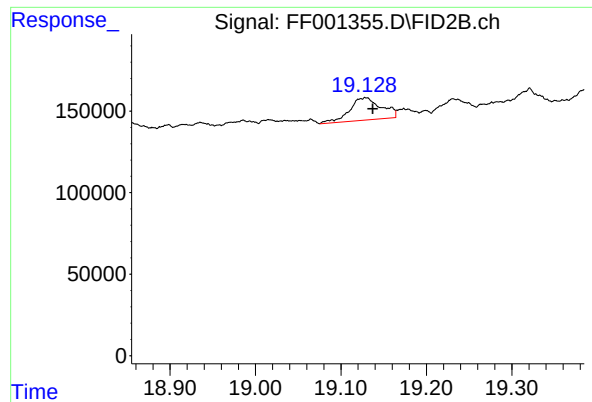

#15 N-TETRATRIACONTANE

R.T.: 19.129 min
Delta R.T.: -0.008 min
Response: 351436
Conc: 2.99 ug/ml

Instrument :
FID_F
ClientSampleId :