

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071423AL\
Data File : FF013073.D
Signal(s) : FID2B.ch
Acq On : 14 Jul 2023 21:38
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 15 01:54:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:52:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.042f	35331	0.229 ug/ml
18) T	n-Dotriacontane (C32)	17.862	76535	0.505 ug/ml
19) T	n-Tetratriacontane (C34)	18.653f	59462	0.427 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071423AL\
Data File : FF013073.D
Signal(s) : FID2B.ch
Acq On : 14 Jul 2023 21:38
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 15 01:54:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:52:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

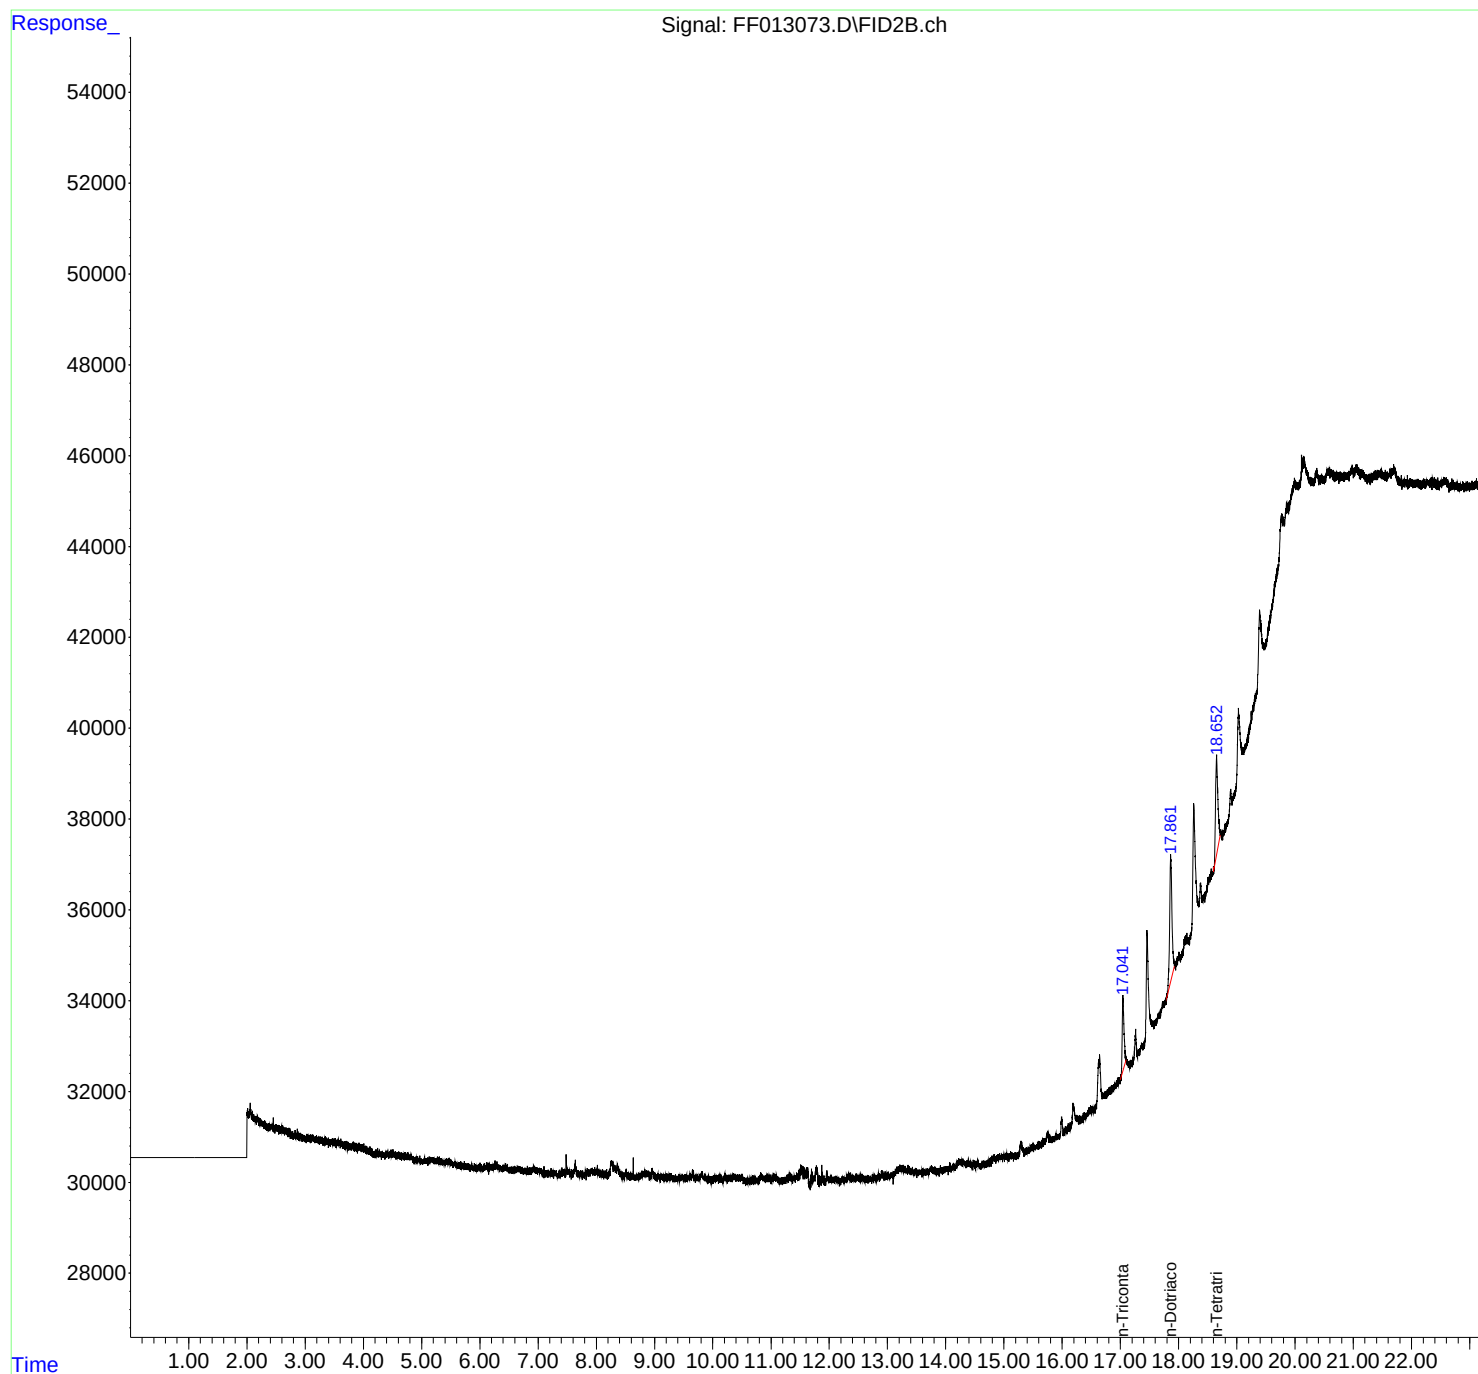


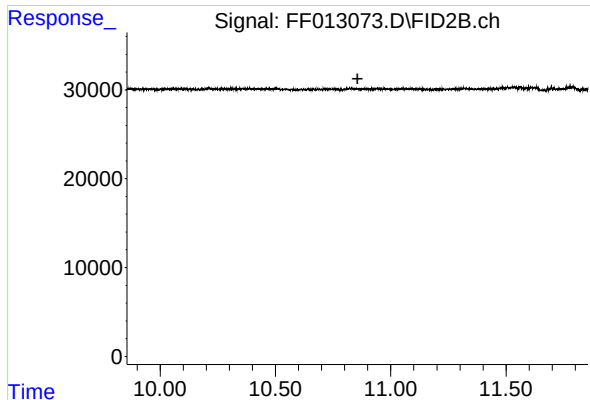

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 10.856 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

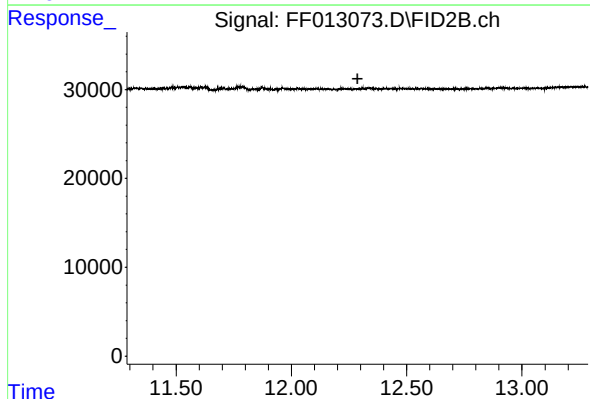


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.287 min
Response: 0
Conc: N.D.

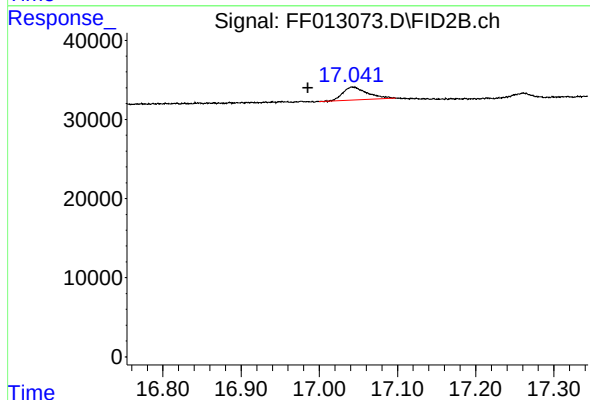


#17 n-Tricontane (C30)

R.T.: 17.042 min
Delta R.T.: 0.057 min
Response: 35331
Conc: 0.23 ug/ml

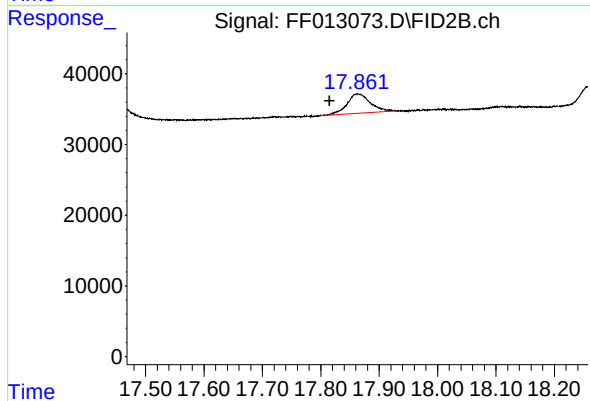

#18 n-Dotriacontane (C32)

R.T.: 17.862 min
Delta R.T.: 0.047 min
Response: 76535
Conc: 0.51 ug/ml

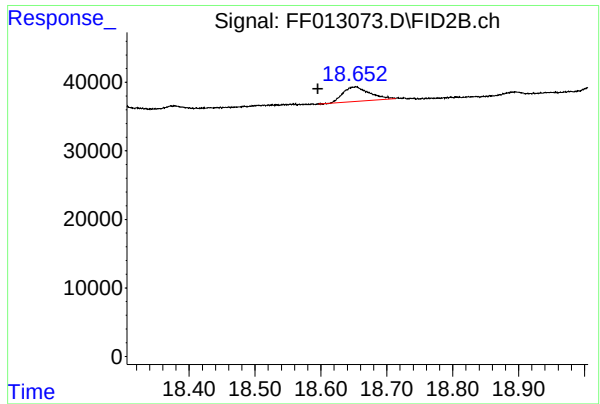

#19 n-Tetratriacontane (C34)

R.T.: 18.653 min

Delta R.T.: 0.057 min

Response: 59462

Conc: 0.43 ug/ml

Instrument :

FID_F

ClientSampleId :