

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF071425\  
 Data File : FF016147.D  
 Signal(s) : FID2B.ch  
 Acq On : 14 Jul 2025 11:50  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jul 14 14:16:46 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF071025.M  
 Quant Title :  
 QLast Update : Thu Jul 10 12:51:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.095	1789202	18.374 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.599f	70257	0.842 ug/ml
-----			


(f)=RT Delta > 1/2 Window (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF071425\  
Data File : FF016147.D  
Signal(s) : FID2B.ch  
Acq On : 14 Jul 2025 11:50  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 14 14:16:46 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF071025.M  
Quant Title :  
QLast Update : Thu Jul 10 12:51:11 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

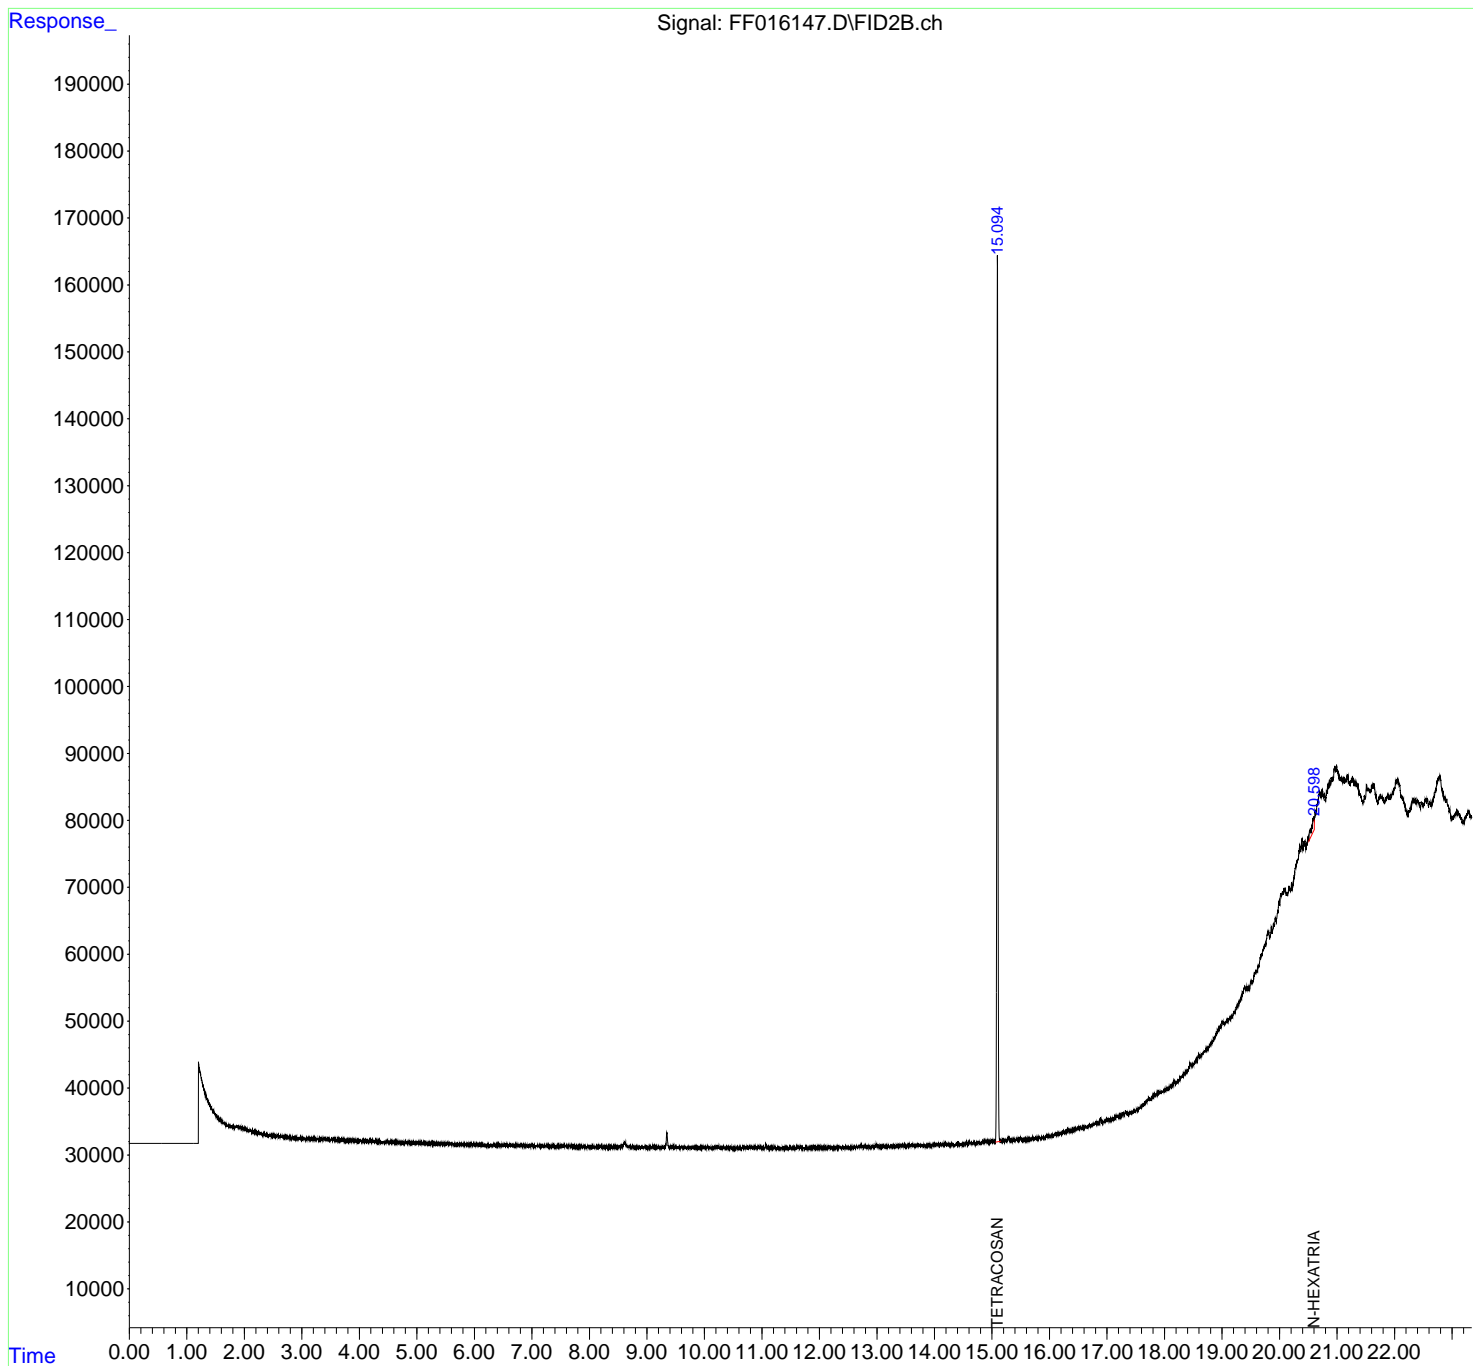


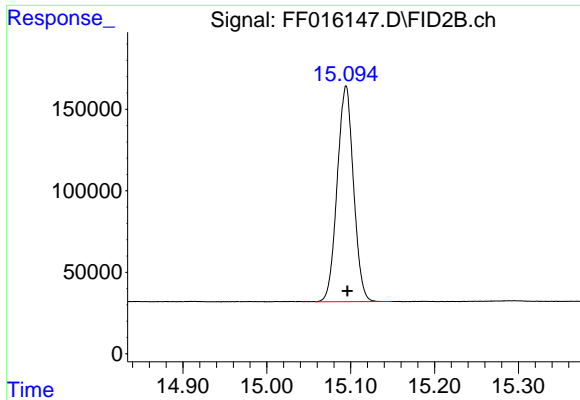

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.095 min  
Delta R.T.: -0.002 min  
Response: 1789202  
Conc: 18.37 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

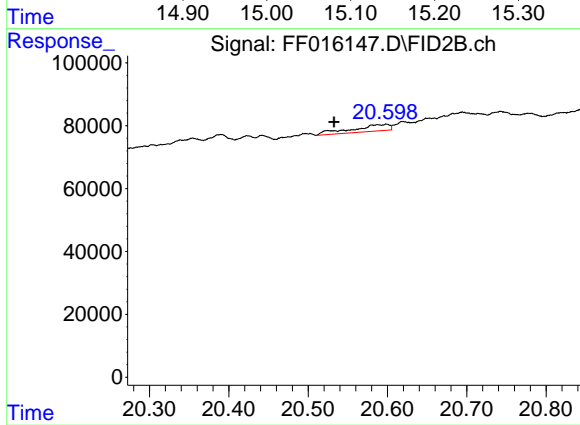

#16 N-HEXATRIACONTANE

R.T.: 20.599 min  
Delta R.T.: 0.066 min  
Response: 70257  
Conc: 0.84 ug/ml