

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071519\
 Data File : FF005045.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jul 2019 12:22
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 16 00:35:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.632f	347598	3.574 ug/ml
Target Compounds				
3)	N-DODECANE	6.413	3061753	24.131 ug/ml
11)	N-HEXACOSANE	15.905	95731	0.866 ug/ml
12)	N-OCTACOSANE	16.862	3169455	28.416 ug/ml
13)	N-TRIACONTANE	17.753	349260	3.109 ug/ml
14)	N-DOTRIACONTANE	18.592	370949	3.257 ug/ml
15)	N-TETRATRIACONTANE	19.383	229101	2.111 ug/ml
16)	N-HEXATRIACONTANE	20.132	130753	1.263 ug/ml
17)	N-OCTATRIACONTANE	20.884	90950	0.954 ug/ml
18)	N-TETRACONTANE	21.832	349434	3.006 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071519\
Data File : FF005045.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2019 12:22
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 16 00:35:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

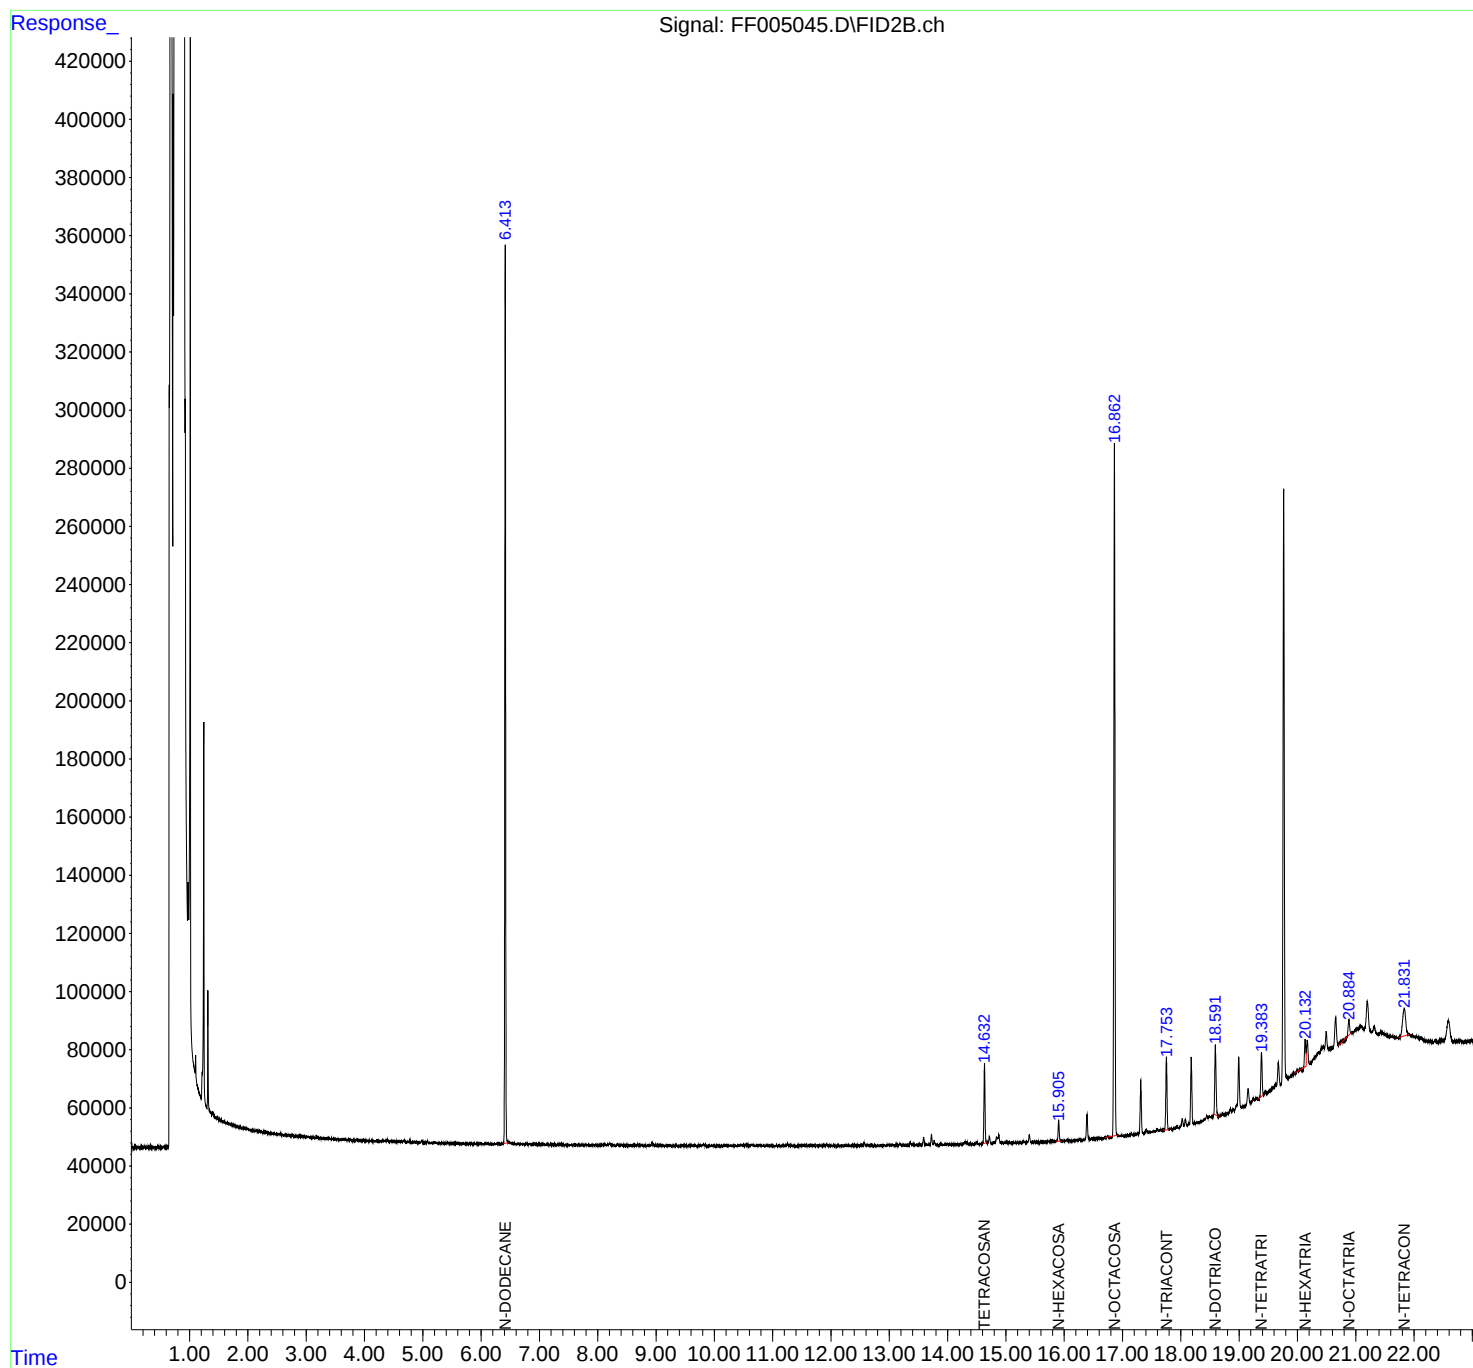

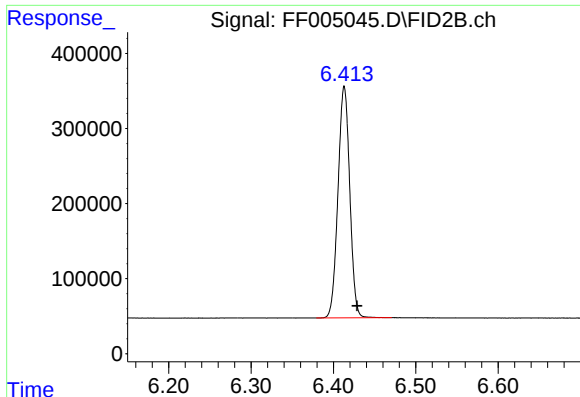


#3 N-DODECANE

R.T.: 6.413 min
Delta R.T.: -0.016 min
Response: 3061753
Conc: 24.13 ug/ml

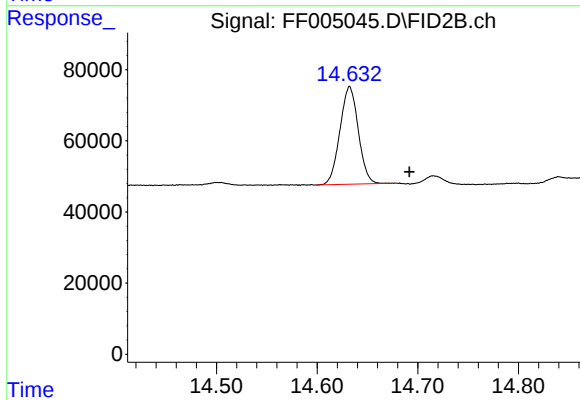


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.632 min
Delta R.T.: -0.059 min
Response: 347598
Conc: 3.57 ug/ml

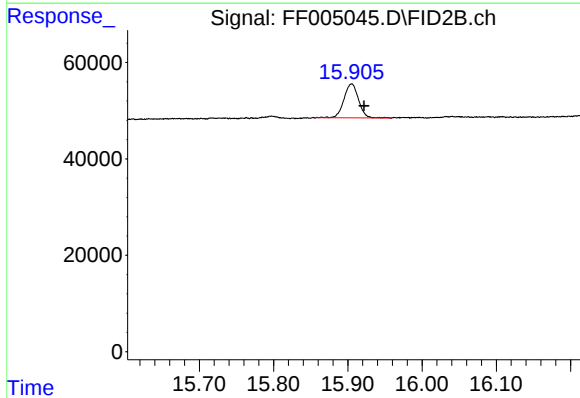


#11 N-HEXACOSANE

R.T.: 15.905 min
Delta R.T.: -0.017 min
Response: 95731
Conc: 0.87 ug/ml

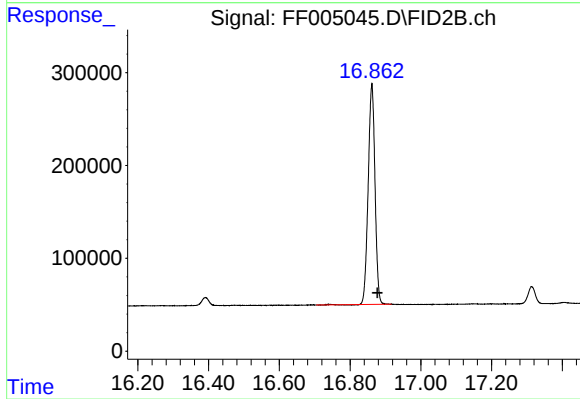


#12 N-OCTACOSANE

R.T.: 16.862 min
Delta R.T.: -0.016 min
Response: 3169455
Conc: 28.42 ug/ml

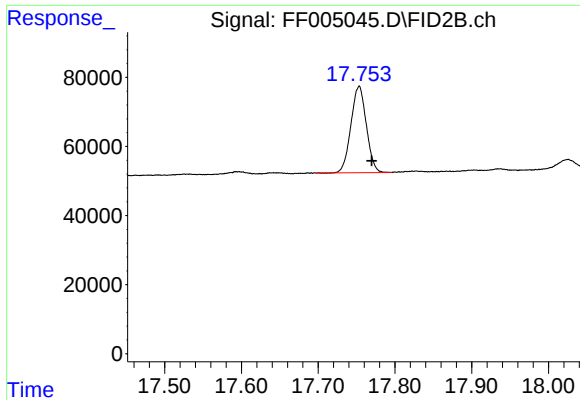


#13 N-TRIACONTANE

R.T.: 17.753 min
Delta R.T.: -0.017 min
Response: 349260
Conc: 3.11 ug/ml

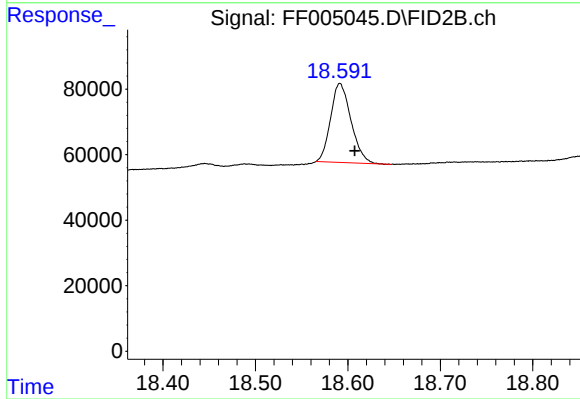


#14 N-DOTRIACONTANE

R.T.: 18.592 min
Delta R.T.: -0.016 min
Response: 370949
Conc: 3.26 ug/ml

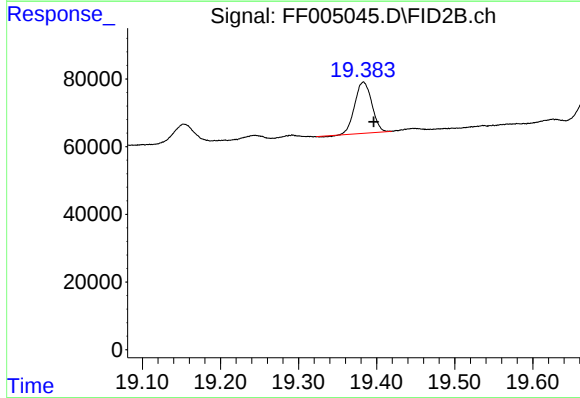


#15 N-TETRATRIACONTANE

R.T.: 19.383 min
Delta R.T.: -0.013 min
Response: 229101
Conc: 2.11 ug/ml

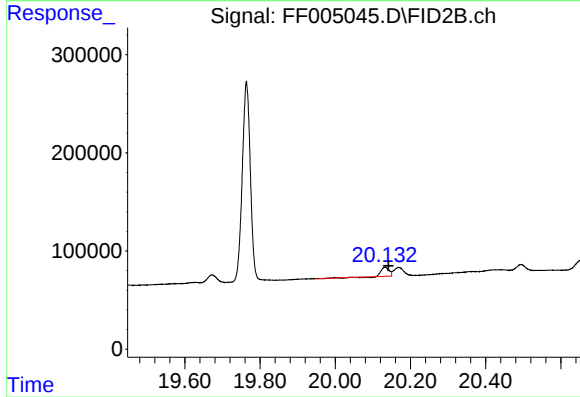


#16 N-HEXATRIACONTANE

R.T.: 20.132 min
Delta R.T.: -0.009 min
Response: 130753
Conc: 1.26 ug/ml

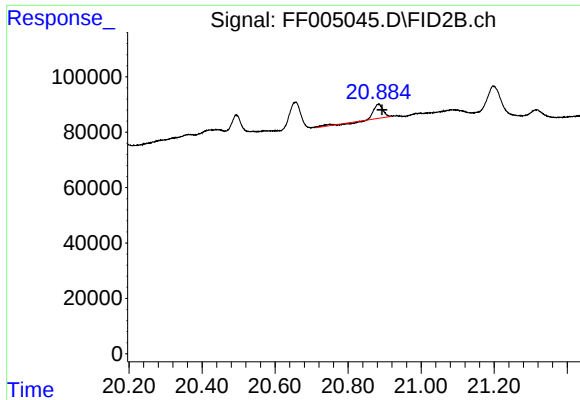

#17 N-OCTATRIACONTANE

R.T.: 20.884 min
Delta R.T.: -0.009 min
Response: 90950
Conc: 0.95 ug/ml

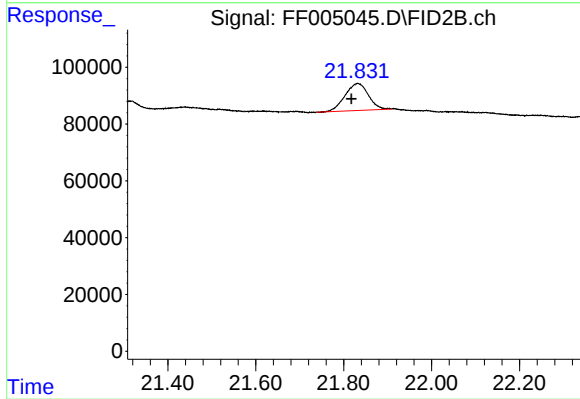

#18 N-TETRACONTANE

R.T.: 21.832 min
Delta R.T.: 0.015 min
Response: 349434
Conc: 3.01 ug/ml