

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
 Data File : FF008776.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jul 2021 08:50
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 16 01:43:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
8) N-DOCOSANE	13.842	75812	0.567 ug/ml
10) N-TETRACOSANE	14.936	564388	4.283 ug/ml
13) N-TRIACONTANE	17.800	102385	0.854 ug/ml
14) N-DOTRIACONTANE	18.633	291632	2.489 ug/ml
15) N-TETRATRIACONTANE	19.410	111299	1.065 ug/ml
16) N-HEXATRIACONTANE	20.179	322452	3.433 ug/ml
18) N-TETRACONTANE	21.845	323483	3.495 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008776.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2021 08:50
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jul 16 01:43:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

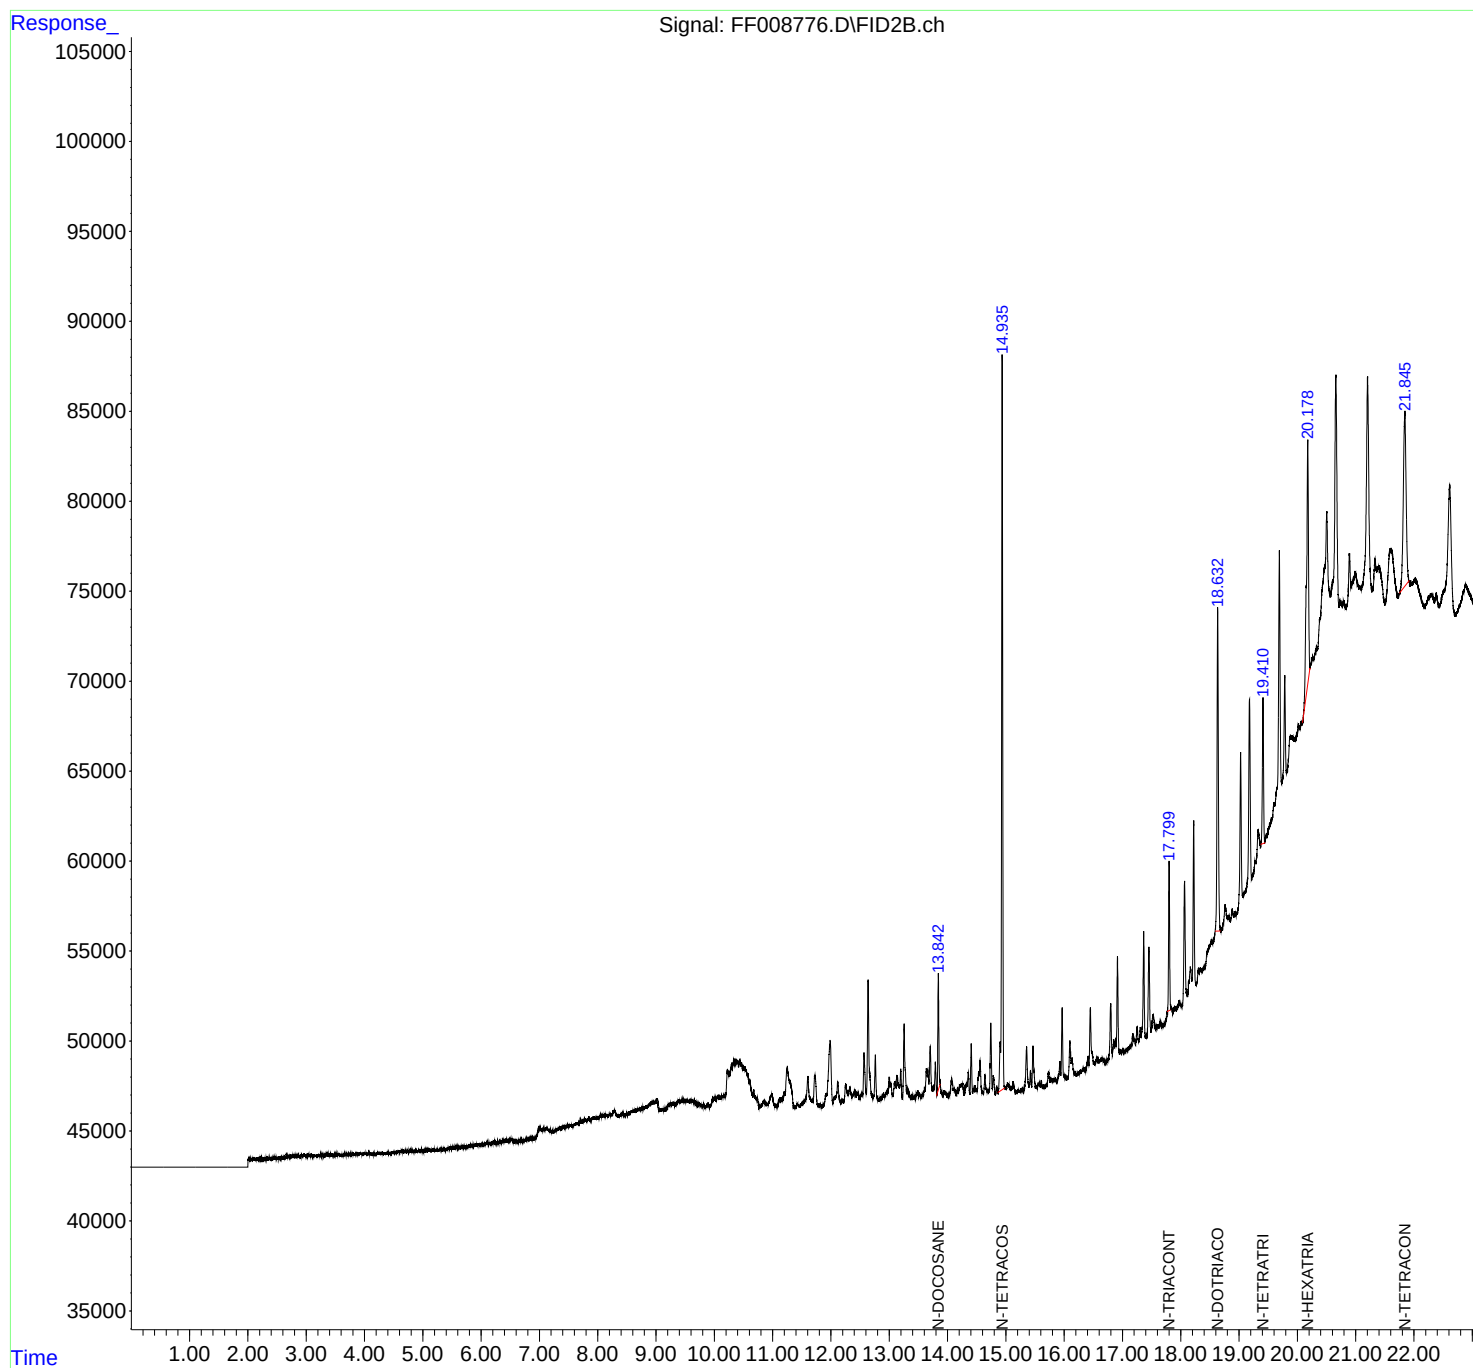


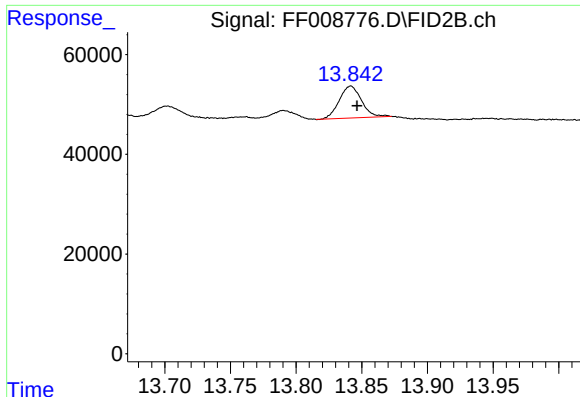

#8 N-DOCOSANE


R.T.: 13.842 min
Delta R.T.: -0.005 min
Response: 75812
Conc: 0.57 ug/ml

Instrument :
FID_F
ClientSampleId :

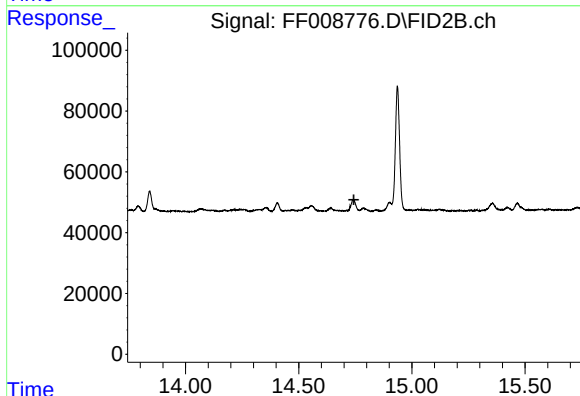


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.744 min
Response: 0
Conc: N.D.

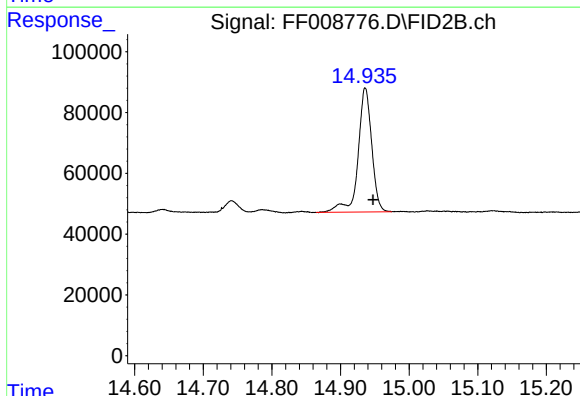


#10 N-TETRACOSANE

R.T.: 14.936 min
Delta R.T.: -0.012 min
Response: 564388
Conc: 4.28 ug/ml

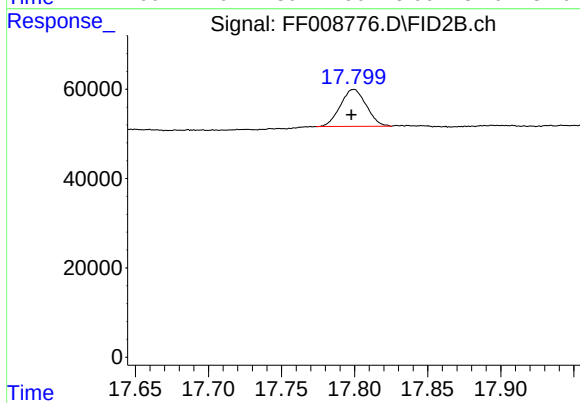

#13 N-TRIACONTANE


R.T.: 17.800 min
Delta R.T.: 0.002 min
Response: 102385
Conc: 0.85 ug/ml

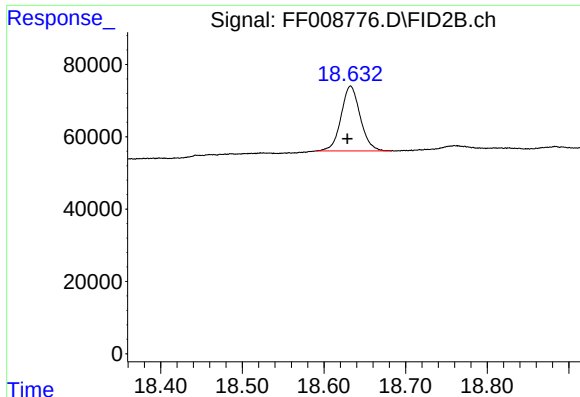

#14 N-DOTRIACONTANE


R.T.: 18.633 min
Delta R.T.: 0.004 min
Response: 291632
Conc: 2.49 ug/ml

Instrument :
FID_F
ClientSampleId :

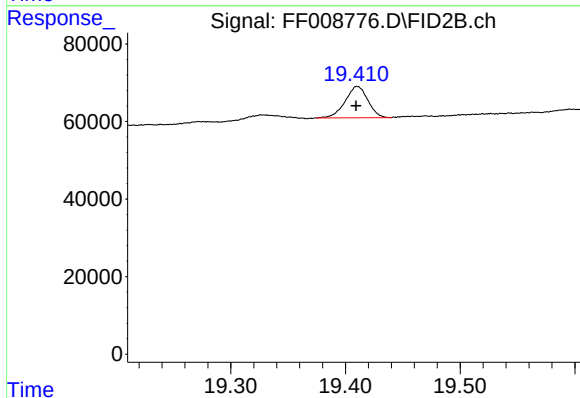


#15 N-TETRATRIACONTANE

R.T.: 19.410 min
Delta R.T.: 0.000 min
Response: 111299
Conc: 1.06 ug/ml

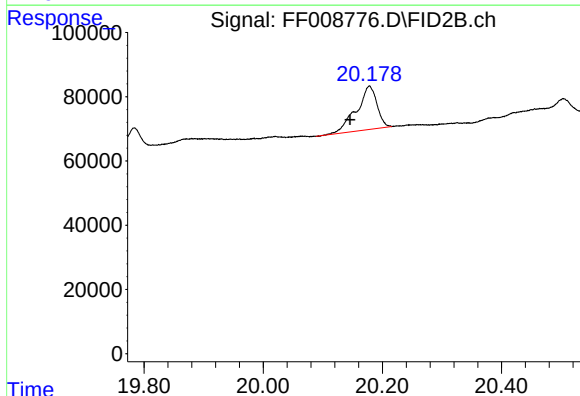

#16 N-HEXATRIACONTANE

R.T.: 20.179 min
Delta R.T.: 0.033 min
Response: 322452
Conc: 3.43 ug/ml

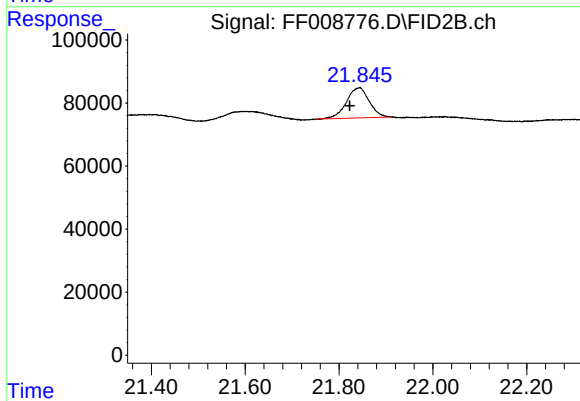

#18 N-TETRACONTANE

R.T.: 21.845 min
Delta R.T.: 0.022 min
Response: 323483
Conc: 3.50 ug/ml