

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008777.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2021 09:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 01:43:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	2491811	21.864 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.633	180956	1.545 ug/ml
18) N-TETRACONTANE	21.847	236542	2.556 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008777.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2021 09:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 01:43:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

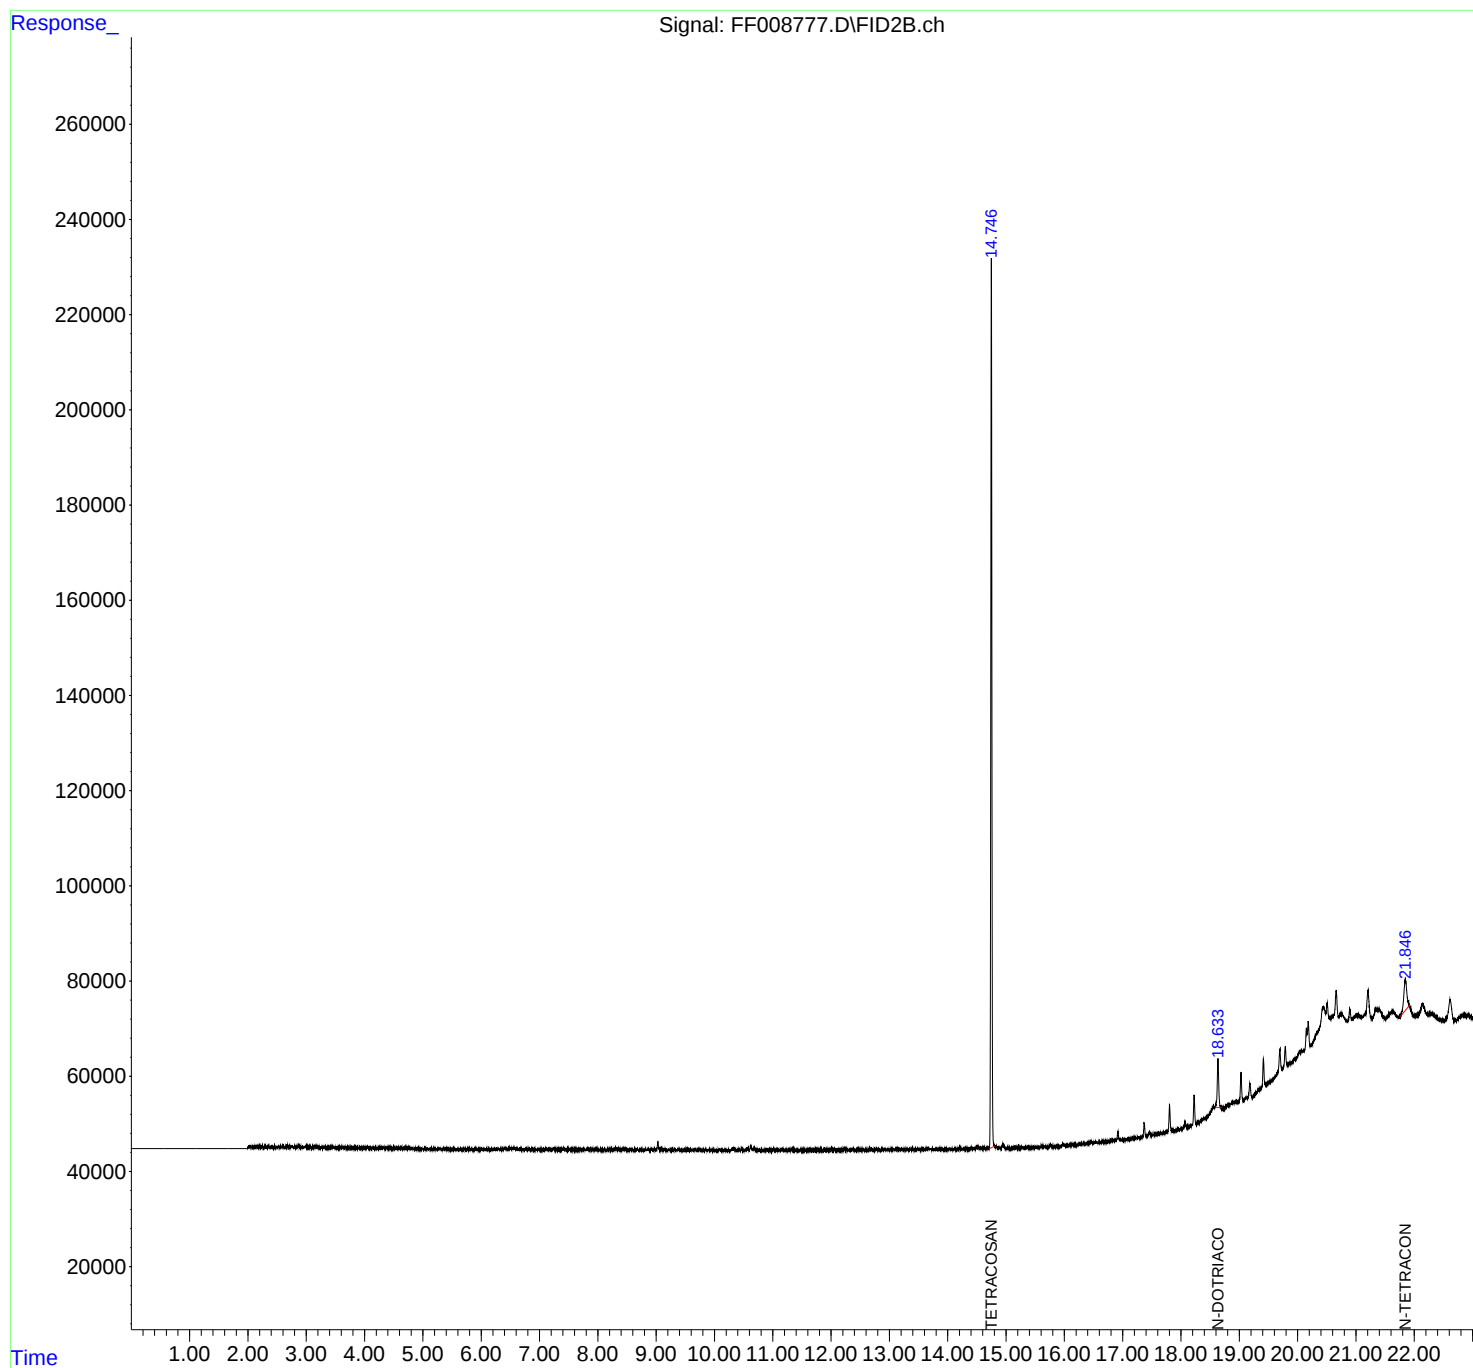


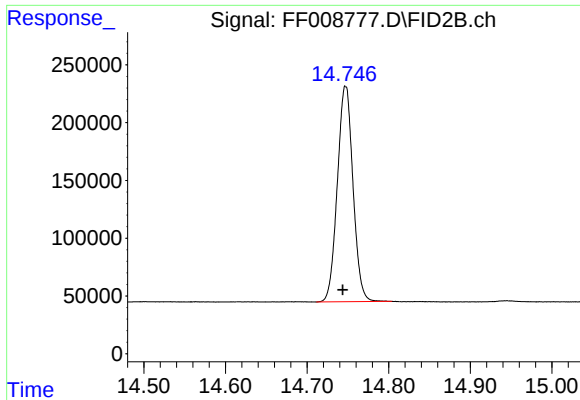

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.747 min
Delta R.T.: 0.003 min
Response: 2491811
Conc: 21.86 ug/ml

Instrument :
FID_F
ClientSampleId :

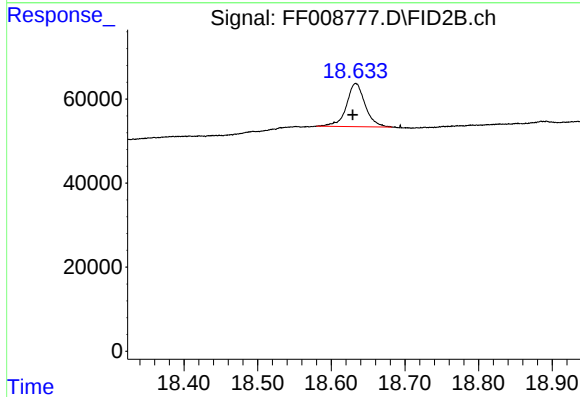

#14 N-DOTRIACONTANE

R.T.: 18.633 min
Delta R.T.: 0.004 min
Response: 180956
Conc: 1.54 ug/ml

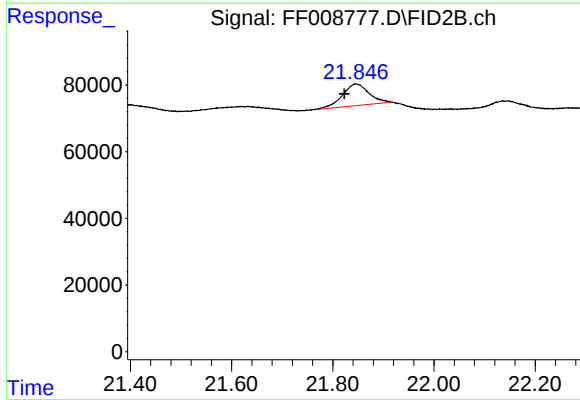

#18 N-TETRACONTANE

R.T.: 21.847 min
Delta R.T.: 0.024 min
Response: 236542
Conc: 2.56 ug/ml